

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101518\
 Data File : VU027653.D
 Acq On : 15 Oct 2018 09:41
 Operator : MD/SY
 Sample : VU1015WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Quant Time: Oct 16 07:47:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 16 07:44:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	191882	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	178799	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	71792	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	66817	44.25	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.50%
7) Chloroethane-d5	1.68	69	58697	50.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.92%
11) 1,1-Dichloroethene-d2	2.27	63	101463	35.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.64%
21) 2-Butanone-d5	4.18	46	138225	113.39	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.39%
24) Chloroform-d	4.65	84	130969	54.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.46%
26) 1,2-Dichloroethane-d4	5.31	65	92529	54.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.34%
32) Benzene-d6	5.34	84	266720	52.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.10%
36) 1,2-Dichloropropane-d6	6.33	67	95258	54.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.54%
41) Toluene-d8	7.57	98	215307	47.01	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.02%
43) trans-1,3-Dichloropropene-	7.85	79	40398	47.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.52%
47) 2-Hexanone-d5	8.31	63	90632	102.24	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.24%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	122048	53.17	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	106.34%
64) 1,2-Dichlorobenzene-d4	11.86	152	77126	54.91	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.82%

Target Compounds

					Qvalue
6) Bromomethane	1.62	94	583	0.624 ug/L	90
8) Chloroethane	1.70	64	546	0.426 ug/L #	66
9) Trichlorofluoromethane	1.89	101	1117	0.522 ug/L	95
10) 1,1,2-Trichloro-1,2,2-trif	2.28	101	1532	1.207 ug/L #	55
12) 1,1-Dichloroethene	2.28	96	1087	0.877 ug/L #	1
13) Acetone	2.32	43	1893	1.893 ug/L	93
14) Carbon disulfide	2.48	76	2588	0.568 ug/L	98
15) Methyl Acetate	2.62	43	2031	1.014 ug/L	94
16) Methylene chloride	2.70	84	867	0.576 ug/L	87
17) trans-1,2-Dichloroethene	2.98	96	668	0.487 ug/L	78
18) Methyl tert-butyl Ether	3.00	73	2206	0.483 ug/L #	85
25) Chloroform	4.67	83	5237	1.913 ug/L	96
27) 1,2-Dichloroethane	5.41	62	1467	0.667 ug/L #	75
33) Benzene	5.39	78	3100	0.528 ug/L	100
39) cis-1,3-Dichloropropene	7.23	75	2379	0.951 ug/L #	68
40) 4-Methyl-2-pentanone	7.47	43	2273	0.912 ug/L #	88
42) Toluene	7.64	91	3298	0.559 ug/L	98

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU101518\
Data File : VU027653.D
Acq On : 15 Oct 2018 09:41
Operator : MD/SY
Sample : VU1015WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Time: Oct 16 07:47:22 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 16 07:44:54 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
45) 1,1,2-Trichloroethane	8.08	97	668	0.489	ug/L #	90
46) Tetrachloroethene	8.23	164	526	0.501	ug/L	81
48) 2-Hexanone	8.37	43	3777	1.919	ug/L #	86
51) Chlorobenzene	9.12	112	1974	0.530	ug/L	88
52) Ethylbenzene	9.25	91	2879	0.440	ug/L	99
53) m,p-Xylene	9.38	106	944	0.394	ug/L	83
58) 1,1,2,2-Tetrachloroethane	10.45	83	1349	0.563	ug/L #	88
59) 1,2,3-Trichloropropane	11.48	75	10250	5.318	ug/L	94
62) 1,3-Dichlorobenzene	11.42	146	1104	0.494	ug/L	98
63) 1,4-Dichlorobenzene	11.51	146	1322	0.567	ug/L #	84
65) 1,2-Dichlorobenzene	11.88	146	1480	0.651	ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101518\
Data File : VU027653.D
Acq On : 15 Oct 2018 09:41
Operator : MD/SY
Sample : VU1015WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Time: Oct 16 07:47:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 16 07:44:54 2018
Response via : Initial Calibration

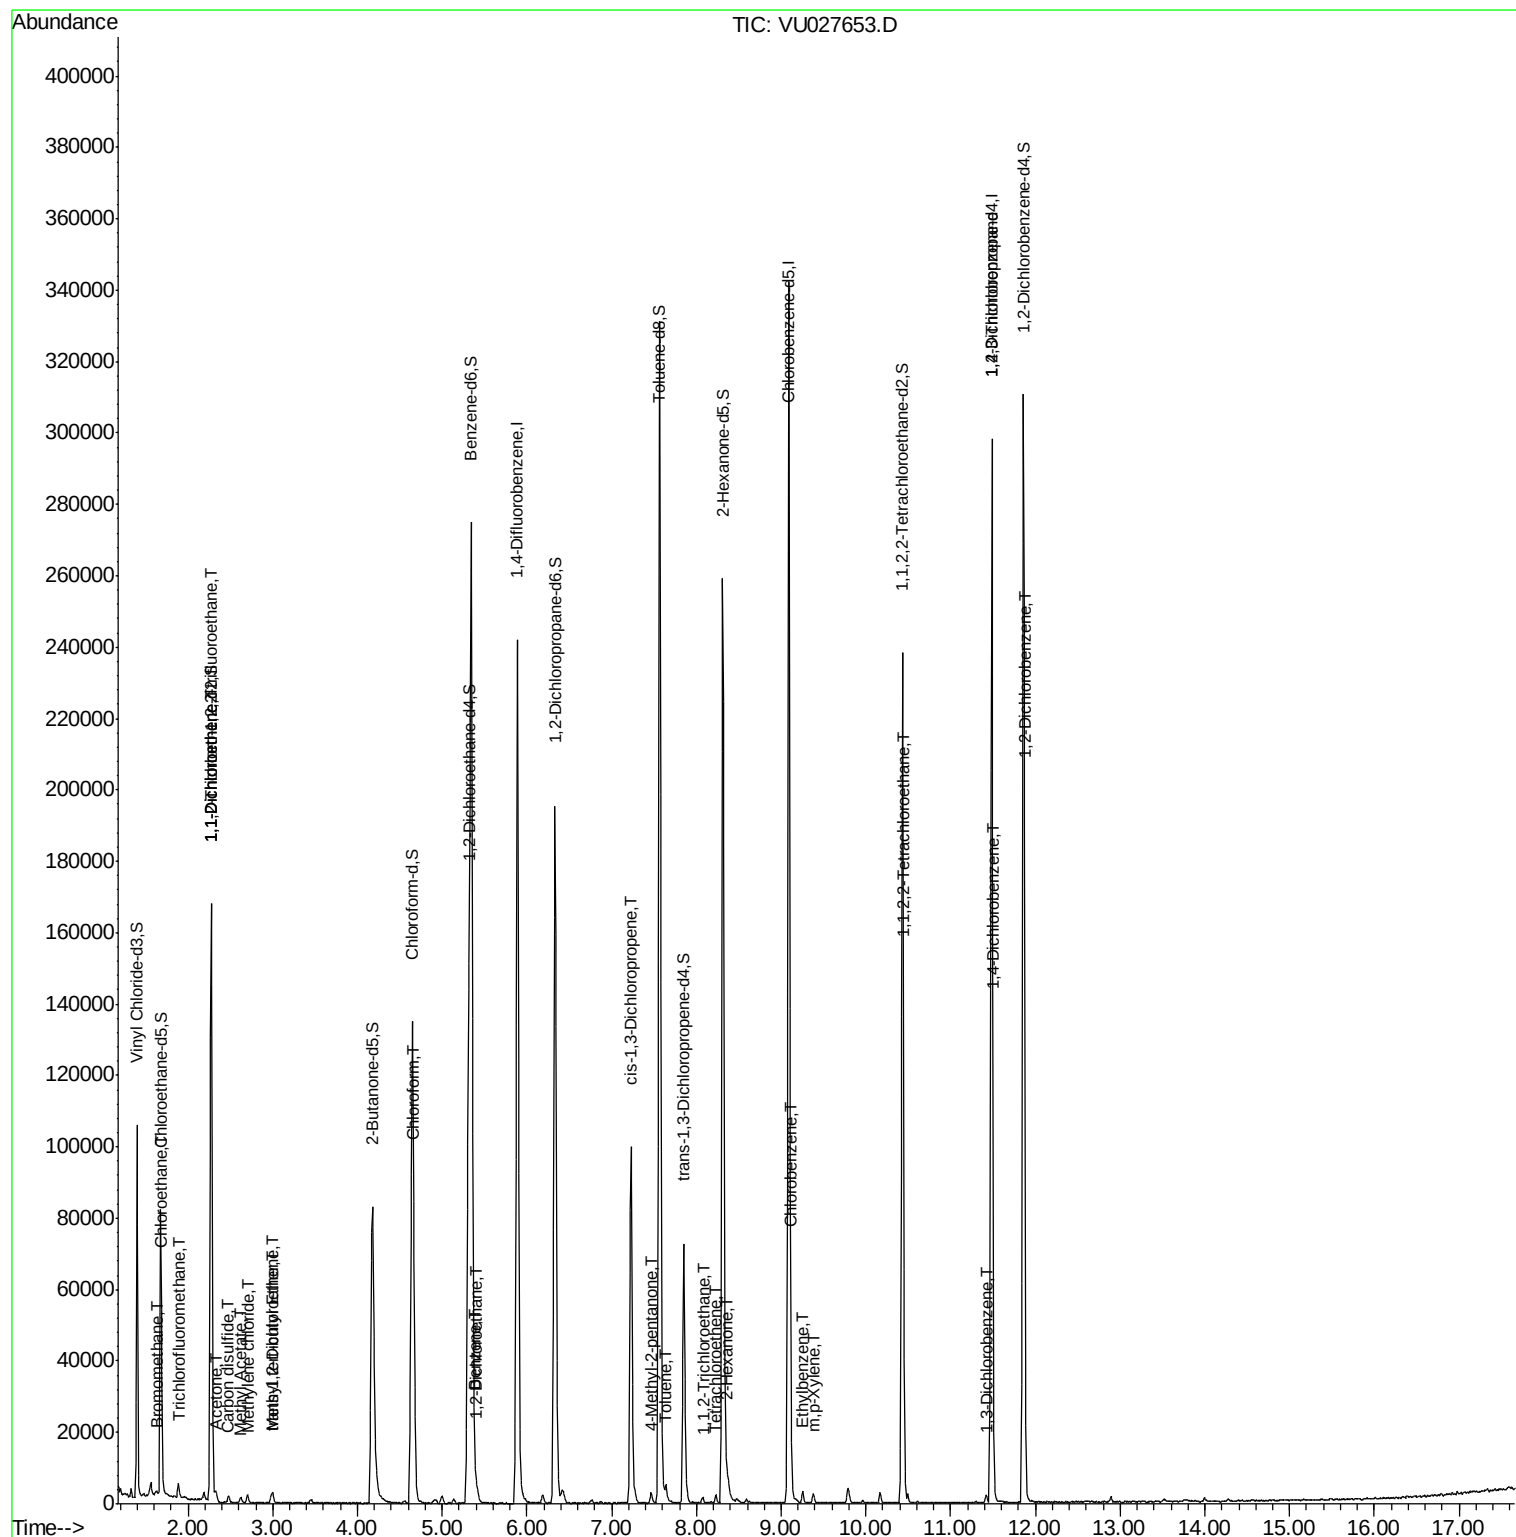

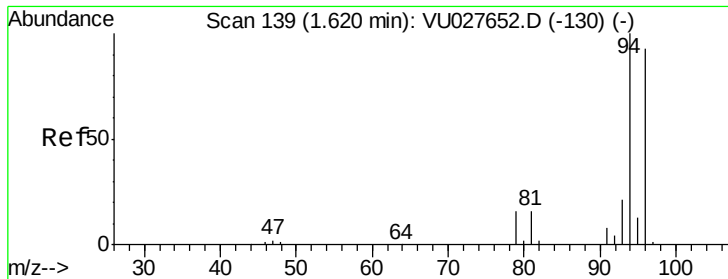

#6

Bromomethane

Concen: 0.624 ug/L

RT: 1.62 min Scan# 140

Delta R.T. -0.00 min

Lab File: VU027653.D

Acq: 15 Oct 2018 09:41

Instrument :

MSVOA_U

ClientSampleId :


VBLK58

Tgt Ion: 94 Resp: 583

Ion Ratio Lower Upper

94 100

96 105.3 66.6 123.8

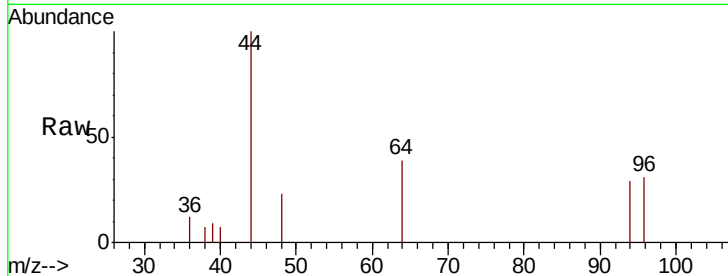

Abundance Ion 94.00 (93.70 to 94.70): VU0

Ion 96.00 (95.70 to 96.70): VU0

500

400

300

200

100



0

1.60

1.62

1.64

Time-->

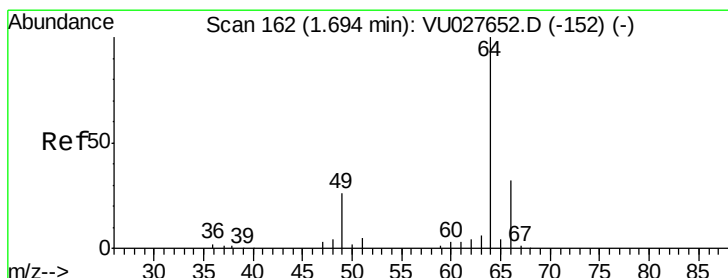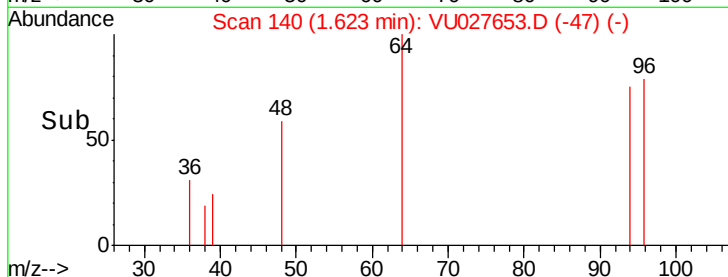

#8

Chloroethane

Concen: 0.426 ug/L

RT: 1.70 min Scan# 163

Delta R.T. -0.00 min

Lab File: VU027653.D


Acq: 15 Oct 2018 09:41

Tgt Ion: 64 Resp: 546

Ion Ratio Lower Upper

64 100

66 12.8 22.0 40.8#

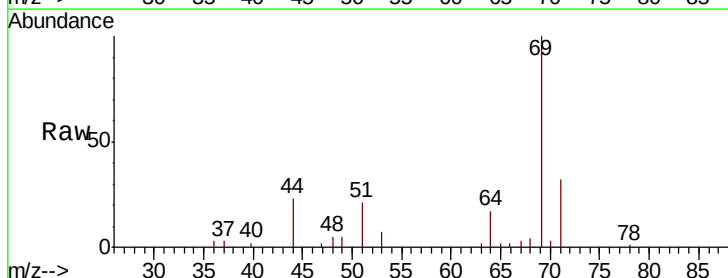

Abundance Ion 64.00 (63.70 to 64.70): VU0

Ion 66.00 (65.70 to 66.70): VU0

1000

500


0


1.68

1.70

1.72

Time-->

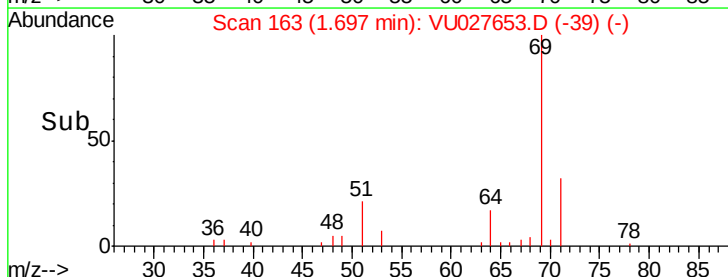







#9

Trichlorofluoromethane
Concen: 0.522 ug/L
RT: 1.89 min Scan# 223
Delta R.T. 0.00 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41

Instrument :
MSVOA_U
ClientSampleId :
VBLK58




Tgt Ion:101 Resp: 1117
Ion Ratio Lower Upper
101 100
103 68.1 51.1 76.7

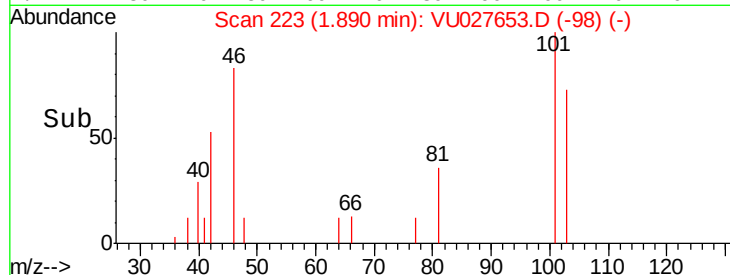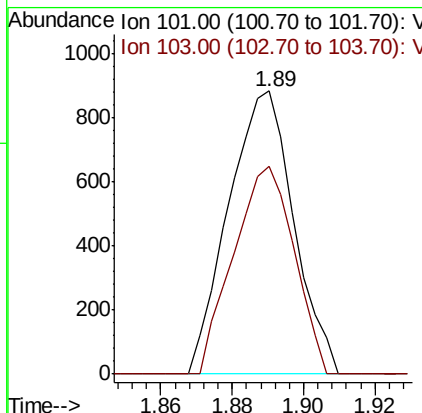


#10

1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 1.207 ug/L
RT: 2.28 min Scan# 343
Delta R.T. -0.01 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41

Tgt Ion:101 Resp: 1532
Ion Ratio Lower Upper
101 100
85 19.3 35.9 53.9#
151 29.0 55.7 83.5#

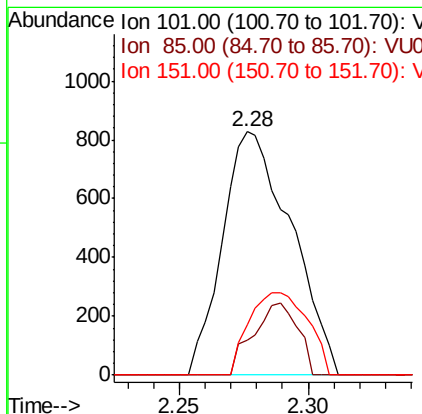

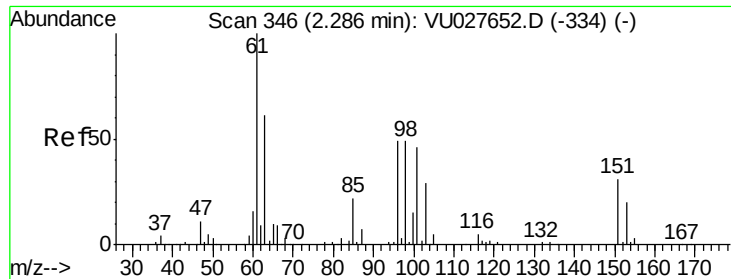

#12

1,1-Dichloroethene

Concen: 0.877 ug/L

RT: 2.28 min Scan# 343

Delta R.T. -0.01 min

Lab File: VU027653.D

Acq: 15 Oct 2018 09:41

Instrument :

MSVOA_U

ClientSampleId :

VBLK58


Tgt Ion: 96 Resp: 1087

Ion Ratio Lower Upper

96 100

61 1113.3 135.2 251.0#




63 9213.4 94.3 175.1#

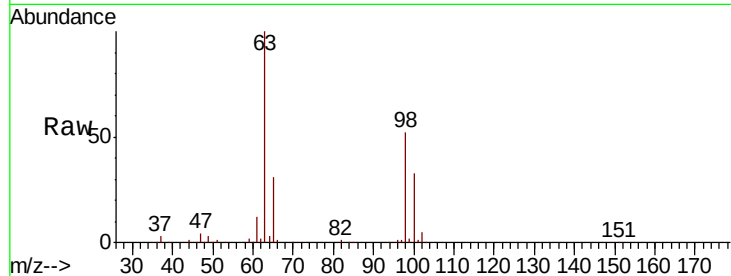

Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

Ion 63.00 (62.70 to 63.70): VU0

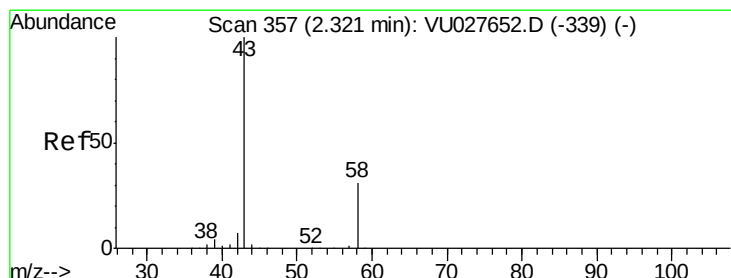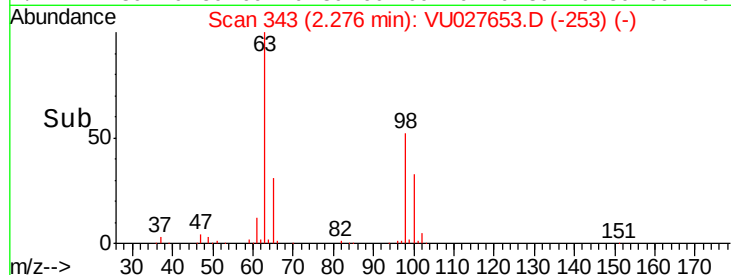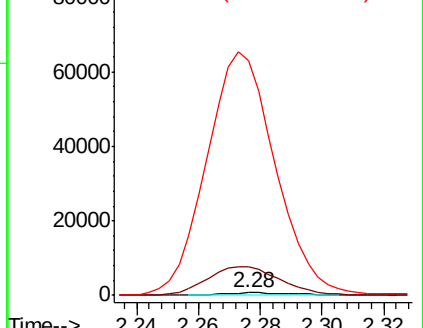

#13

Acetone

Concen: 1.893 ug/L

RT: 2.32 min Scan# 357

Delta R.T. -0.00 min

Lab File: VU027653.D


Acq: 15 Oct 2018 09:41

Tgt Ion: 43 Resp: 1893

Ion Ratio Lower Upper



43 100


58 26.7 0.0 60.8

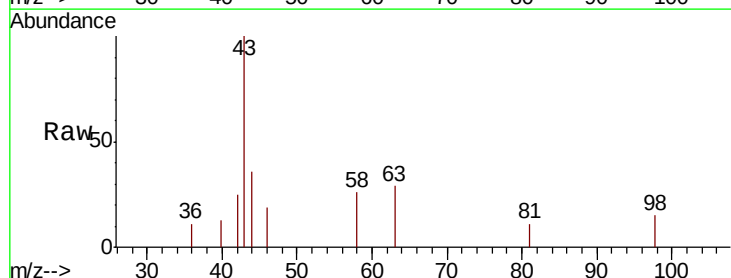

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

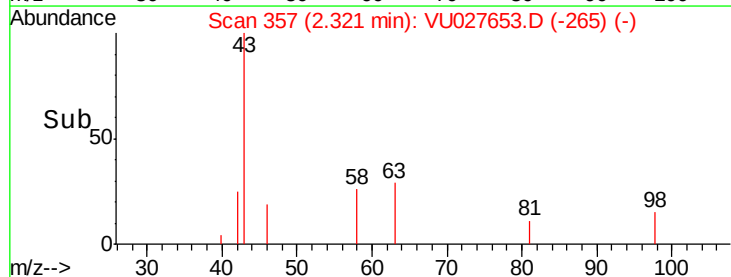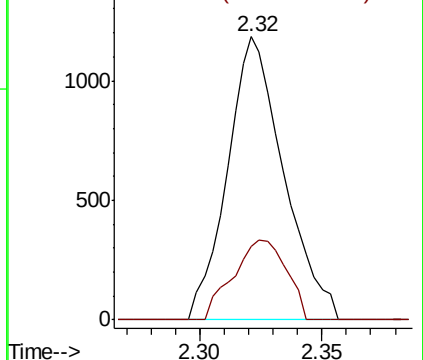



#14

Carbon disulfide

Concen: 0.568 ug/L

RT: 2.48 min Scan# 406

Delta R.T. -0.00 min

Lab File: VU027653.D

Acq: 15 Oct 2018 09:41

Instrument :

MSVOA_U

ClientSampleId :


VBLK58

Tgt Ion: 76 Resp: 2588

Ion Ratio Lower Upper




76 100

78 8.7 7.4 11.2



Abundance Ion 76.00 (75.70 to 76.70): VU0

Ion 78.00 (77.70 to 78.70): VU0

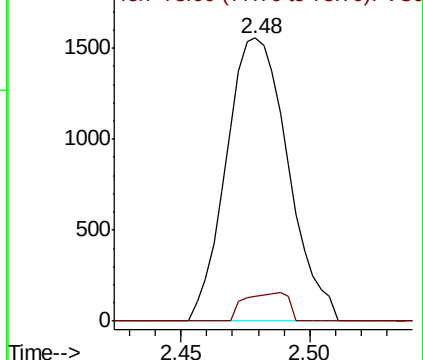

#15

Methyl Acetate

Concen: 1.014 ug/L

RT: 2.62 min Scan# 450

Delta R.T. 0.00 min

Lab File: VU027653.D


Acq: 15 Oct 2018 09:41

Tgt Ion: 43 Resp: 2031

Ion Ratio Lower Upper



43 100


74 17.1 16.0 24.0



Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 74.00 (73.70 to 74.70): VU0

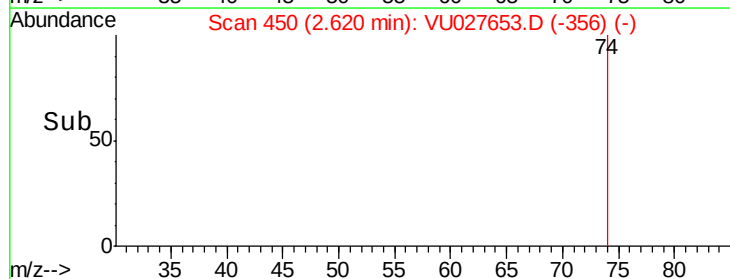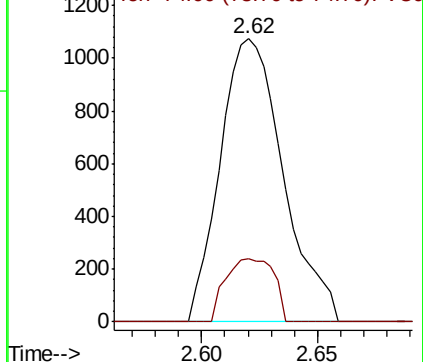


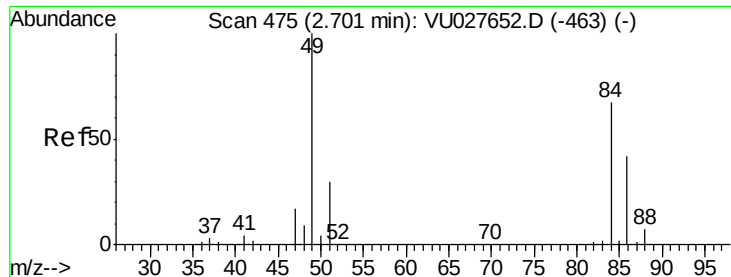




#16
Methylene chloride
Concen: 0.576 ug/L
RT: 2.70 min Scan# 476
Delta R.T. -0.00 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41

Instrument :
MSVOA_U
ClientSampled :
VBLK58

Tgt Ion: 84 Resp: 867
Ion Ratio Lower Upper
84 100
86 55.2 44.6 82.8
49 158.1 98.3 182.5

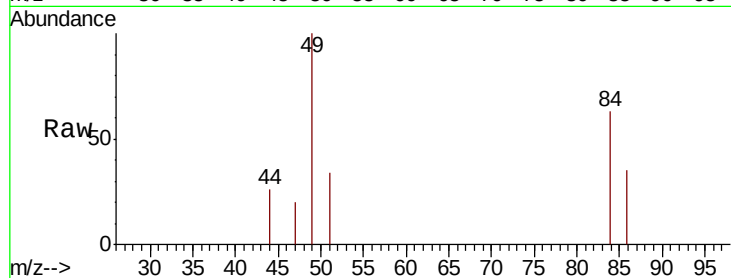


Abundance Ion 84.00 (83.70 to 84.70): VU0
Ion 86.00 (85.70 to 86.70): VU0
Ion 49.00 (48.70 to 49.70): VU0

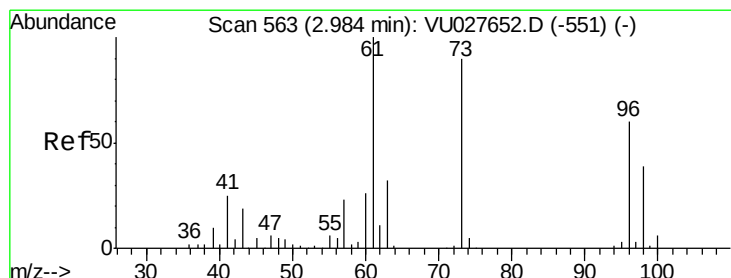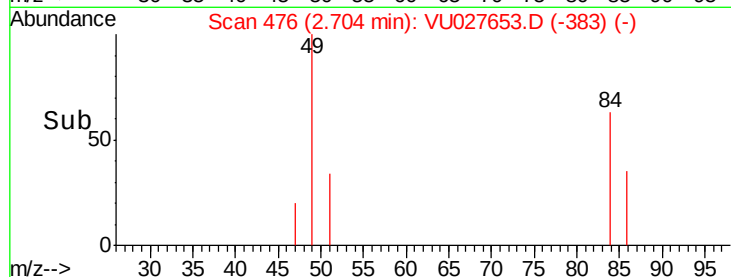
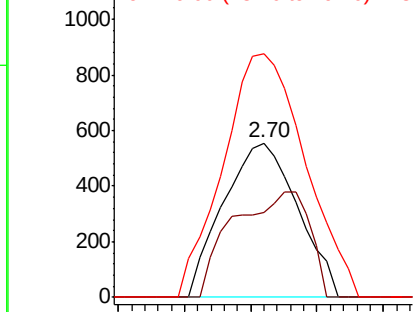



#17
trans-1,2-Dichloroethene
Concen: 0.487 ug/L
RT: 2.98 min Scan# 563
Delta R.T. -0.00 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41

Tgt Ion: 96 Resp: 668
Ion Ratio Lower Upper
96 100
61 122.8 110.9 205.9
98 55.1 43.7 81.1

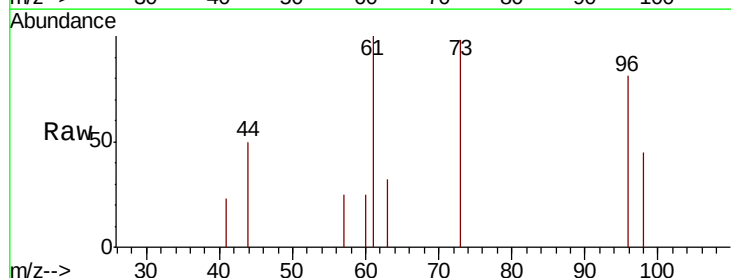

Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.00 (60.70 to 61.70): VU0
Ion 98.00 (97.70 to 98.70): VU0

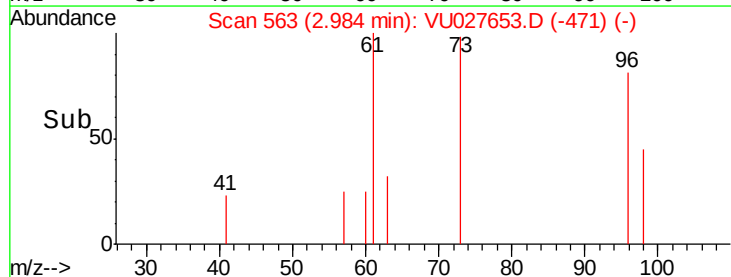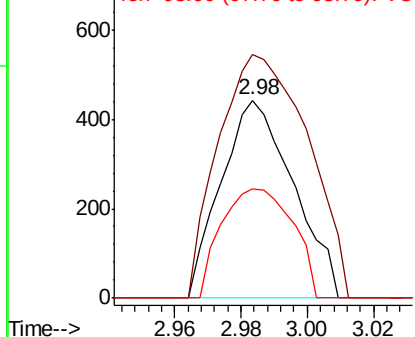


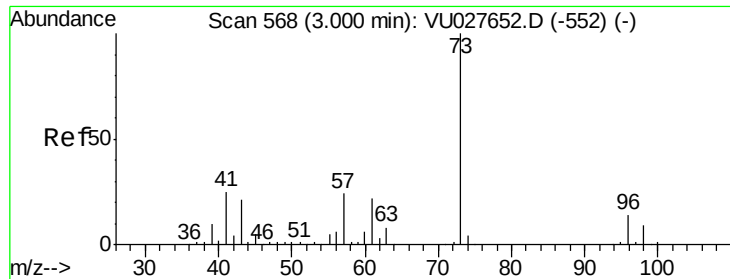




#18
Methyl tert-butyl Ether
Concen: 0.483 ug/L
RT: 3.00 min Scan# 568
Delta R.T. -0.00 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41

Instrument :
MSVOA_U
ClientSampled :
VBLK58

Tgt Ion: 73 Resp: 2206
Ion Ratio Lower Upper
73 100
43 7.6 16.5 24.7#
57 22.7 19.4 29.0




Abundance Ion 73.00 (72.70 to 73.70): VU0
Ion 43.00 (42.70 to 43.70): VU0
Ion 57.00 (56.70 to 57.70): VU0

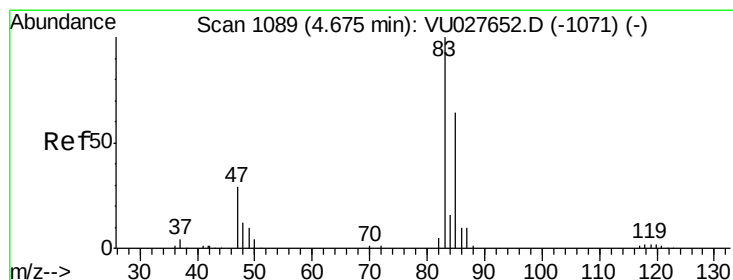
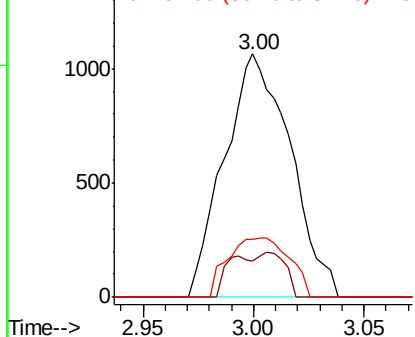



#25
Chloroform
Concen: 1.913 ug/L
RT: 4.67 min Scan# 1089
Delta R.T. -0.00 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41

Tgt Ion: 83 Resp: 5237
Ion Ratio Lower Upper
83 100
85 67.1 45.0 83.6

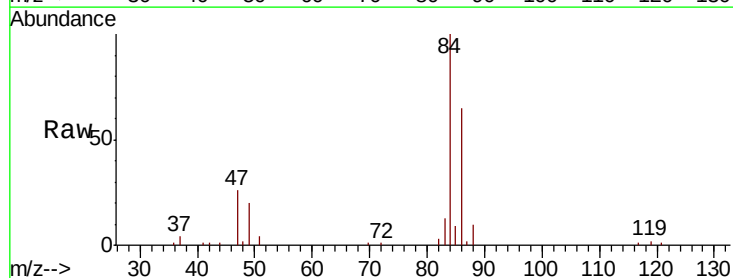

Abundance Ion 83.00 (82.70 to 83.70): VU0
Ion 85.00 (84.70 to 85.70): VU0



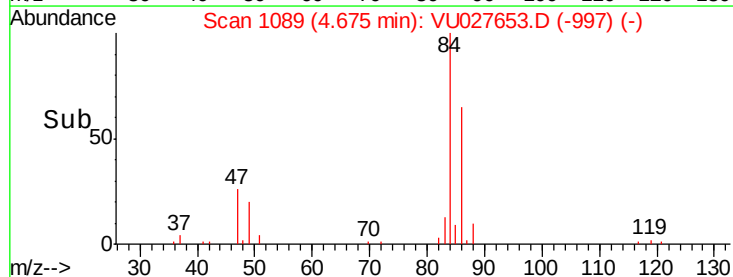
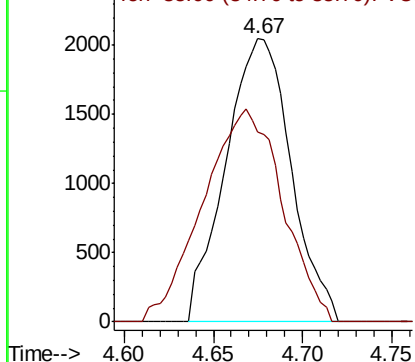


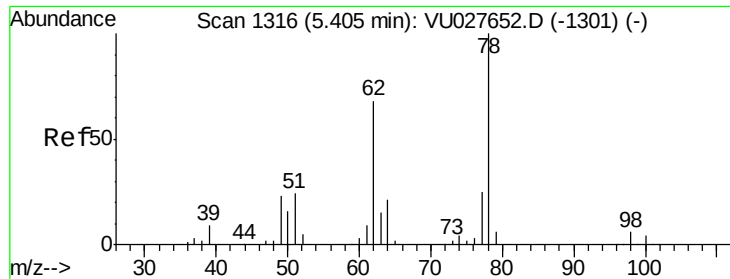

#27
 1,2-Dichloroethane
 Concen: 0.667 ug/L
 RT: 5.41 min Scan# 1319
 Delta R.T. 0.01 min
 Lab File: VU027653.D
 Acq: 15 Oct 2018 09:41




Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58


Tgt Ion: 62 Resp: 1467
 Ion Ratio Lower Upper
 62 100
 98 0.0 7.1 10.7#

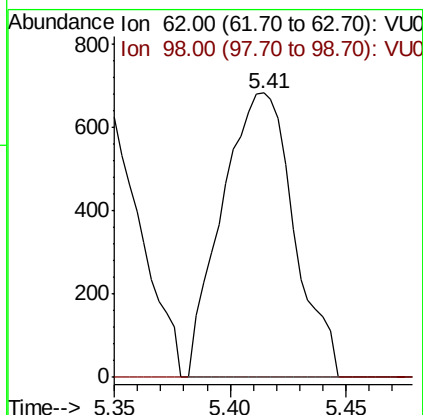

#33
 Benzene
 Concen: 0.528 ug/L
 RT: 5.39 min Scan# 1312
 Delta R.T. -0.00 min
 Lab File: VU027653.D
 Acq: 15 Oct 2018 09:41

Tgt Ion: 78 Resp: 3100


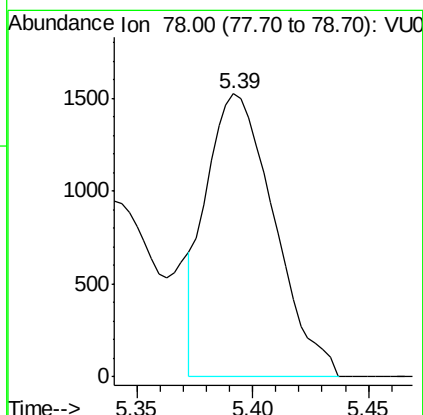




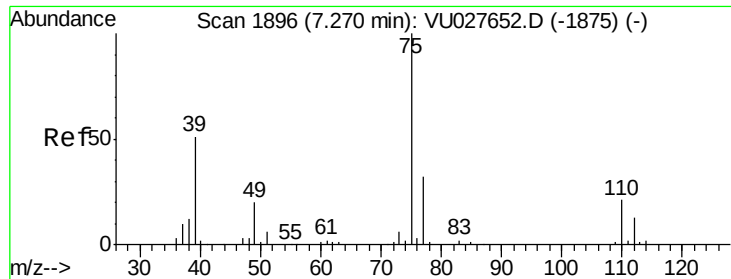

#39
 cis-1,3-Dichloropropene
 Concen: 0.951 ug/L
 RT: 7.23 min Scan# 1884
 Delta R.T. -0.04 min
 Lab File: VU027653.D
 Acq: 15 Oct 2018 09:41




Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58


Tgt Ion: 75 Resp: 2379
 Ion Ratio Lower Upper
 75 100
 77 49.2 22.1 41.1#

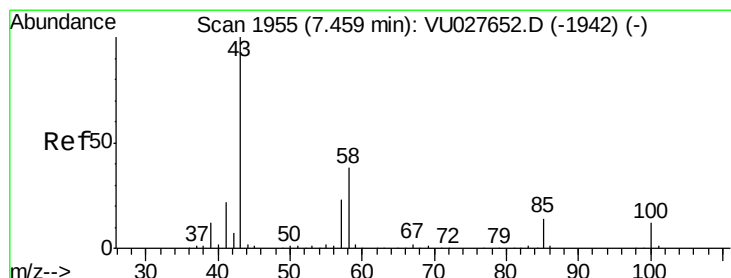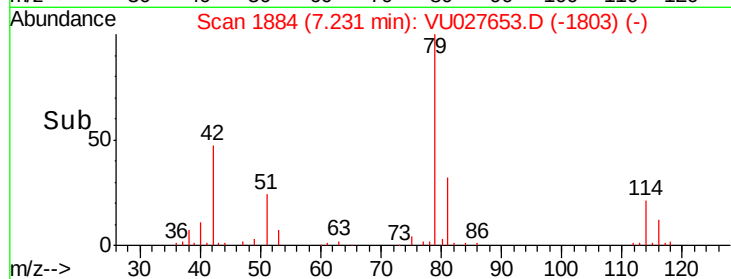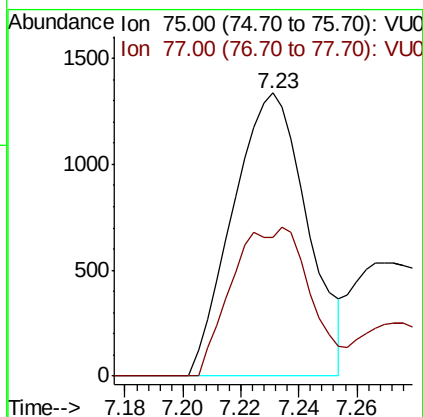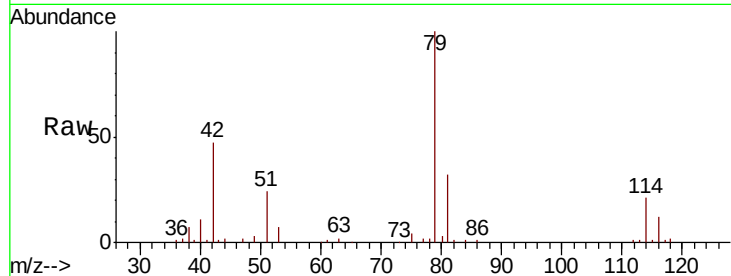

#40
 4-Methyl-2-pentanone
 Concen: 0.912 ug/L
 RT: 7.47 min Scan# 1957
 Delta R.T. 0.00 min
 Lab File: VU027653.D
 Acq: 15 Oct 2018 09:41

Tgt Ion: 43 Resp: 2273
 Ion Ratio Lower Upper
 43 100
 58 32.3 30.7 46.1
 100 5.4 10.2 15.4#

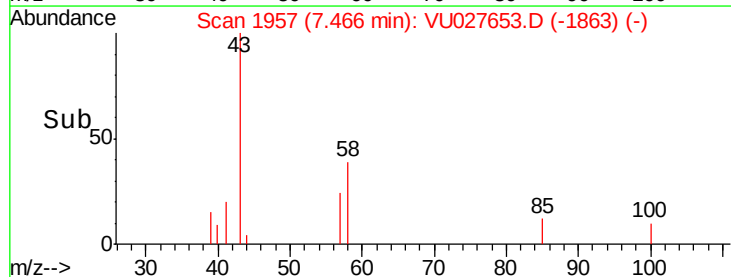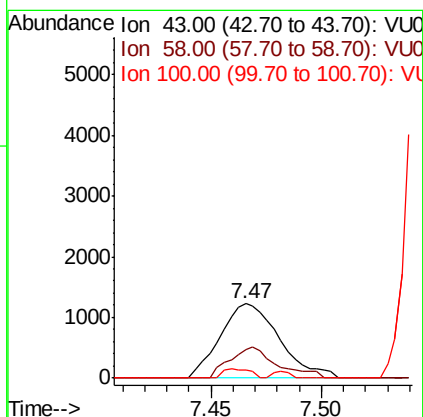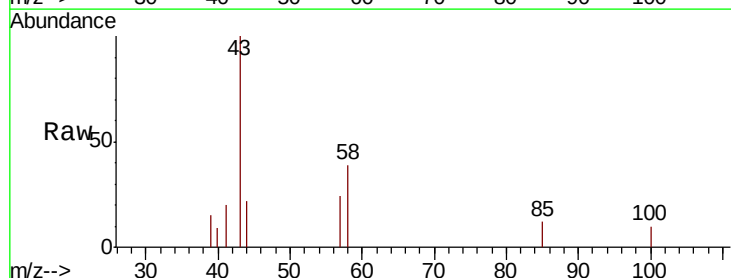

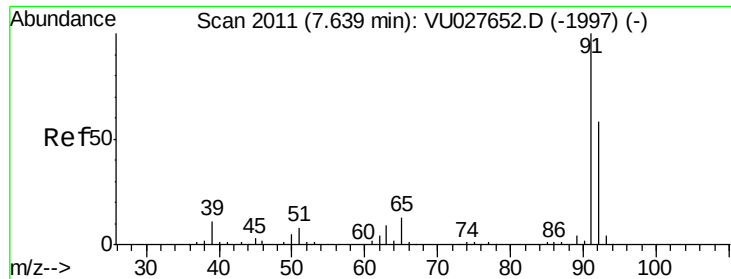

#42

Toluene

Concen: 0.559 ug/L

RT: 7.64 min Scan# 2012

Delta R.T. 0.00 min

Lab File: VU027653.D

Acq: 15 Oct 2018 09:41

Instrument :

MSVOA_U

ClientSampleId :


VBLK58

Tgt Ion: 91 Resp: 3298

Ion Ratio Lower Upper

91 100

92 55.9 40.2 74.6

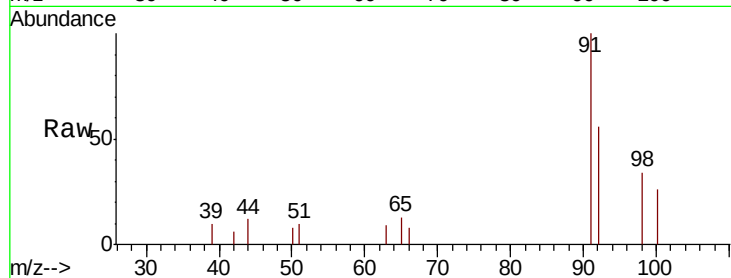

Abundance Ion 91.00 (90.70 to 91.70): VU0

Ion 92.00 (91.70 to 92.70): VU0

7.64

2000

1500

1000



500

0

Time-->

7.60

7.65

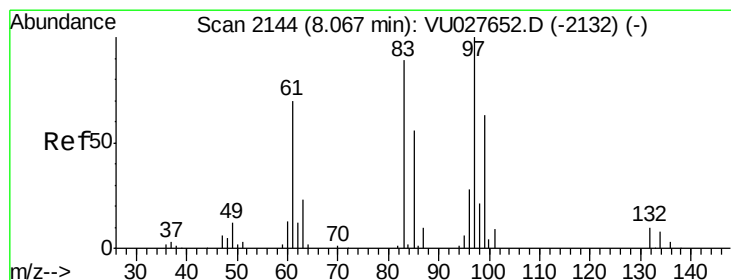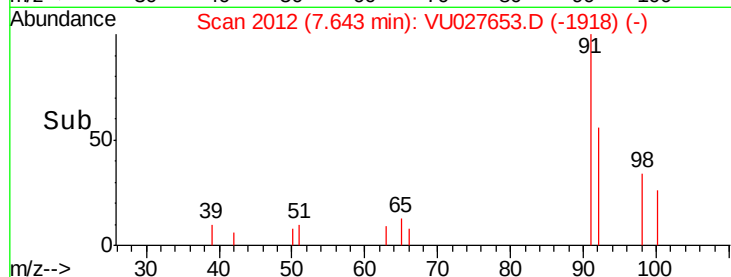

#45

1,1,2-Trichloroethane

Concen: 0.489 ug/L

RT: 8.08 min Scan# 2147

Delta R.T. 0.01 min

Lab File: VU027653.D

Acq: 15 Oct 2018 09:41

Tgt Ion: 97 Resp: 668


Ion Ratio Lower Upper

97 100

99 80.3 43.2 80.2#

83 95.4 64.3 119.5

85 62.3 41.0 76.2

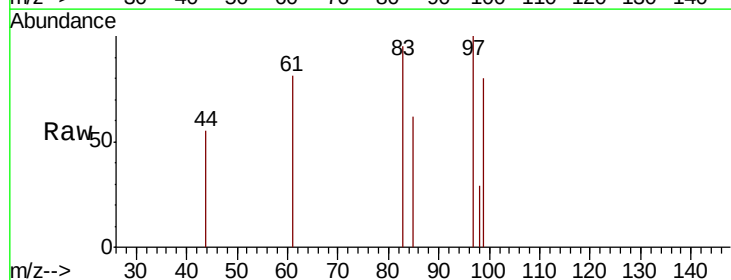

Abundance Ion 97.00 (96.70 to 97.70): VU0

Ion 99.00 (98.70 to 99.70): VU0

Ion 83.00 (82.70 to 83.70): VU0

Ion 85.00 (84.70 to 85.70): VU0

600

500

400

300

200

100

0


Time-->


8.04

8.06

8.08

8.10




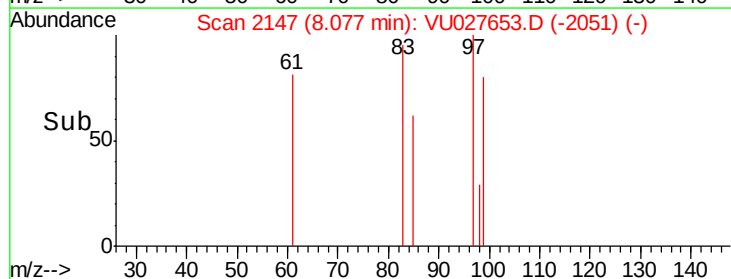


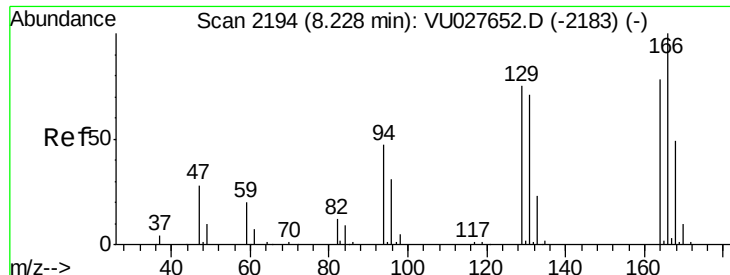

#46
Tetrachloroethene
Concen: 0.501 ug/L
RT: 8.23 min Scan# 2194
Delta R.T. -0.00 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41




Instrument :
MSVOA_U
ClientSampleId :
VBLK58


Tgt Ion:164 Resp: 526
Ion Ratio Lower Upper
164 100
129 77.2 67.0 124.4
131 82.8 65.1 120.9
166 101.0 90.4 167.8

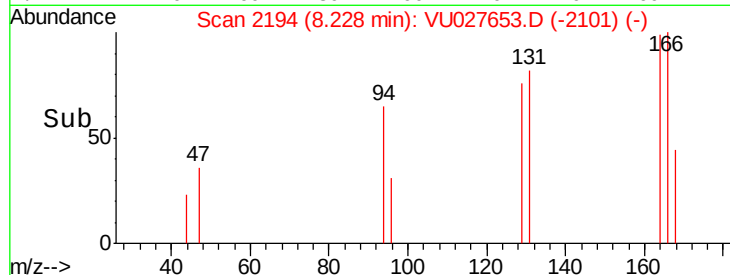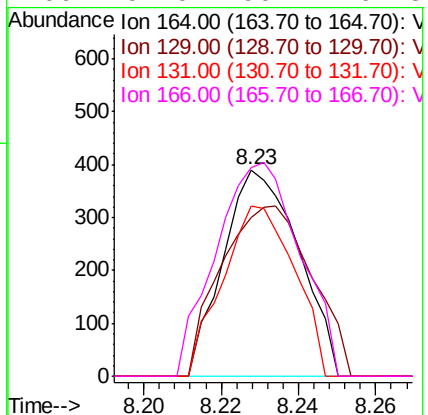

#48
2-Hexanone
Concen: 1.919 ug/L
RT: 8.37 min Scan# 2237
Delta R.T. 0.00 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41

Tgt Ion: 43 Resp: 3777
Ion Ratio Lower Upper
43 100
58 42.1 42.7 64.1#
57 15.4 14.5 21.7
100 2.9 8.2 12.2#

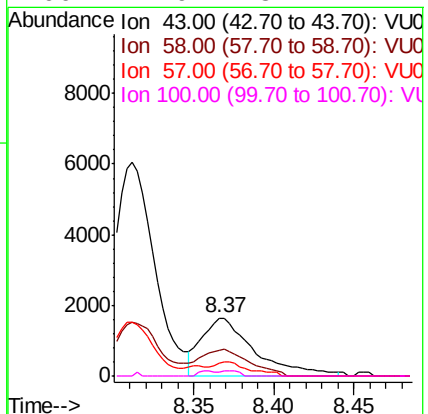


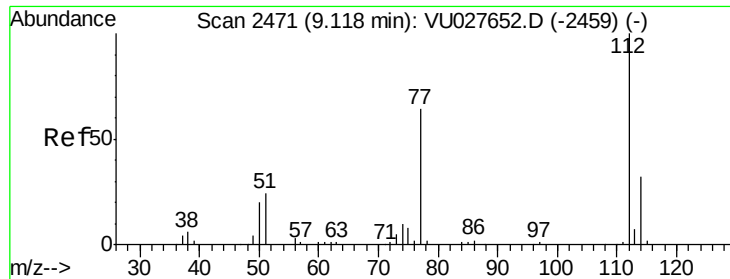




#51
Chlorobenzene
Concen: 0.530 ug/L
RT: 9.12 min Scan# 2472
Delta R.T. -0.00 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Tgt Ion: 112 Resp: 1974
Ion Ratio Lower Upper
112 100
114 26.9 22.3 41.5
77 75.0 51.7 77.5




Abundance Ion 112.00 (111.70 to 112.70): V
Ion 114.00 (113.70 to 114.70): V
Ion 77.00 (76.70 to 77.70): V


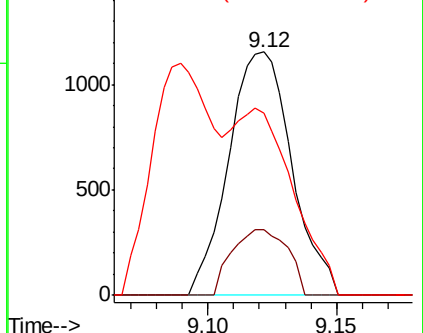



#52
Ethylbenzene
Concen: 0.440 ug/L
RT: 9.25 min Scan# 2513
Delta R.T. 0.00 min
Lab File: VU027653.D
Acq: 15 Oct 2018 09:41

Tgt Ion: 91 Resp: 2879
Ion Ratio Lower Upper
91 100
106 28.9 20.6 38.4



Abundance Ion 91.00 (90.70 to 91.70): V
Ion 106.00 (105.70 to 106.70): V

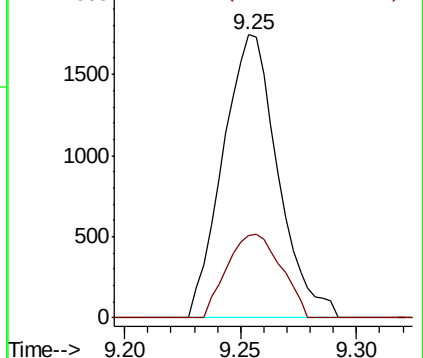


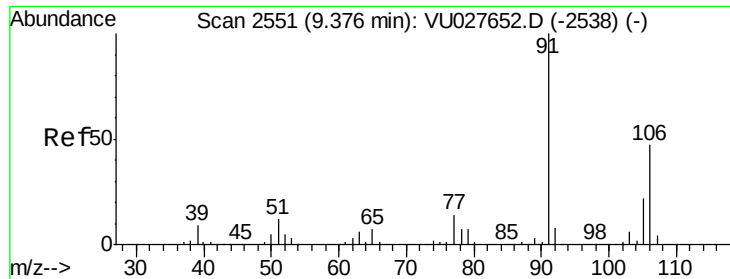




#53
 m,p-Xylene
 Concen: 0.394 ug/L
 RT: 9.38 min Scan# 2553
 Delta R.T. 0.01 min
 Lab File: VU027653.D
 Acq: 15 Oct 2018 09:41

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Tgt Ion: 106 Resp: 944
 Ion Ratio Lower Upper
 106 100
 91 180.2 145.0 269.4




Abundance Ion 106.00 (105.70 to 106.70): V
 Ion 91.00 (90.70 to 91.70): VU0


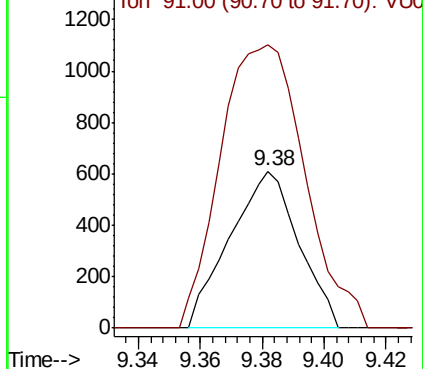



#58
 1,1,2,2-Tetrachloroethane
 Concen: 0.563 ug/L
 RT: 10.45 min Scan# 2886
 Delta R.T. -0.01 min
 Lab File: VU027653.D
 Acq: 15 Oct 2018 09:41

Tgt Ion: 83 Resp: 1349
 Ion Ratio Lower Upper
 83 100
 85 69.7 45.2 84.0
 131 27.2 6.7 10.1#



Abundance Ion 83.00 (82.70 to 83.70): VU0
 Ion 85.00 (84.70 to 85.70): VU0
 Ion 131.00 (130.70 to 131.70): V

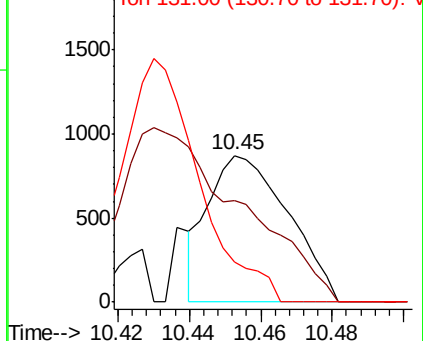


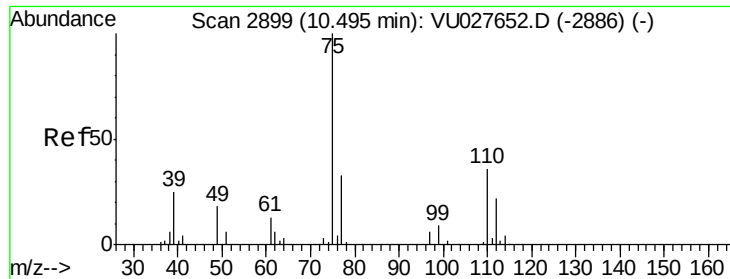




#59
 1,2,3-Trichloropropane
 Concen: 5.318 ug/L
 RT: 11.48 min Scan# 3207
 Delta R.T. 0.99 min
 Lab File: VU027653.D
 Acq: 15 Oct 2018 09:41

Instrument :
 MSVOA_U
 ClientSampled :
 VBLK58

Tgt Ion: 75 Resp: 10250
 Ion Ratio Lower Upper
 75 100
 77 35.6 25.7 38.5




Abundance Ion 75.00 (74.70 to 75.70): VU0
 Ion 77.00 (76.70 to 77.70): VU0


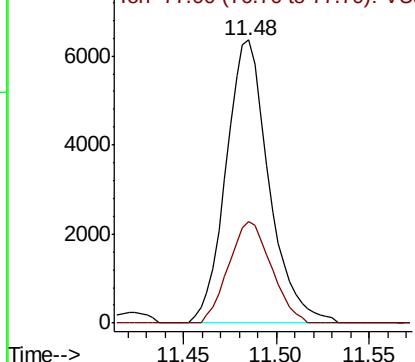



#62
 1,3-Dichlorobenzene
 Concen: 0.494 ug/L
 RT: 11.42 min Scan# 3188
 Delta R.T. 0.01 min
 Lab File: VU027653.D
 Acq: 15 Oct 2018 09:41

Tgt Ion: 146 Resp: 1104
 Ion Ratio Lower Upper
 146 100
 111 43.3 29.0 53.8
 148 66.3 45.4 84.2



Abundance Ion 146.00 (145.70 to 146.70): V
 Ion 111.00 (110.70 to 111.70): V
 Ion 148.00 (147.70 to 148.70): V

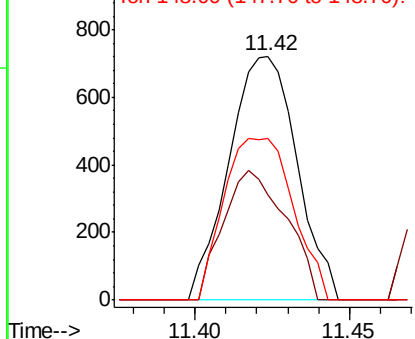

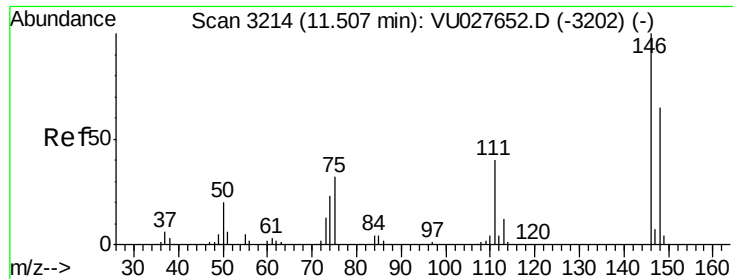

#63

1,4-Dichlorobenzene

Concen: 0.567 ug/L

RT: 11.51 min Scan# 3214

Delta R.T. -0.00 min

Lab File: VU027653.D

Acq: 15 Oct 2018 09:41





Instrument :

MSVOA_U

ClientSampleId :

VBLK58

Tgt Ion:	146	Resp:	1322
Ion	Ratio	Lower	Upper
146	100		
111	56.7	28.1	52.1#
148	70.4	44.4	82.5

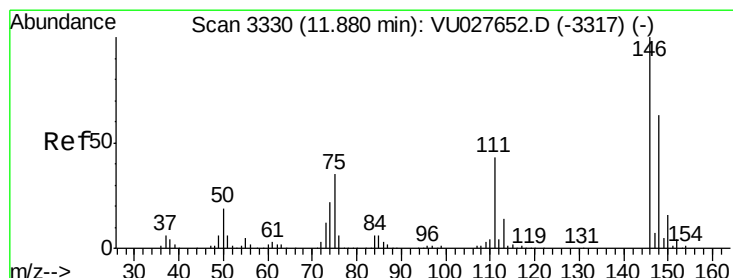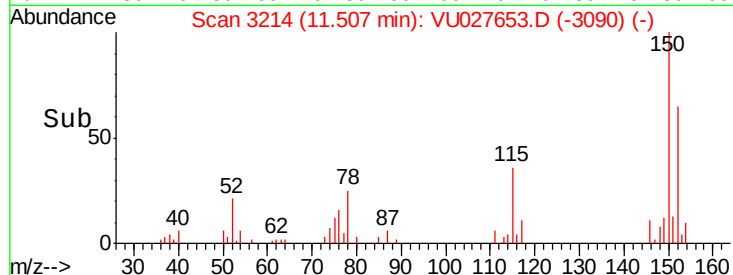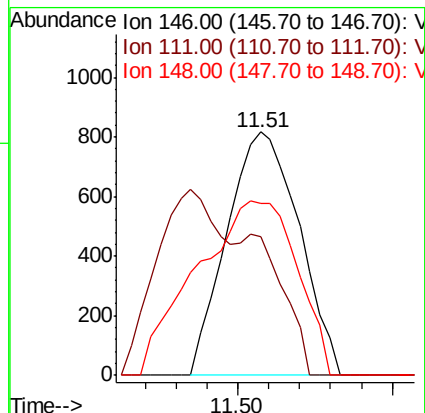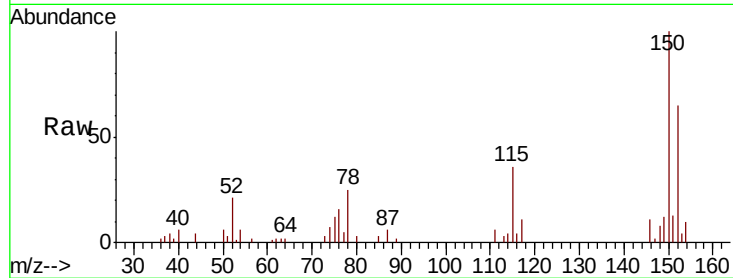

#65

1,2-Dichlorobenzene

Concen: 0.651 ug/L

RT: 11.88 min Scan# 3330

Delta R.T. -0.00 min

Lab File: VU027653.D

Acq: 15 Oct 2018 09:41

Tgt Ion:	146	Resp:	1480
Ion	Ratio	Lower	Upper
146	100		
111	57.1	34.9	52.3#
148	69.3	51.6	77.4

