

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101518\
 Data File : VU027655.D
 Acq On : 15 Oct 2018 10:27
 Operator : MD/SY
 Sample : J5405-17
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	64	70	85	rBV	97626	100747	13.18%	1.749%
2	1.681	151	158	180	rVB	77704	101743	13.31%	1.767%
3	2.273	332	342	357	rBV	151992	236099	30.89%	4.099%
4	2.440	391	394	398	rBV2	385	333	0.04%	0.006%
5	2.540	423	425	428	rBV2	184	110	0.01%	0.002%
6	2.665	461	464	465	rBV	217	126	0.02%	0.002%
7	2.701	470	475	483	rVB3	1175	1791	0.23%	0.031%
8	2.762	490	494	496	rBV	256	154	0.02%	0.003%
9	2.832	511	516	518	rBV2	535	493	0.06%	0.009%
10	2.868	525	527	530	rVB	187	91	0.01%	0.002%
11	2.916	540	542	545	rBV	168	101	0.01%	0.002%
12	2.935	546	548	550	rVB	157	47	0.01%	0.001%
13	2.990	558	565	566	rBV2	761	689	0.09%	0.012%
14	3.090	593	596	600	rBV	135	83	0.01%	0.001%
15	3.151	613	615	616	rBV	145	62	0.01%	0.001%
16	3.180	622	624	632	rVB	162	104	0.01%	0.002%
17	3.273	650	653	655	rBV	88	46	0.01%	0.001%
18	3.292	655	659	665	rVB2	222	214	0.03%	0.004%
19	3.324	666	669	672	rVV2	214	149	0.02%	0.003%
20	3.450	705	708	710	rBV2	322	198	0.03%	0.003%
21	3.492	718	721	724	rBV	85	48	0.01%	0.001%
22	3.659	772	773	777	rVB	184	59	0.01%	0.001%
23	3.688	777	782	786	rBV	178	136	0.02%	0.002%
24	3.710	786	789	791	rBV	108	73	0.01%	0.001%
25	3.733	794	796	799	rVB	135	89	0.01%	0.002%
26	3.765	804	806	807	rVV	148	63	0.01%	0.001%
27	3.778	807	810	812	rVB	185	86	0.01%	0.001%
28	3.855	831	834	835	rBV	111	53	0.01%	0.001%
29	3.890	840	845	848	rBV	116	100	0.01%	0.002%
30	3.906	848	850	853	rVB	165	82	0.01%	0.001%
31	4.125	916	918	921	rVB2	164	93	0.01%	0.002%
32	4.180	921	935	961	rBV	81987	217955	28.51%	3.784%
33	4.443	1015	1017	1022	rVB2	322	239	0.03%	0.004%
34	4.469	1023	1025	1030	rVB2	307	219	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101518\
 Data File : VU027655.D
 Acq On : 15 Oct 2018 10:27
 Operator : MD/SY
 Sample : J5405-17
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	4.508	1033	1037	1041	rBV2	387	282	0.04%	0.005%
36	4.527	1041	1043	1045	rBV	120	67	0.01%	0.001%
37	4.553	1048	1051	1054	rVB2	148	88	0.01%	0.002%
38	4.572	1054	1057	1061	rBV	179	111	0.01%	0.002%
39	4.652	1064	1082	1109	rBV	121338	301216	39.41%	5.230%
40	4.845	1139	1142	1146	rVB	75	49	0.01%	0.001%
41	4.868	1146	1149	1151	rBV	70	47	0.01%	0.001%
42	4.887	1151	1155	1159	rBV2	290	333	0.04%	0.006%
43	4.935	1168	1170	1173	rVB	151	63	0.01%	0.001%
44	4.964	1176	1179	1185	rBV2	209	176	0.02%	0.003%
45	4.987	1185	1186	1187	rVV2	314	109	0.01%	0.002%
46	4.996	1187	1189	1196	rVB3	680	539	0.07%	0.009%
47	5.131	1227	1231	1240	rVB2	397	497	0.07%	0.009%
48	5.186	1245	1248	1251	rVB2	175	127	0.02%	0.002%
49	5.215	1251	1257	1260	rBV	100	102	0.01%	0.002%
50	5.247	1265	1267	1271	rVB	124	52	0.01%	0.001%
51	5.344	1272	1297	1327	rBV2	254234	764381	100.00%	13.272%
52	5.562	1363	1365	1369	rVB	212	107	0.01%	0.002%
53	5.594	1373	1375	1382	rVB	139	128	0.02%	0.002%
54	5.630	1382	1386	1388	rBV	64	45	0.01%	0.001%
55	5.668	1393	1398	1401	rBV	110	75	0.01%	0.001%
56	5.691	1401	1405	1411	rBV	122	160	0.02%	0.003%
57	5.717	1411	1413	1415	rVV	110	61	0.01%	0.001%
58	5.746	1419	1422	1429	rVB	256	252	0.03%	0.004%
59	5.781	1429	1433	1435	rBV	78	59	0.01%	0.001%
60	5.887	1452	1466	1491	rBV	245645	495900	64.88%	8.610%
61	6.106	1531	1534	1537	rVB2	183	131	0.02%	0.002%
62	6.125	1538	1540	1542	rBV	140	74	0.01%	0.001%
63	6.186	1550	1559	1566	rVB4	1198	2010	0.26%	0.035%
64	6.334	1590	1605	1626	rBV	180647	364944	47.74%	6.336%
65	6.504	1656	1658	1660	rVB	160	84	0.01%	0.001%
66	6.530	1660	1666	1671	rBV	80	100	0.01%	0.002%
67	6.755	1732	1736	1738	rBV2	207	168	0.02%	0.003%
68	6.790	1744	1747	1751	rBV	173	124	0.02%	0.002%
69	6.868	1765	1771	1775	rVB3	436	546	0.07%	0.009%
70	6.987	1805	1808	1810	rBV	69	47	0.01%	0.001%
71	7.035	1817	1823	1826	rBV	118	102	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101518\
 Data File : VU027655.D
 Acq On : 15 Oct 2018 10:27
 Operator : MD/SY
 Sample : J5405-17
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	7.231	1872	1884	1902	rBV	91204	166372	21.77%	2.889%
73	7.389	1928	1933	1939	rVB2	305	335	0.04%	0.006%
74	7.414	1939	1941	1944	rBV	69	50	0.01%	0.001%
75	7.430	1944	1946	1948	rVB	112	64	0.01%	0.001%
76	7.466	1950	1957	1965	rBV2	805	1143	0.15%	0.020%
77	7.511	1969	1971	1974	rBB	119	83	0.01%	0.001%
78	7.565	1974	1988	2008	rBV	309487	542873	71.02%	9.426%
79	7.733	2037	2040	2042	rBV	249	131	0.02%	0.002%
80	7.852	2066	2077	2101	rBV	66940	114929	15.04%	1.995%
81	7.983	2116	2118	2122	rVB	164	81	0.01%	0.001%
82	8.038	2131	2135	2138	rBV	213	159	0.02%	0.003%
83	8.180	2172	2179	2186	rBV2	376	642	0.08%	0.011%
84	8.231	2190	2195	2200	rVB3	585	609	0.08%	0.011%
85	8.311	2208	2220	2249	rBV	253398	445335	58.26%	7.732%
86	8.543	2289	2292	2296	rBV2	247	159	0.02%	0.003%
87	8.585	2303	2305	2308	rBV3	361	197	0.03%	0.003%
88	8.842	2383	2385	2388	rBV	93	58	0.01%	0.001%
89	8.932	2411	2413	2415	rVB	151	79	0.01%	0.001%
90	9.089	2450	2462	2486	rBV	354399	590903	77.30%	10.260%
91	9.260	2506	2515	2521	rBV3	899	1422	0.19%	0.025%
92	9.379	2547	2552	2562	rVB4	1023	1405	0.18%	0.024%
93	9.424	2563	2566	2567	rBV2	125	74	0.01%	0.001%
94	9.784	2673	2678	2679	rBV3	788	590	0.08%	0.010%
95	10.433	2867	2880	2898	rBV	230741	369490	48.34%	6.415%
96	10.607	2930	2934	2939	rBV2	274	374	0.05%	0.006%
97	10.774	2981	2986	2992	rBV	313	362	0.05%	0.006%
98	11.080	3078	3081	3085	rBV2	218	147	0.02%	0.003%
99	11.485	3195	3207	3224	rBV	295712	471144	61.64%	8.180%
100	11.861	3311	3324	3348	rBV	282248	454198	59.42%	7.886%


Sum of corrected areas: 5759439

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101518\
Data File : VU027655.D
Acq On : 15 Oct 2018 10:27
Operator : MD/SY
Sample : J5405-17
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

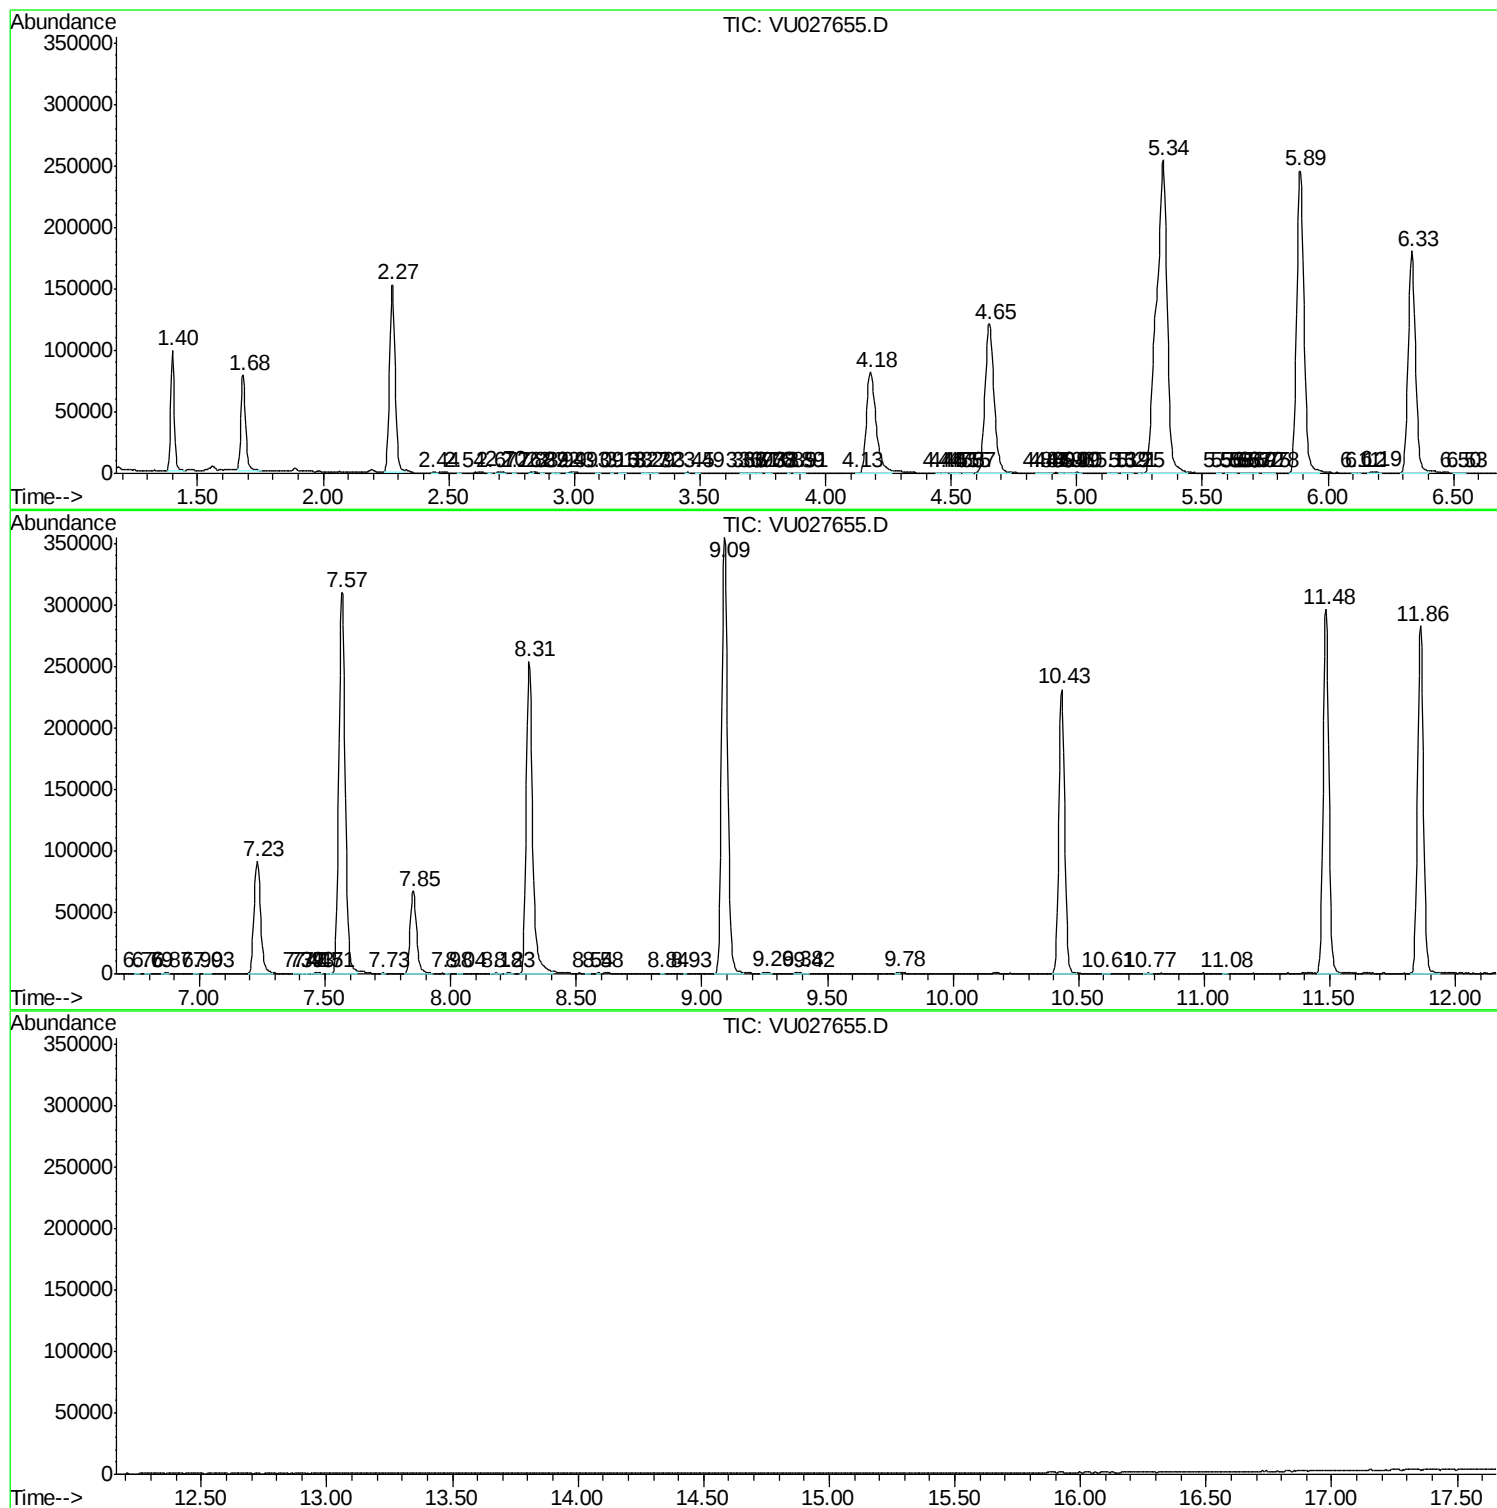

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101518\
Data File : VU027655.D
Acq On : 15 Oct 2018 10:27
Operator : MD/SY
Sample : J5405-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101518\
Data File : VU027655.D
Acq On : 15 Oct 2018 10:27
Operator : MD/SY
Sample : J5405-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc