

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101518\
 Data File : VU027661.D
 Acq On : 15 Oct 2018 12:51
 Operator : MD/SY
 Sample : J5403-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.398	63	70	87	rBV	98315	97828	13.18%	1.757%
2	1.665	146	153	166	rBV	74399	93554	12.60%	1.680%
3	2.189	310	316	321	rVB4	1171	1508	0.20%	0.027%
4	2.270	330	341	354	rBV	151758	230308	31.03%	4.137%
5	2.443	392	395	397	rBV	180	158	0.02%	0.003%
6	2.466	398	402	403	rVV	417	335	0.05%	0.006%
7	2.476	403	405	412	rVB	620	544	0.07%	0.010%
8	2.623	441	451	460	rVB3	926	1426	0.19%	0.026%
9	2.701	468	475	482	rVB3	1155	1891	0.25%	0.034%
10	2.832	508	516	527	rBV3	988	1813	0.24%	0.033%
11	2.980	558	562	563	rBV	433	251	0.03%	0.005%
12	3.437	699	704	706	rBV	260	210	0.03%	0.004%
13	4.038	887	891	899	rBV	187	147	0.02%	0.003%
14	4.176	920	934	972	rBV2	77348	209984	28.29%	3.772%
15	4.450	1018	1019	1027	rVB2	242	160	0.02%	0.003%
16	4.530	1038	1044	1047	rVB2	209	264	0.04%	0.005%
17	4.649	1063	1081	1107	rBV	119464	292532	39.41%	5.254%
18	4.884	1152	1154	1158	rVV	292	260	0.04%	0.005%
19	4.910	1158	1162	1163	rVV2	285	236	0.03%	0.004%
20	4.919	1163	1165	1169	rVB2	250	161	0.02%	0.003%
21	4.984	1182	1185	1187	rBV2	381	250	0.03%	0.004%
22	5.102	1218	1222	1225	rBV	118	117	0.02%	0.002%
23	5.122	1226	1228	1231	rBV2	260	184	0.02%	0.003%
24	5.340	1270	1296	1321	rBV2	248006	742323	100.00%	13.333%
25	5.530	1352	1355	1365	rVB2	264	225	0.03%	0.004%
26	5.668	1391	1398	1400	rBV	121	118	0.02%	0.002%
27	5.887	1452	1466	1496	rBV	242720	476957	64.25%	8.567%
28	5.990	1496	1498	1505	rVB3	382	344	0.05%	0.006%
29	6.176	1551	1556	1557	rBV3	964	842	0.11%	0.015%
30	6.331	1588	1604	1624	rBV	178429	355762	47.93%	6.390%
31	6.430	1633	1635	1643	rVB3	1016	1051	0.14%	0.019%
32	6.533	1664	1667	1670	rBV	183	181	0.02%	0.003%
33	6.697	1715	1718	1723	rVV	201	144	0.02%	0.003%
34	6.758	1734	1737	1741	rVV2	318	292	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101518\
 Data File : VU027661.D
 Acq On : 15 Oct 2018 12:51
 Operator : MD/SY
 Sample : J5403-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	6.868	1763	1771	1773	rBV2	640	712	0.10%	0.013%
36	6.922	1785	1788	1795	rVB2	221	220	0.03%	0.004%
37	7.106	1842	1845	1849	rBV2	208	146	0.02%	0.003%
38	7.228	1870	1883	1901	rBV	89738	159401	21.47%	2.863%
39	7.318	1910	1911	1914	rVB	274	128	0.02%	0.002%
40	7.392	1930	1934	1937	rVV2	356	238	0.03%	0.004%
41	7.472	1952	1959	1966	rVV3	909	1165	0.16%	0.021%
42	7.565	1975	1988	2010	rBV	298394	522565	70.40%	9.386%
43	7.720	2033	2036	2037	rBV	331	174	0.02%	0.003%
44	7.852	2065	2077	2098	rVV	63783	109085	14.70%	1.959%
45	8.073	2143	2146	2147	rBV	309	159	0.02%	0.003%
46	8.122	2157	2161	2163	rBV2	189	164	0.02%	0.003%
47	8.167	2170	2175	2177	rBV	158	146	0.02%	0.003%
48	8.228	2190	2194	2197	rBV3	715	735	0.10%	0.013%
49	8.311	2208	2220	2262	rBV	249916	432273	58.23%	7.764%
50	8.533	2287	2289	2293	rVB	333	142	0.02%	0.003%
51	8.569	2296	2300	2302	rBV2	182	160	0.02%	0.003%
52	8.594	2306	2308	2310	rVV2	397	146	0.02%	0.003%
53	8.623	2313	2317	2320	rVB3	485	376	0.05%	0.007%
54	8.649	2320	2325	2328	rBV2	275	272	0.04%	0.005%
55	8.925	2409	2411	2416	rVV	231	136	0.02%	0.002%
56	8.987	2425	2430	2433	rVV2	230	195	0.03%	0.004%
57	9.048	2443	2449	2450	rVV	186	182	0.02%	0.003%
58	9.089	2450	2462	2492	rVV	341143	564560	76.05%	10.140%
59	9.205	2495	2498	2503	rVB2	397	331	0.04%	0.006%
60	9.257	2503	2514	2520	rBV2	933	1357	0.18%	0.024%
61	9.350	2539	2543	2544	rVV	179	122	0.02%	0.002%
62	9.379	2547	2552	2565	rVB3	659	1160	0.16%	0.021%
63	9.540	2598	2602	2605	rVB2	168	162	0.02%	0.003%
64	9.710	2651	2655	2660	rBV	118	121	0.02%	0.002%
65	9.778	2671	2676	2677	rBV	625	421	0.06%	0.008%
66	9.800	2682	2683	2690	rVB	589	425	0.06%	0.008%
67	9.983	2737	2740	2742	rVB	191	129	0.02%	0.002%
68	10.167	2793	2797	2798	rBV2	404	303	0.04%	0.005%
69	10.327	2844	2847	2850	rBV	197	120	0.02%	0.002%
70	10.369	2857	2860	2862	rBV	210	140	0.02%	0.003%
71	10.433	2866	2880	2897	rBV	233175	367656	49.53%	6.604%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101518\
 Data File : VU027661.D
 Acq On : 15 Oct 2018 12:51
 Operator : MD/SY
 Sample : J5403-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	10.575	2922	2924	2929	rBV2	186	124	0.02%	0.002%
73	10.642	2943	2945	2949	rVB2	187	128	0.02%	0.002%
74	10.761	2979	2982	2985	rBV	151	126	0.02%	0.002%
75	10.797	2989	2993	2994	rBV	176	117	0.02%	0.002%
76	10.880	3017	3019	3022	rBV	167	131	0.02%	0.002%
77	11.109	3087	3090	3094	rVB2	181	143	0.02%	0.003%
78	11.138	3094	3099	3101	rBV2	241	230	0.03%	0.004%
79	11.215	3118	3123	3124	rVV	145	157	0.02%	0.003%
80	11.260	3134	3137	3141	rVB	207	127	0.02%	0.002%
81	11.308	3147	3152	3154	rBV	204	152	0.02%	0.003%
82	11.417	3182	3186	3195	rVB2	461	562	0.08%	0.010%
83	11.485	3195	3207	3224	rBV	285595	443144	59.70%	7.960%
84	11.655	3257	3260	3264	rVB2	409	308	0.04%	0.006%
85	11.678	3264	3267	3269	rBV	239	156	0.02%	0.003%
86	11.861	3312	3324	3347	rVV	276985	440569	59.35%	7.913%
87	12.012	3368	3371	3372	rBV	285	165	0.02%	0.003%
88	12.083	3390	3393	3397	rVB	328	190	0.03%	0.003%
89	12.105	3398	3400	3406	rVB2	232	193	0.03%	0.003%
90	12.141	3409	3411	3417	rVB2	342	312	0.04%	0.006%
91	12.166	3417	3419	3421	rBV2	190	123	0.02%	0.002%
92	12.363	3478	3480	3483	rBV	207	121	0.02%	0.002%
93	12.707	3584	3587	3592	rBV2	206	238	0.03%	0.004%
94	12.896	3642	3646	3650	rVB3	223	202	0.03%	0.004%
95	13.363	3788	3791	3794	rBV2	248	198	0.03%	0.004%
96	13.459	3818	3821	3825	rVB2	289	195	0.03%	0.004%
97	13.961	3975	3977	3979	rBV	276	132	0.02%	0.002%
98	14.125	4023	4028	4030	rBV3	339	313	0.04%	0.006%
99	14.318	4085	4088	4091	rBV	308	188	0.03%	0.003%
100	14.916	4271	4274	4279	rBV	400	427	0.06%	0.008%




Sum of corrected areas: 5567458

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101518\
Data File : VU027661.D
Acq On : 15 Oct 2018 12:51
Operator : MD/SY
Sample : J5403-18
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Title :

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

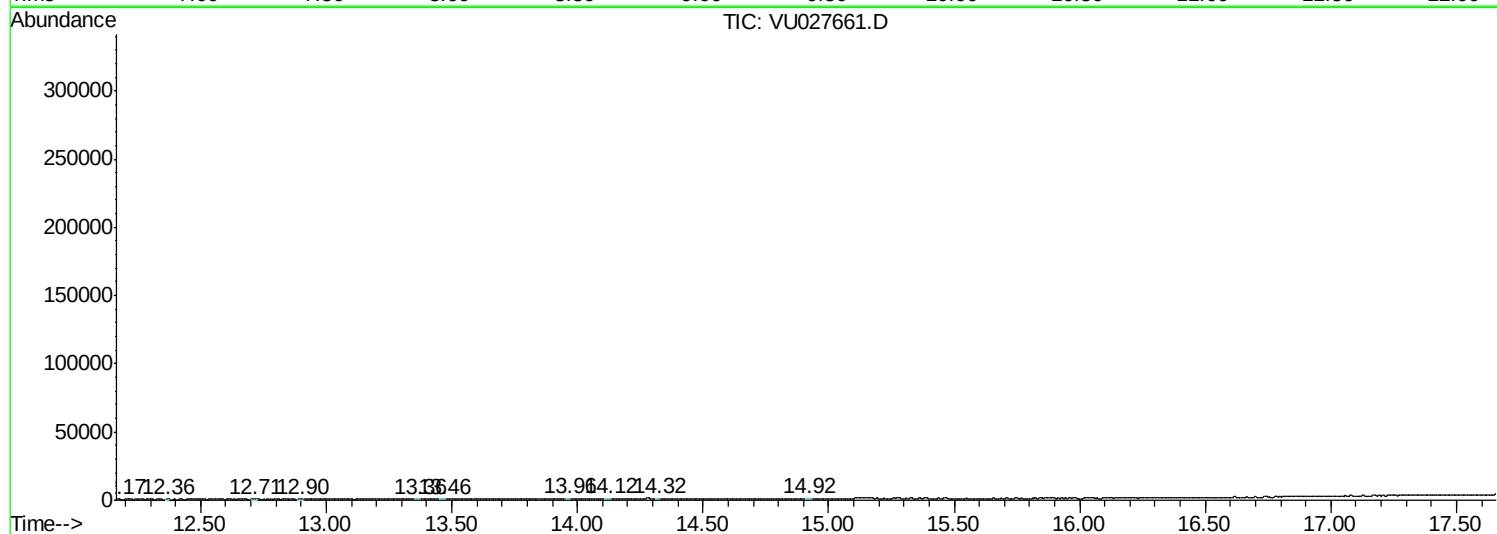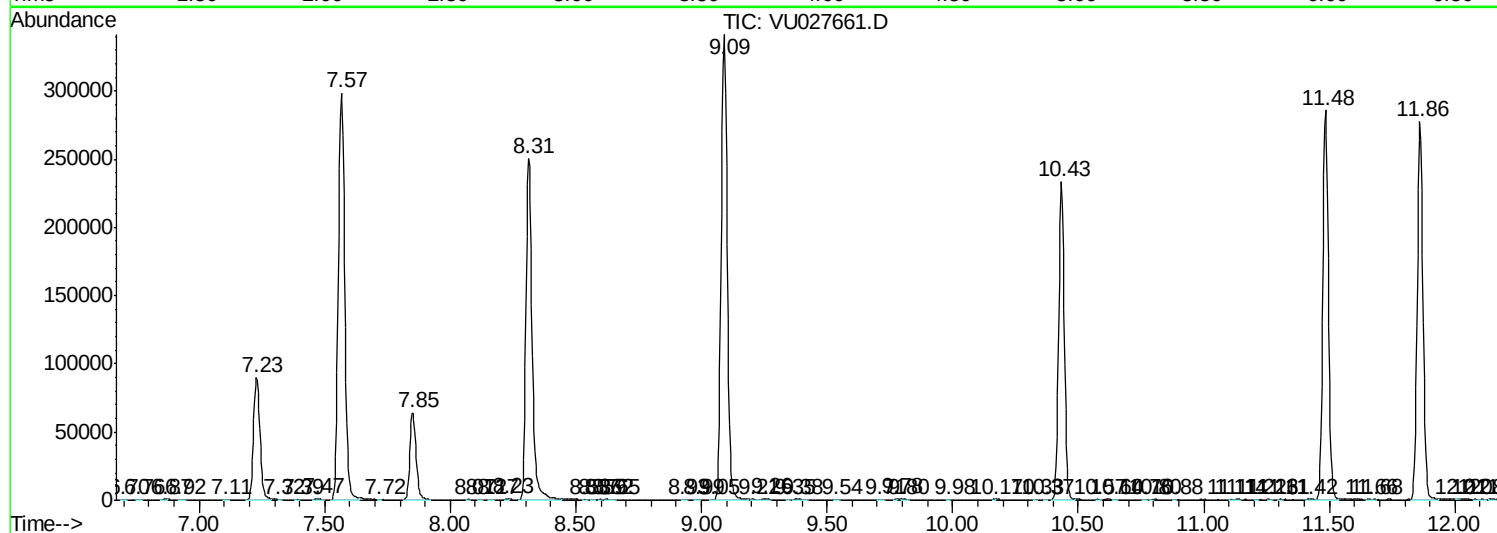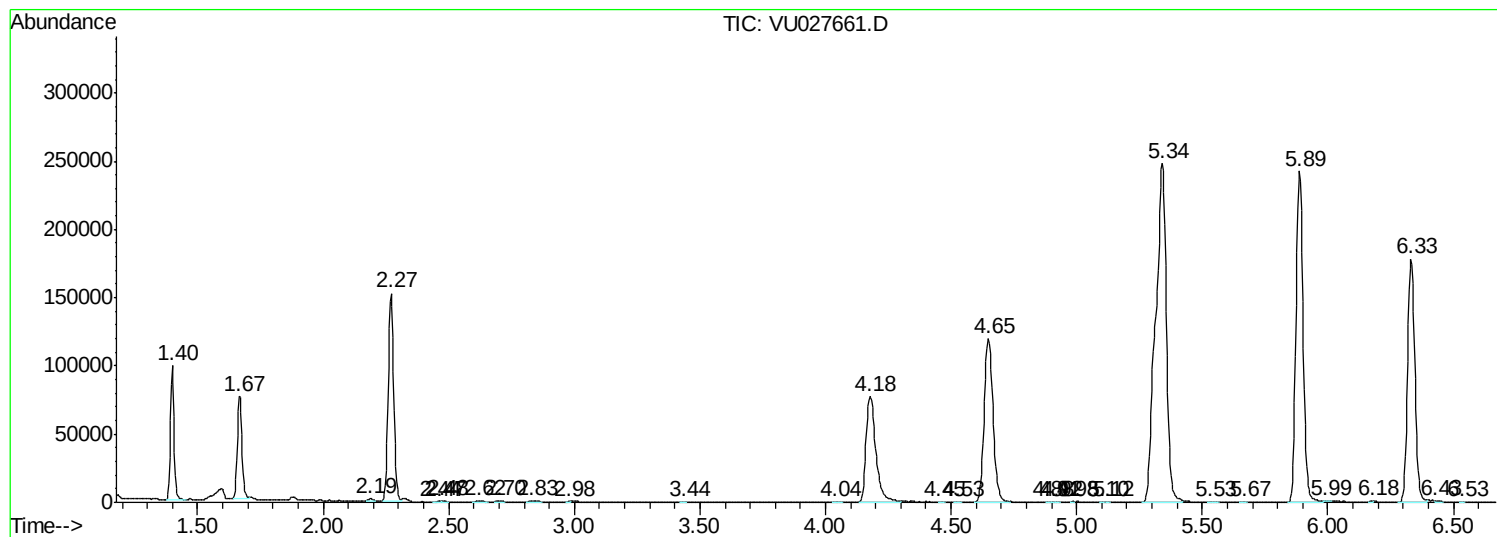

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101518\
Data File : VU027661.D
Acq On : 15 Oct 2018 12:51
Operator : MD/SY
Sample : J5403-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Title :

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101518\
Data File : VU027661.D
Acq On : 15 Oct 2018 12:51
Operator : MD/SY
Sample : J5403-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Title :

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc