


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101518\
 Data File : VU027651.D
 Acq On : 15 Oct 2018 07:42
 Operator : MD/SY
 Sample : BFB43
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB43

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis
 Last Update : Tue Oct 16 07:44:54 2018

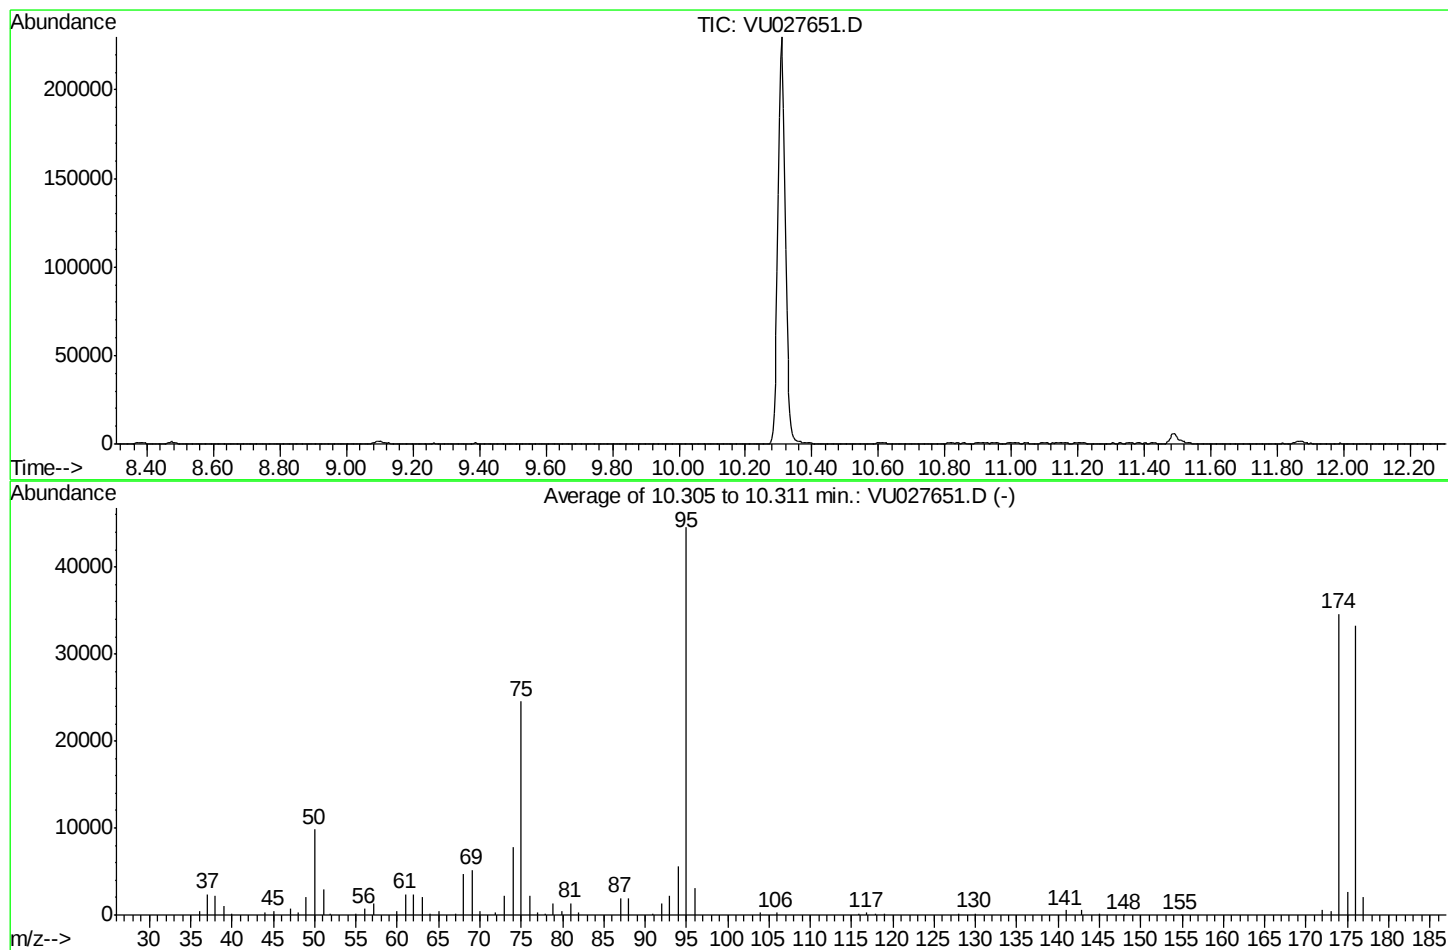

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	9830	PASS
75	95	30	80	55.1	24541	PASS
95	95	100	100	100.0	44576	PASS
96	95	5	9	7.0	3130	PASS
173	174	0.00	2	1.1	395	PASS
174	95	50	120	77.6	34594	PASS
175	174	5	9	7.8	2693	PASS
176	174	95	101	96.1	33232	PASS
177	176	5	9	6.2	2056	PASS

m/z	Abundance
43.90	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	439.0
37.10	2488.0
38.00	2272.0
39.00	1052.0
39.90	106.0
43.90	444.0
45.00	500.0
47.00	690.0
48.10	382.0
49.00	2005.0
50.00	9881.0
51.10	2872.0
52.00	162.0
55.00	101.0
56.00	698.0
57.10	1339.0
60.00	529.0
61.00	2347.0
62.00	2438.0
63.00	2016.0
64.00	219.0
65.00	533.0
67.10	122.0
68.00	4718.0
69.00	5032.0
70.00	414.0
71.90	235.0
73.00	2313.0
74.00	7765.0
75.00	23856.0
76.00	2144.0
77.00	301.0
77.90	195.0
78.90	1340.0
79.90	339.0
80.90	1299.0
82.00	262.0
87.00	1918.0
88.00	1772.0
91.00	189.0
92.00	1383.0
93.00	2110.0
94.00	5443.0
95.00	43888.0
96.00	3292.0
104.00	268.0
105.90	235.0
115.90	133.0
116.90	279.0
117.80	157.0
118.90	250.0
127.90	172.0
129.90	149.0
141.00	542.0
142.90	539.0
145.00	128.0
148.00	108.0
172.00	635.0
173.00	600.0
174.00	33056.0
175.00	2620.0
175.90	31464.0
177.00	1952.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	420.0
37.00	2429.0
38.00	2246.0
39.00	1079.0
39.90	128.0
43.90	476.0
45.00	502.0
47.00	735.0
48.10	342.0
49.00	2089.0
50.00	10156.0
51.10	3067.0
52.00	142.0
55.00	110.0
56.00	711.0
57.10	1346.0
60.00	520.0
61.00	2493.0
62.00	2476.0
63.00	2095.0
64.00	218.0
65.00	520.0
67.10	134.0
68.00	4941.0
69.00	5358.0
70.00	432.0
71.90	266.0
73.00	2336.0
74.00	8023.0
75.00	25480.0
76.00	2322.0
77.10	327.0
77.90	216.0
78.90	1324.0
79.90	385.0
80.90	1406.0
81.90	296.0
87.00	2053.0
88.00	1906.0
91.00	170.0
92.00	1373.0
93.00	2301.0
94.00	5823.0
95.00	45984.0
96.00	3235.0
104.00	235.0
105.90	246.0
115.90	154.0
116.80	307.0
117.80	149.0
118.90	224.0
127.90	172.0
129.90	178.0
141.00	557.0
142.90	549.0
145.00	126.0
154.90	107.0
171.90	649.0
173.00	587.0
174.00	35872.0
175.00	2776.0
176.00	34464.0
177.00	2103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	372.0
37.00	2212.0
38.00	2107.0
39.00	982.0
39.90	120.0
43.90	446.0
45.00	464.0
47.00	654.0
48.00	263.0
49.00	1998.0
50.00	9453.0
51.10	2952.0
51.90	122.0
55.00	123.0
56.00	681.0
57.10	1199.0
60.00	487.0
61.00	2392.0
62.00	2243.0
63.00	1970.0
64.00	198.0
65.10	488.0
66.90	148.0
68.00	4705.0
69.00	5118.0
70.00	399.0
71.90	228.0
73.00	2144.0
74.00	7553.0
75.00	24288.0
76.00	2195.0
77.10	283.0
77.90	207.0
78.90	1223.0
79.90	412.0
81.00	1366.0
81.90	297.0
87.00	1958.0
88.00	1942.0
90.90	147.0
92.00	1257.0
93.00	2253.0
94.00	5442.0
95.00	43856.0
96.00	2864.0
103.90	194.0
105.90	227.0
115.90	170.0
116.90	289.0
117.90	115.0
118.90	191.0
127.90	135.0
129.90	164.0
140.90	519.0
142.90	490.0
145.00	113.0
154.90	117.0
171.90	566.0
174.00	34856.0
175.00	2683.0
176.00	33768.0
177.00	2113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43