

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U101519\
 Data File : VU035189.D
 Acq On : 15 Oct 2019 13:58
 Operator : JC/SP
 Sample : K5317-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CF6

Quant Time: Oct 15 16:24:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 15 15:10:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.87	114	157857	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	163156	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	59375	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	42786	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.67	69	42631	4.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.80%
11) 1,1-Dichloroethene-d2	2.26	63	63805	3.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.80%
20) 2-Butanone-d5	4.18	46	148798	54.15	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.30%
24) Chloroform-d	4.63	84	92255	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.80%
26) 1,2-Dichloroethane-d4	5.29	65	52577	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	5.32	84	172832	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.31	67	64787	5.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.40%
41) Toluene-d8	7.55	98	140138	3.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.80%
43) trans-1,3-Dichloropropene-	7.84	79	19707	4.28	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.60%
46) 2-Hexanone-d5	8.30	63	100979	46.13	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.26%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	56035	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.00%
64) 1,2-Dichlorobenzene-d4	11.84	152	49300	4.92	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.40%


Target Compounds					Ovalue
13) Acetone	2.32	43	7140	3.172 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101519\
Data File : VU035189.D
Acq On : 15 Oct 2019 13:58
Operator : JC/SP
Sample : K5317-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF6

Quant Time: Oct 15 16:24:09 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 15 15:10:16 2019
Response via : Initial Calibration

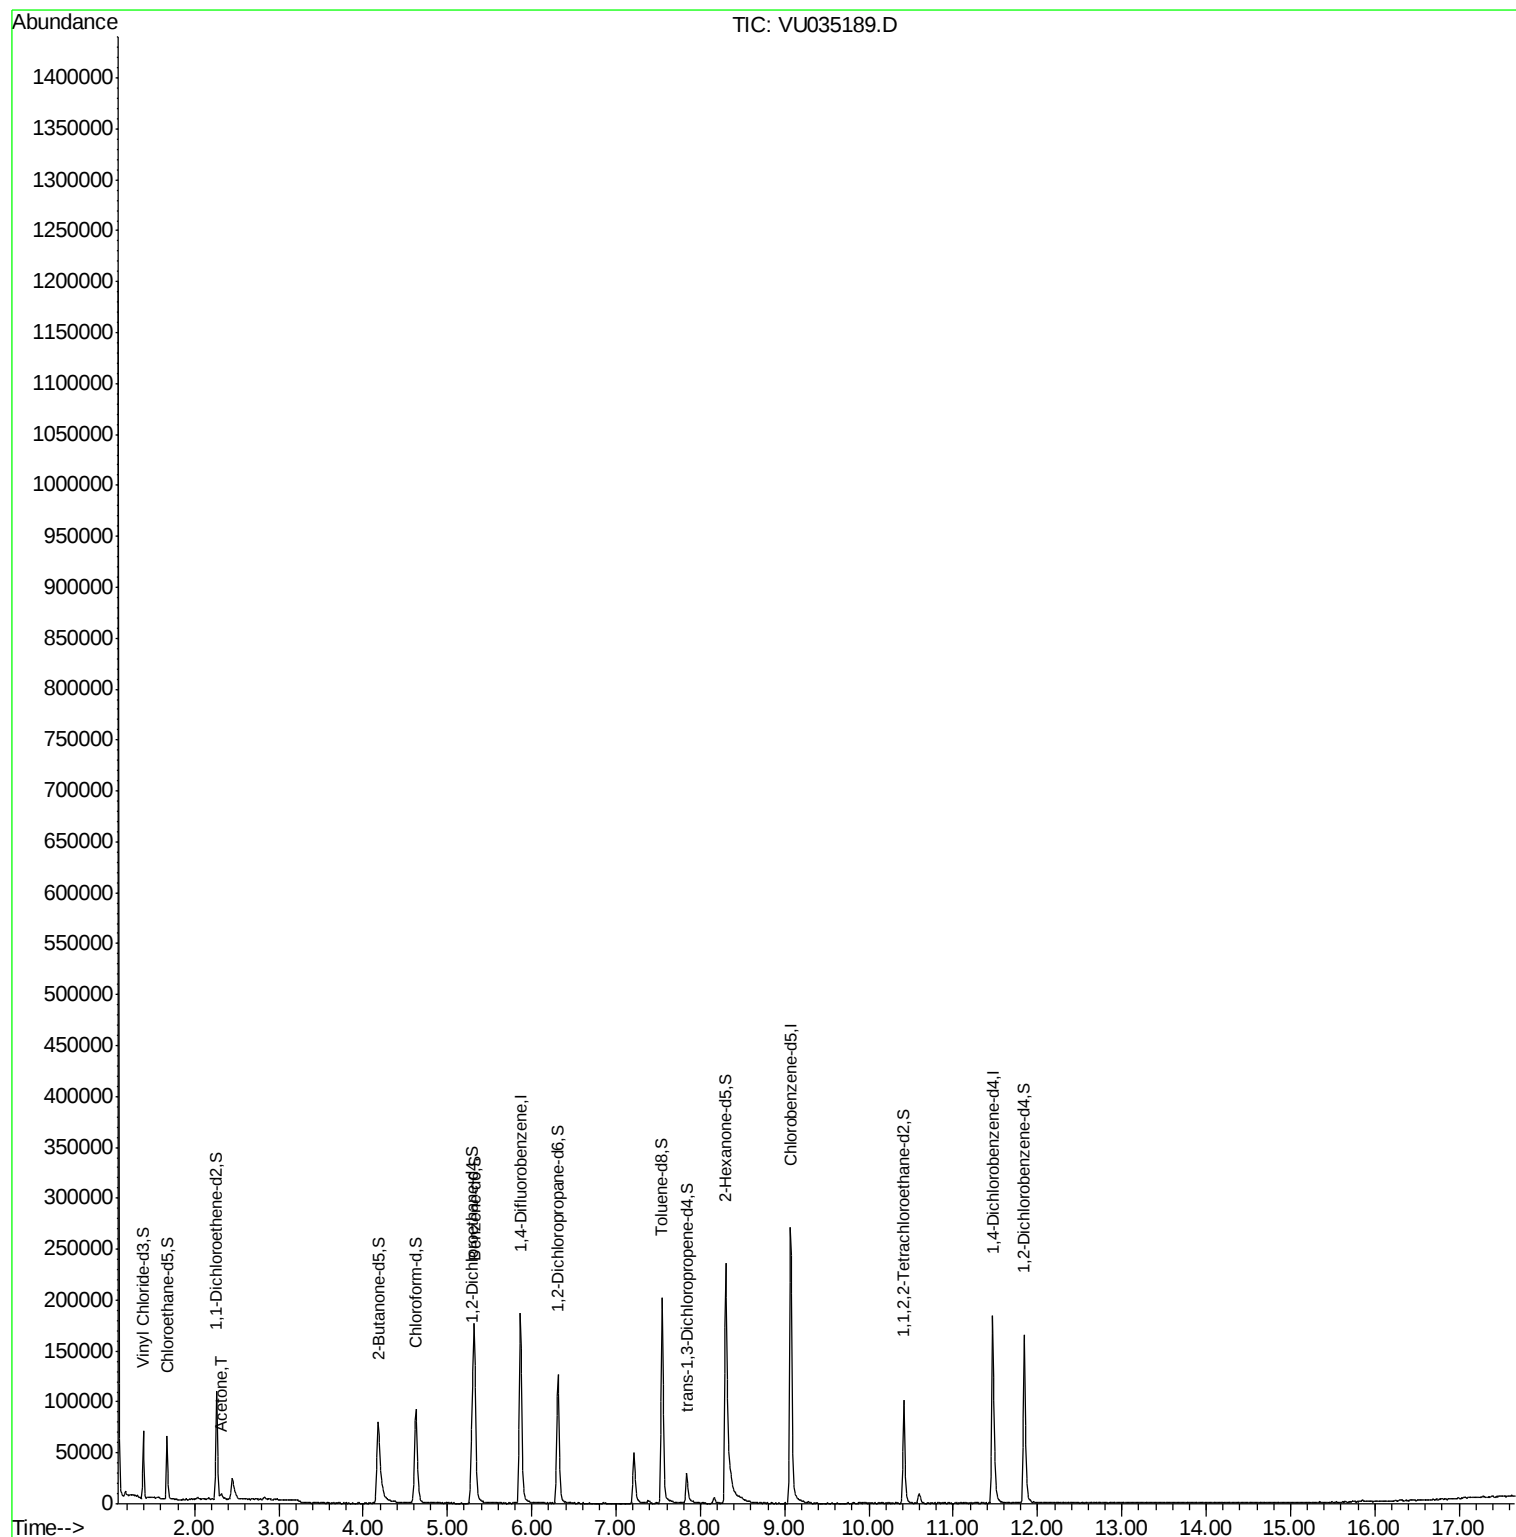

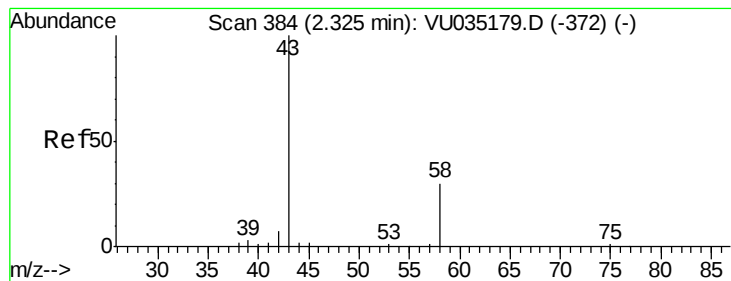

#13
 Acetone
 Concen: 3.172 ug/L
 RT: 2.32 min Scan# 382
 Delta R.T. 0.01 min
 Lab File: VU035189.D
 Acq: 15 Oct 2019 13:58

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CF6

Tot Ion: 43 Resp: 7140
 Ion Ratio Lower Upper
 43 100
 58 25.2 0.0 66.6

