

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101519\
 Data File : VU035191.D
 Acq On : 15 Oct 2019 14:46
 Operator : JC/SP
 Sample : K5317-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CF8

Quant Time: Oct 15 16:28:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 15 15:10:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	144760	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	153251	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	56672	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	41773	4.88	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.60%
7) Chloroethane-d5	1.68	69	40062	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.40%
11) 1,1-Dichloroethene-d2	2.26	63	59761	3.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.20%
20) 2-Butanone-d5	4.18	46	150719	59.81	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.62%
24) Chloroform-d	4.63	84	86407	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.00%
26) 1,2-Dichloroethane-d4	5.29	65	50266	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.00%
32) Benzene-d6	5.32	84	161271	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
36) 1,2-Dichloropropane-d6	6.31	67	61357	5.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.20%
41) Toluene-d8	7.55	98	132478	3.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.20%
43) trans-1,3-Dichloropropene-	7.84	79	18777	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.31	63	94184	45.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.60%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	52877	5.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.40%
64) 1,2-Dichlorobenzene-d4	11.84	152	47700	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%


Target Compounds					Ovalue
13) Acetone	2.33	43	6666	3.230 ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101519\
Data File : VU035191.D
Acq On : 15 Oct 2019 14:46
Operator : JC/SP
Sample : K5317-15
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CF8

Quant Time: Oct 15 16:28:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 15 15:10:16 2019
Response via : Initial Calibration

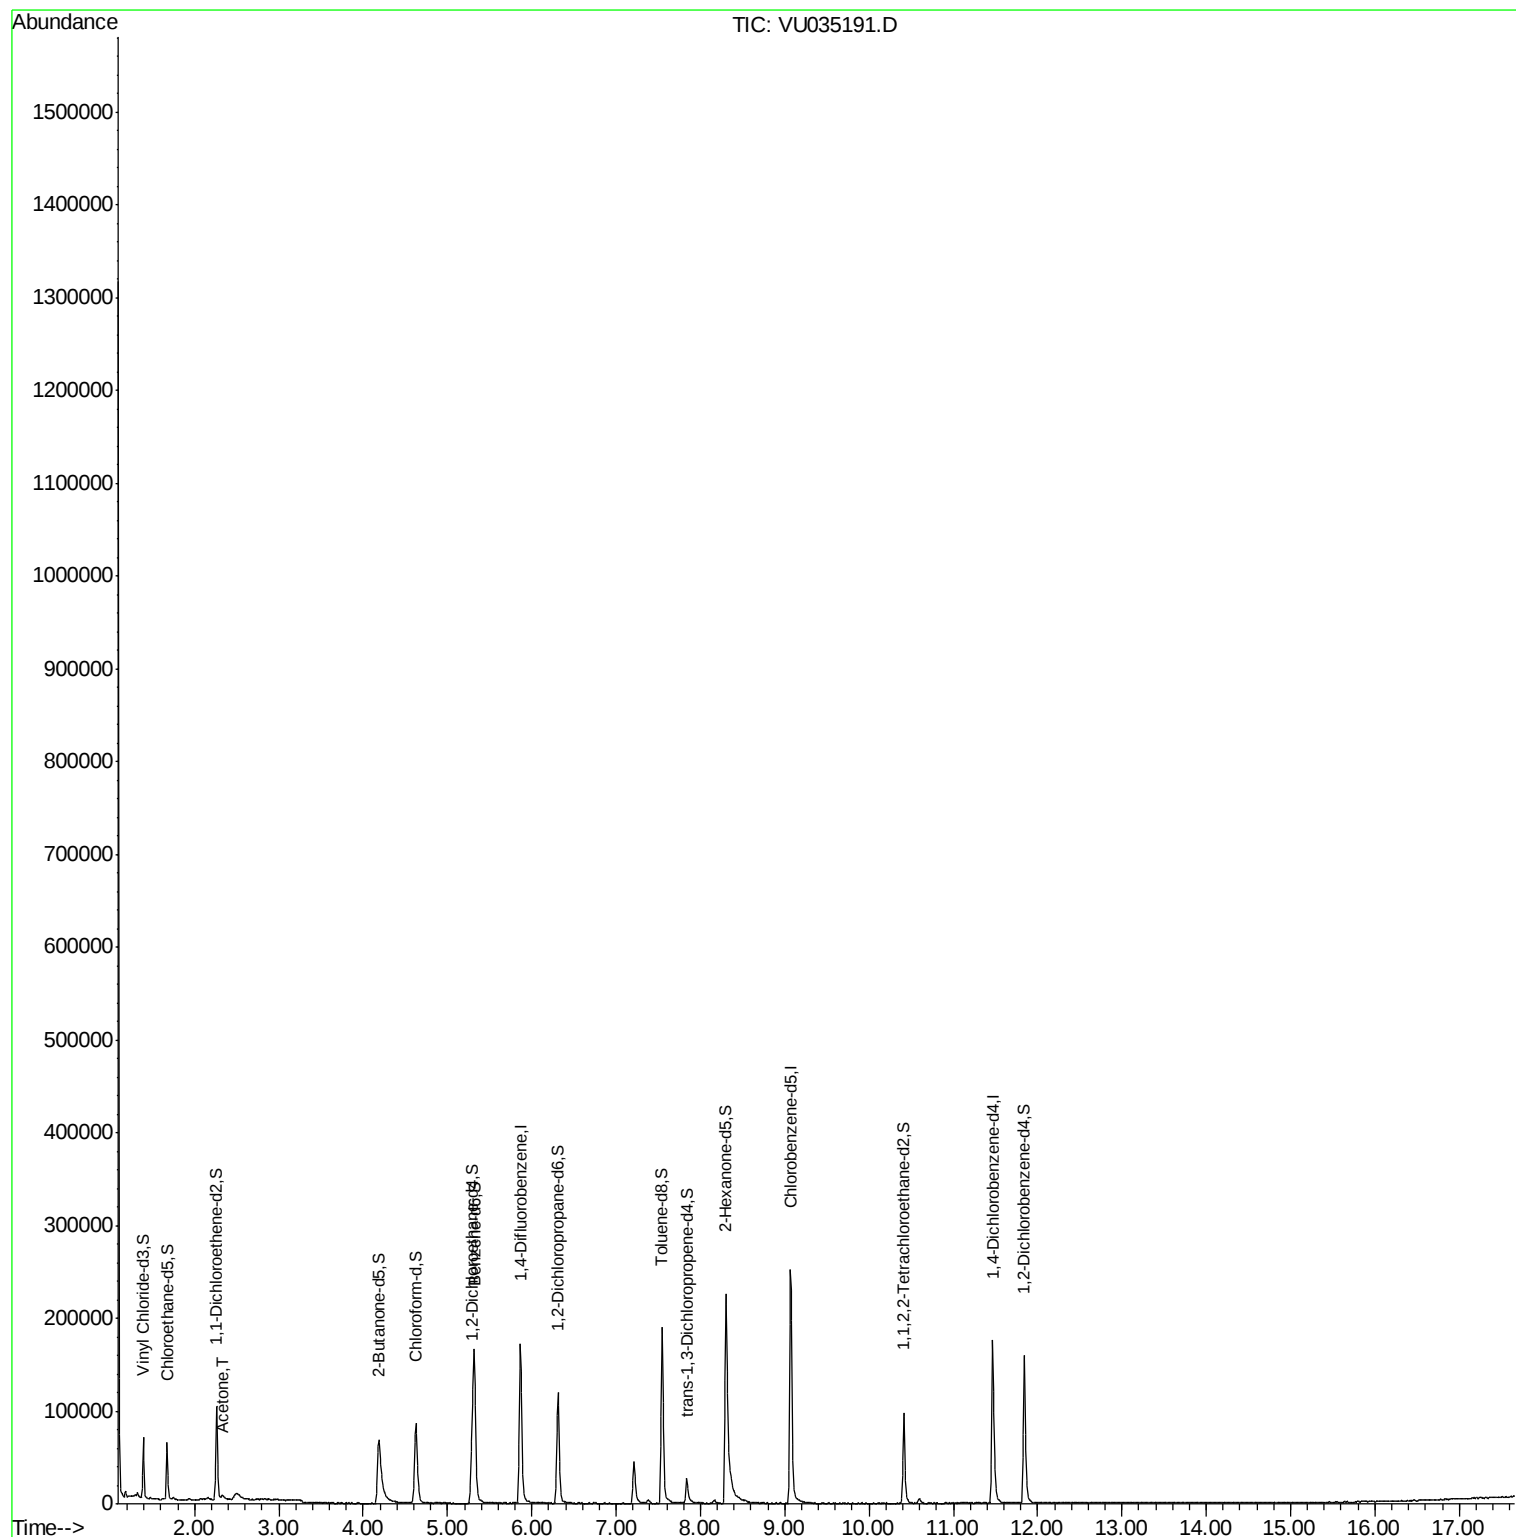

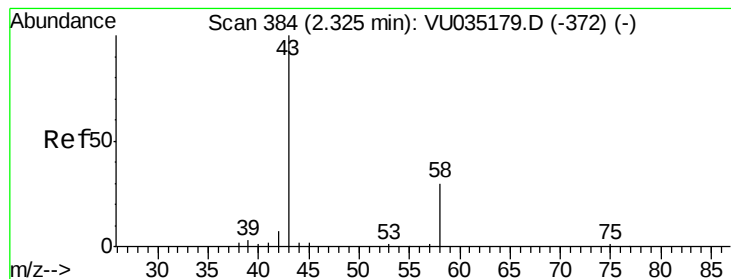

#13
 Acetone
 Concen: 3.230 ug/L
 RT: 2.33 min Scan# 386
 Delta R.T. 0.02 min
 Lab File: VU035191.D
 Acq: 15 Oct 2019 14:46

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CF8

Tot Ion: 43 Resp: 6666
 Ion Ratio Lower Upper
 43 100
 58 20.6 0.0 66.6

