


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101519\
Data File : VU035178.D
Acq On : 15 Oct 2019 08:26
Operator : JC/SP
Sample : BFB20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB20

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Oct 17 11:17:21 2019

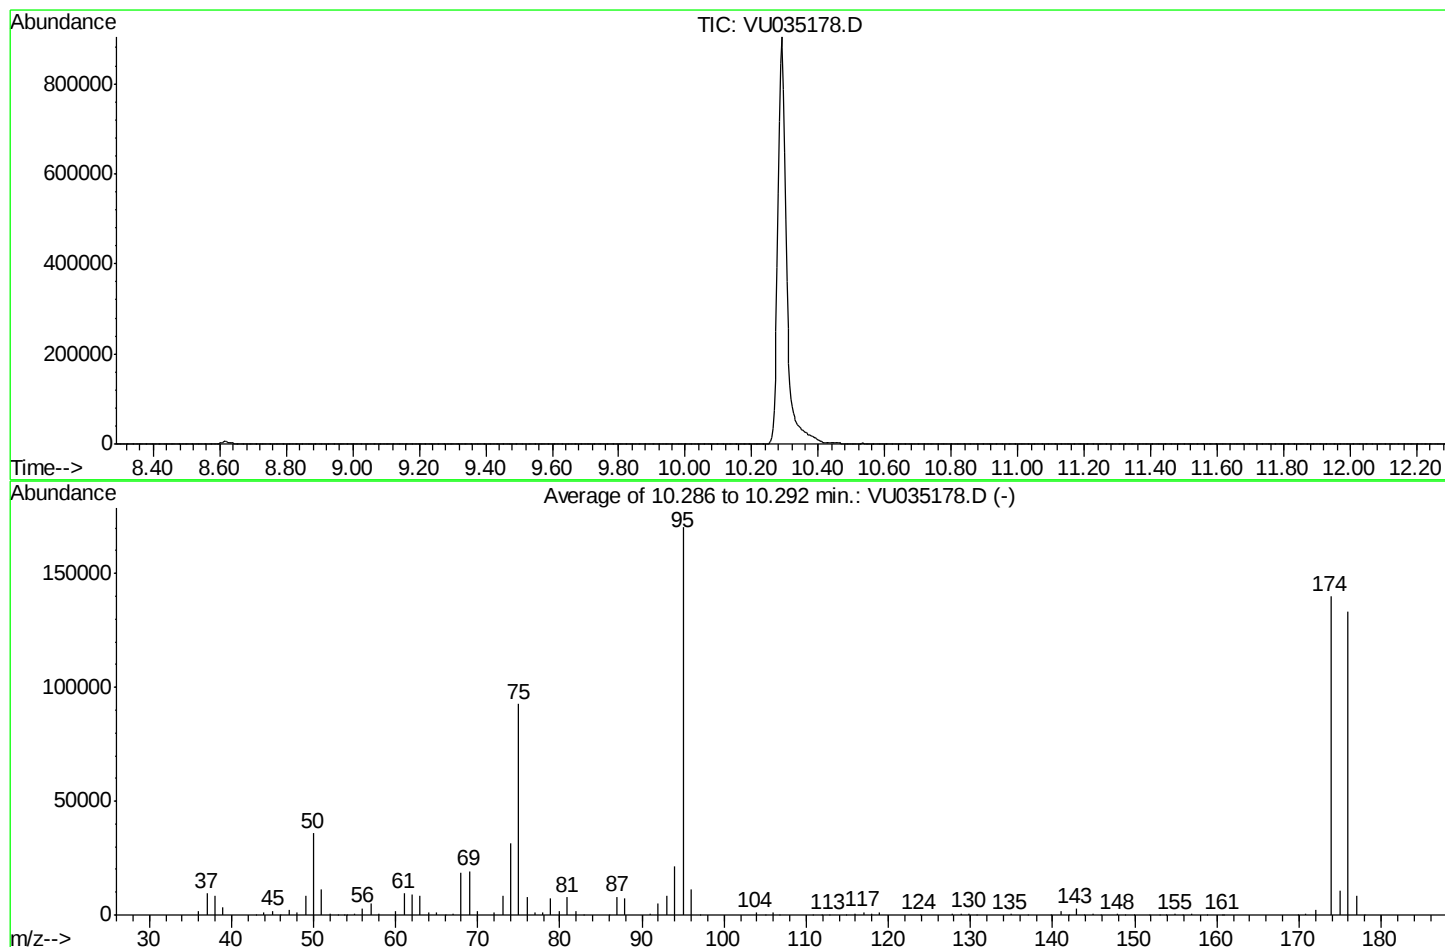

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	35973	PASS
75	95	30	80	54.4	92544	PASS
95	95	100	100	100.0	170240	PASS
96	95	5	9	6.5	11020	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.2	139861	PASS
175	174	5	9	7.5	10493	PASS
176	174	95	101	95.3	133306	PASS
177	176	5	9	6.4	8571	PASS

m/z	Abundance
36.00	1655.0
37.00	9315.0
38.00	8394.0
39.00	3195.0
40.00	455.0
43.00	132.0
44.00	1502.0
45.10	1799.0
46.00	200.0
47.00	2287.0
47.90	1092.0
49.00	8256.0
50.00	35552.0
51.00	11090.0
52.00	582.0
53.00	233.0
53.80	153.0
55.00	635.0
56.00	2964.0
57.00	5086.0
58.00	303.0
60.00	1829.0
61.00	9012.0
62.00	8994.0
63.00	7874.0
64.00	1210.0
65.00	1229.0
66.10	204.0
67.00	526.0
68.00	18416.0
69.00	18896.0
70.00	1491.0
72.00	946.0
73.00	8452.0
74.00	30688.0
75.00	88880.0
76.00	7784.0
77.00	1166.0
78.00	917.0
78.90	7462.0
80.00	1996.0
80.90	7491.0
81.90	1810.0
82.90	215.0
86.00	239.0
87.00	7834.0
87.90	7249.0
91.00	804.0
92.00	5095.0
93.00	8232.0
94.00	20920.0
95.00	164352.0
96.00	10692.0
97.00	325.0
103.90	895.0
105.00	271.0
105.90	841.0
106.70	249.0
110.80	101.0
111.80	111.0
112.80	158.0
114.80	196.0
115.90	670.0
117.00	1285.0
117.90	673.0
118.90	1296.0
123.90	125.0
127.80	517.0
128.90	320.0
129.80	630.0
130.80	228.0
134.90	346.0
136.90	274.0
139.80	171.0
141.00	1646.0
141.90	222.0
142.90	2541.0
143.90	109.0
144.90	559.0
145.90	291.0
147.90	507.0
148.90	148.0
149.90	156.0
153.00	124.0
153.80	112.0
155.00	364.0
156.90	248.0
158.90	190.0
160.70	180.0
170.80	263.0
172.00	2278.0
173.90	131584.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

175.00	10069.0
175.90	126128.0
177.00	8077.0
177.90	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

m/z	Abundance
36.00	1700.0
37.00	9644.0
38.00	8505.0
39.00	3451.0
40.00	406.0
44.00	1476.0
45.10	1878.0
45.90	223.0
47.00	2353.0
47.90	1219.0
49.00	8855.0
50.00	37104.0
51.00	11830.0
52.00	629.0
53.00	216.0
53.80	142.0
55.00	645.0
56.00	2996.0
57.00	5440.0
58.00	364.0
60.00	1909.0
61.00	9597.0
62.00	9426.0
63.00	8547.0
64.00	1080.0
65.00	1299.0
66.10	224.0
67.00	515.0
68.00	19416.0
69.00	19864.0
70.00	1500.0
72.00	983.0
73.00	8989.0
74.00	32680.0
75.00	95848.0
76.00	8363.0
77.00	1215.0
78.00	919.0
78.90	7800.0
79.90	1979.0
80.90	7989.0
81.90	1816.0
82.90	206.0
85.90	315.0
87.00	8278.0
87.90	7487.0
91.00	803.0
92.00	5531.0
93.00	9051.0
94.00	22240.0
95.00	175424.0
96.00	11429.0
97.00	318.0
103.90	992.0
105.00	259.0
105.90	875.0
106.80	227.0
110.80	134.0
111.90	168.0
112.80	199.0
114.80	226.0
115.90	712.0
116.90	1337.0
117.90	783.0
118.90	1217.0
123.90	145.0
127.80	620.0
128.90	335.0
129.90	729.0
130.80	265.0
134.90	372.0
136.90	305.0
139.80	191.0
141.00	1745.0
141.90	253.0
142.90	2636.0
144.90	546.0
145.90	282.0
147.90	509.0
148.90	165.0
149.80	212.0
151.80	102.0
155.00	393.0
155.80	104.0
156.90	316.0
158.90	213.0
160.70	168.0
169.90	101.0
170.90	343.0
172.00	2328.0
173.90	144192.0
175.00	10743.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

175.90137280.0

177.008827.0

177.90180.0

Instrument :
MSVOA_U

ClientSampleId :
BFB20

m/z	Abundance
36.00	1681.0
37.00	9101.0
38.00	8152.0
39.00	3586.0
40.00	362.0
44.00	1429.0
45.00	1621.0
45.90	215.0
47.00	2231.0
48.00	1206.0
49.00	8469.0
50.00	35264.0
51.00	11288.0
52.00	568.0
53.00	153.0
54.00	105.0
55.00	586.0
56.00	2758.0
57.00	5244.0
58.00	332.0
60.00	1886.0
61.00	9376.0
62.00	9177.0
63.00	8226.0
64.00	956.0
65.00	1447.0
66.10	196.0
67.00	447.0
68.00	18248.0
69.00	19016.0
70.00	1362.0
72.00	952.0
73.00	8735.0
74.00	31792.0
75.00	92904.0
76.00	8068.0
77.00	1179.0
77.90	788.0
78.90	7485.0
79.90	1898.0
80.90	7736.0
81.90	1664.0
82.90	220.0
85.90	335.0
87.00	8066.0
87.90	6899.0
90.90	741.0
92.00	5387.0
93.00	8802.0
94.00	21424.0
95.00	170944.0
96.00	10940.0
97.10	244.0
103.90	984.0
104.90	248.0
105.90	876.0
106.80	179.0
110.80	152.0
111.90	174.0
112.80	184.0
114.80	227.0
115.90	724.0
116.90	1237.0
117.90	745.0
118.90	1087.0
123.80	127.0
127.80	635.0
128.80	323.0
129.90	710.0
130.80	278.0
134.90	355.0
136.90	273.0
139.80	183.0
141.00	1659.0
141.90	255.0
142.90	2496.0
144.80	495.0
145.90	313.0
147.90	439.0
148.80	160.0
149.80	223.0
154.90	415.0
156.90	381.0
158.80	255.0
160.90	195.0
169.90	126.0
170.90	377.0
172.00	2173.0
173.90	143808.0
175.00	10668.0
175.90	136512.0
177.00	8809.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

178.00

162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20

Scan 2847 (10.244 min): VU035178.D
BFB20

m/z	Abundance
39.90	607.0
43.90	457.0

Instrument :
MSVOA_U
ClientSampleId :
BFB20