


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101520\
Data File : VU040716.D
Acq On : 15 Oct 2020 13:36
Operator : SY/MD
Sample : L4401-01DL 2X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFSC1DL

Manual Integrations
APPROVED

apatel
10/19/2020 2:37:17 PM

Quant Time: Oct 16 04:57:10 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 16 04:23:22 2020
Response via : Initial Calibration

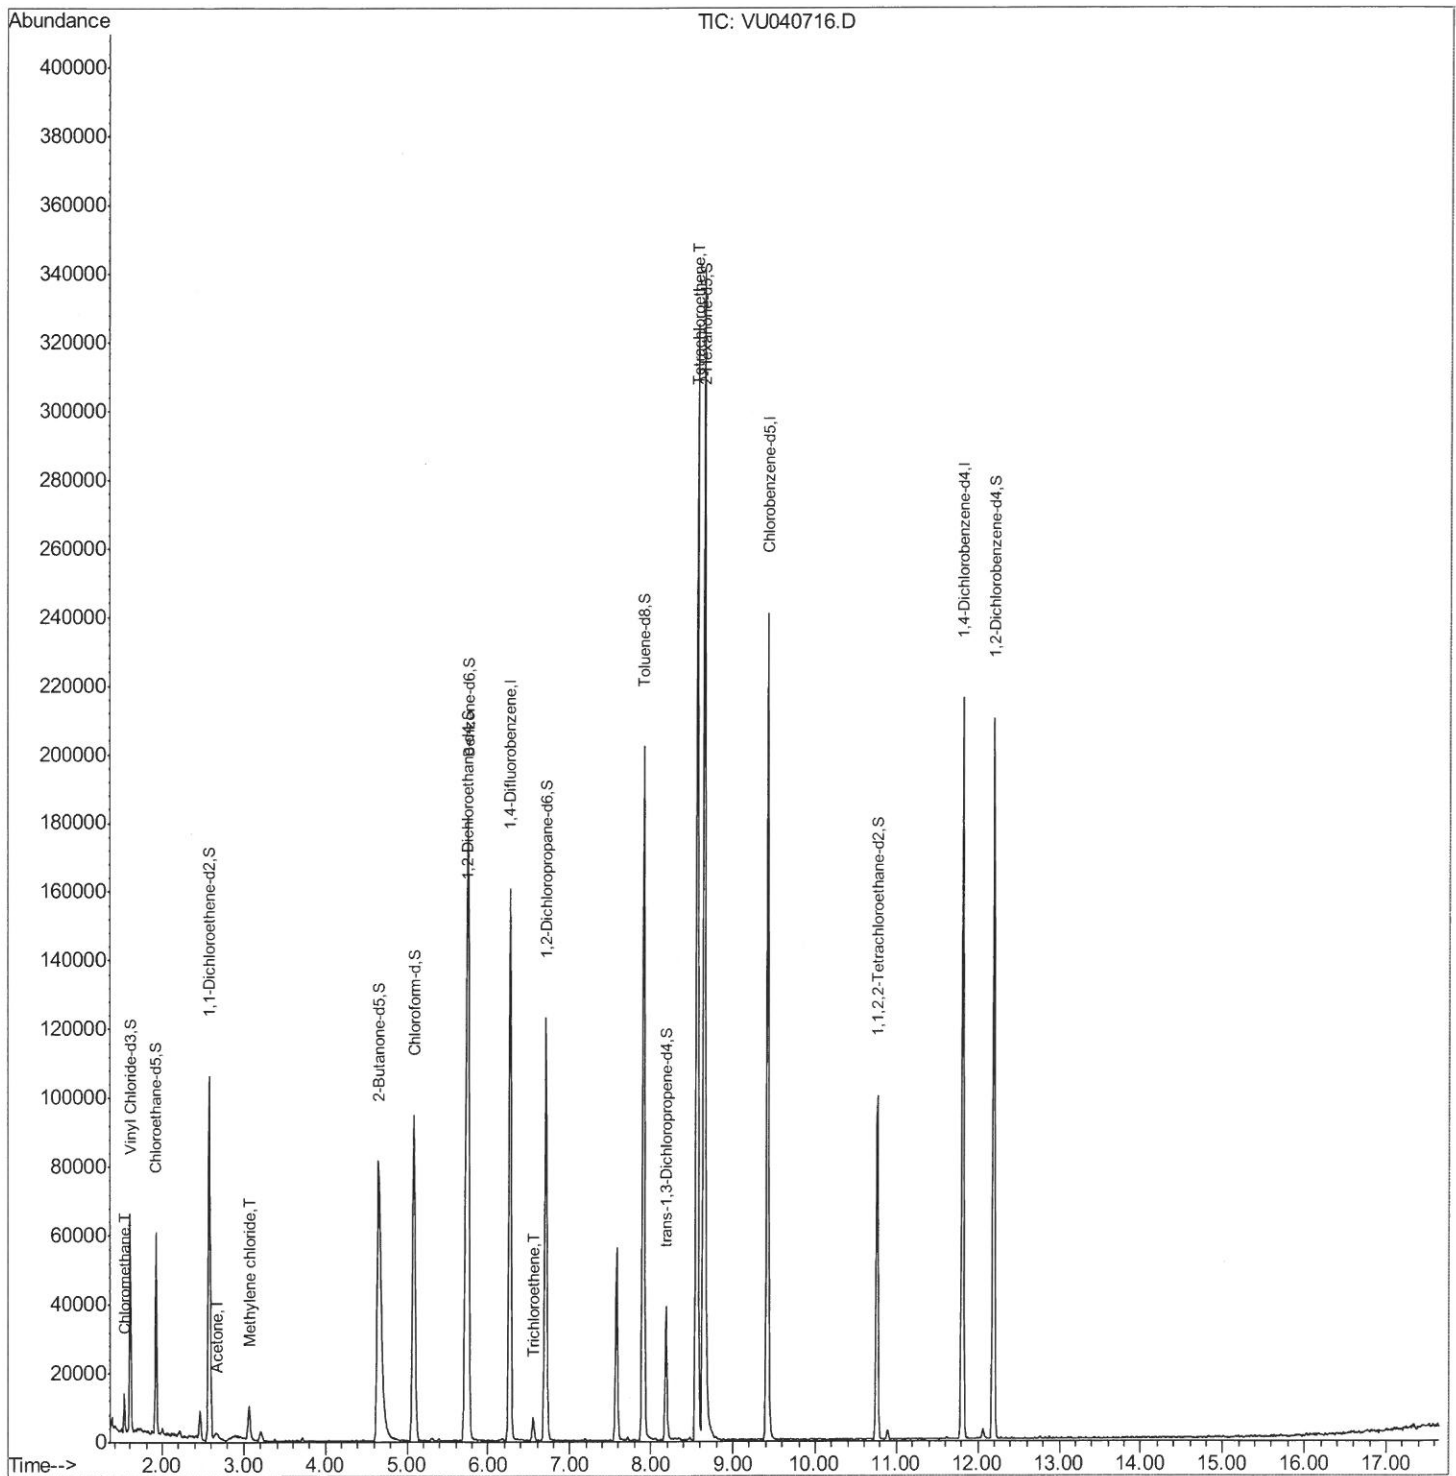

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101520\
Data File : VU040716.D
Acq On : 15 Oct 2020 13:36
Operator : SY/MD
Sample : L4401-01DL 2X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFSC1DL

Manual Integrations
APPROVED

apatel
10/19/2020 2:37:17 PM

Quant Time: Oct 16 04:31:54 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 16 04:23:22 2020
Response via : Initial Calibration

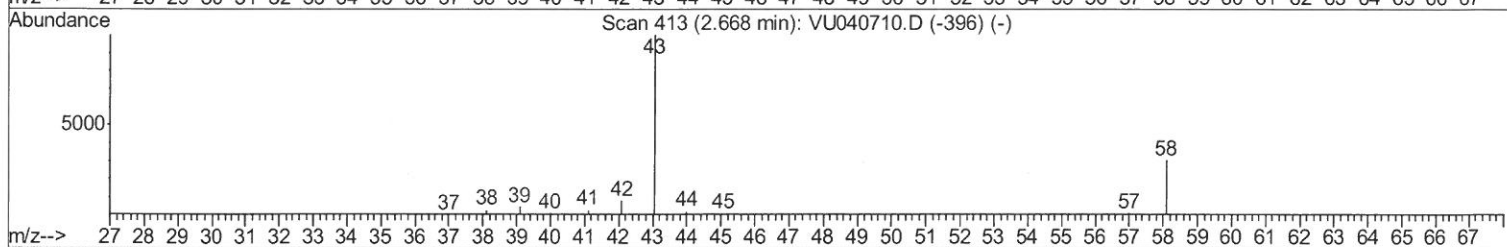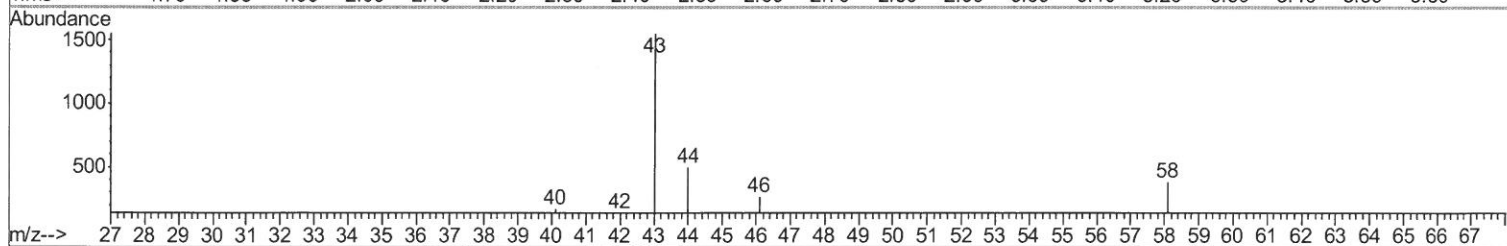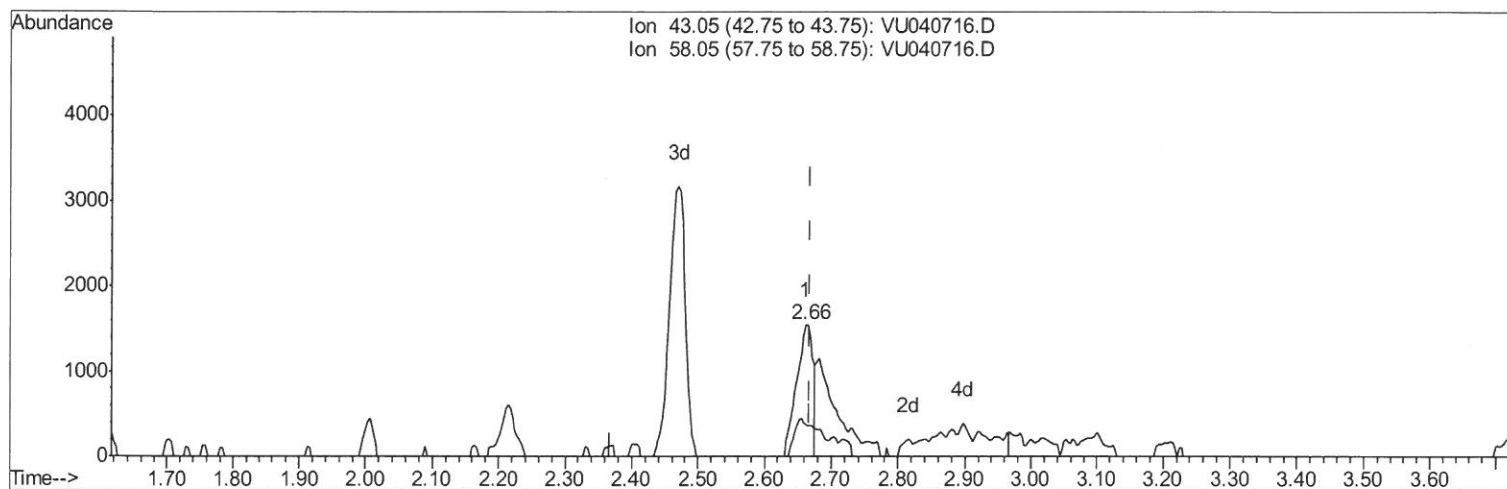

TIC: VU040716.D

(13) Acetone (T)

2.662min (-0.007) 1.07ug/L

response 2625

Ion	Exp%	Act%
43.05	100	100
58.05	30.30	41.37
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101520\
 Data File : VU040716.D
 Acq On : 15 Oct 2020 13:36
 Operator : SY/MD
 Sample : L4401-01DL 2X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFSC1DL

Manual Integrations
 APPROVED

apatel
 10/19/2020 2:37:17 PM

Quant Time: Oct 16 04:31:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 16 04:23:22 2020
 Response via : Initial Calibration

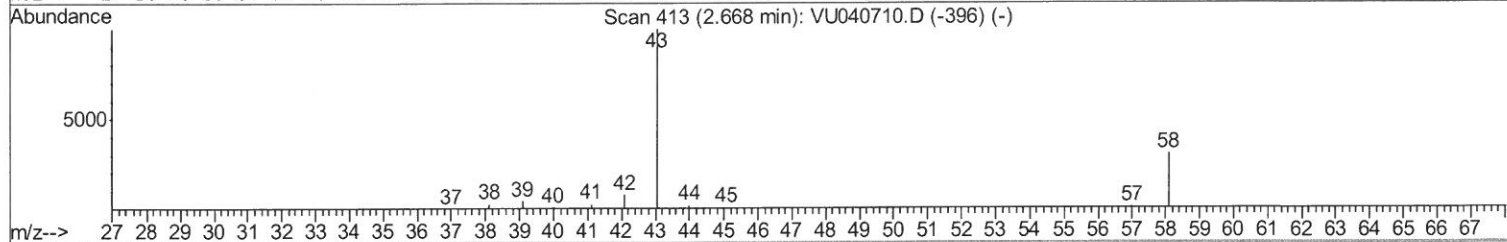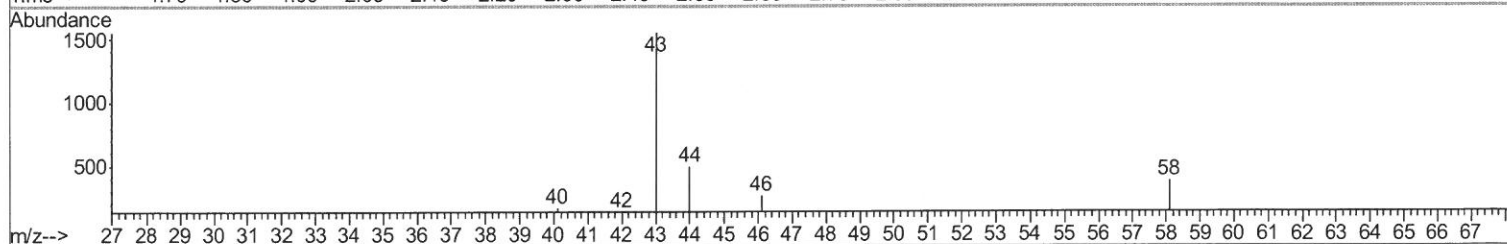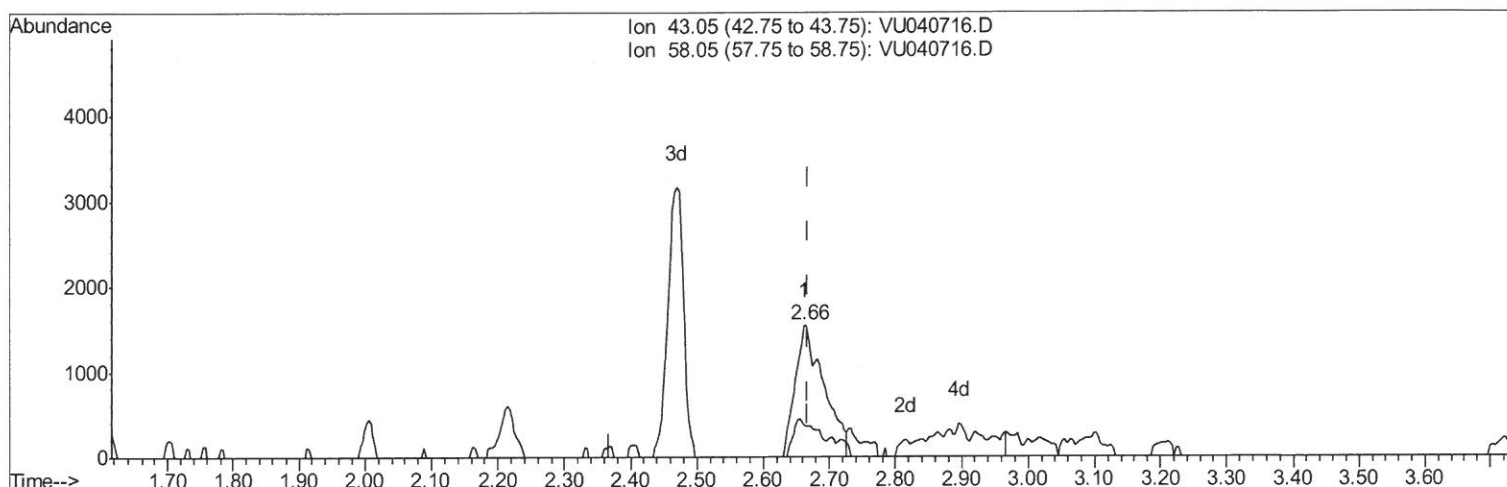

(13) Acetone (T)

2.662min (-0.007) 1.92ug/L m

response 4705

Ion Exp% Act%

43.05 100 100

58.05 30.30 23.08

0.00 0.00 0.00

0.00 0.00 0.00

MD
10/19/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101520\
 Data File : VU040716.D
 Acq On : 15 Oct 2020 13:36
 Operator : SY/MD
 Sample : L4401-01DL 2X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFSC1DL

Manual Integrations
 APPROVED

apatel
 10/19/2020 2:37:17 PM

Quant Time: Oct 16 04:57:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 16 04:23:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	119252	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	125203	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	53490	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	41148	4.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.20%
7) Chloroethane-d5	1.92	69	37523	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.40%
11) 1,1-Dichloroethene-d2	2.58	63	65558	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	4.65	46	160713	50.83	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.66%
24) Chloroform-d	5.08	84	85835	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.72	65	51984	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
32) Benzene-d6	5.74	84	155234	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
36) 1,2-Dichloropropane-d6	6.70	67	54892	4.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.00%
41) Toluene-d8	7.91	98	125451	4.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.00%
43) trans-1,3-Dichloropropene-	8.19	79	20560	4.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.60%
46) 2-Hexanone-d5	8.64	63	114581	46.82	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.64%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	47348	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	50797	5.12	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.40%

Target Compounds

					Ovalue
3) Chloromethane	1.53	50	7286	0.721	ug/L 98
13) Acetone	2.66	43	4705m	1.920	ug/L
16) Methylene chloride	3.06	84	3941	0.361	ug/L 94
34) Trichloroethene	6.55	95	2159	0.207	ug/L 91
47) Tetrachloroethene	8.56	164	68536	9.213	ug/L 96

7 mg
 10/19/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed