

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101520\  
 Data File : VU040711.D  
 Acq On : 15 Oct 2020 11:22  
 Operator : SY/MD  
 Sample : VU1015WBL01  
 Misc : 25.0mL/MSVOA U/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VBLK29

Quant Time: Oct 16 04:37:21 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Fri Oct 16 04:23:22 2020  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Difluorobenzene     | 6.26  | 114  | 117778   | 5.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 9.42  | 117  | 124559   | 5.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 11.81 | 152  | 49848    | 5.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                                |        |       |          |          |      |         |
|--------------------------------|--------|-------|----------|----------|------|---------|
| 4) Vinyl Chloride-d3           | 1.60   | 65    | 46299    | 4.74     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 40 - 130 | Recovery | =    | 94.80%  |
| 7) Chloroethane-d5             | 1.92   | 69    | 40741    | 5.41     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 130 | Recovery | =    | 108.20% |
| 11) 1,1-Dichloroethene-d2      | 2.58   | 63    | 72927    | 3.82     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 125 | Recovery | =    | 76.40%  |
| 20) 2-Butanone-d5              | 4.66   | 46    | 171151   | 54.80    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 40 - 130 | Recovery | =    | 109.60% |
| 24) Chloroform-d               | 5.08   | 84    | 90630    | 5.29     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 105.80% |
| 26) 1,2-Dichloroethane-d4      | 5.72   | 65    | 56718    | 5.44     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 108.80% |
| 32) Benzene-d6                 | 5.74   | 84    | 169565   | 5.05     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 101.00% |
| 36) 1,2-Dichloropropane-d6     | 6.70   | 67    | 59374    | 5.32     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 140 | Recovery | =    | 106.40% |
| 41) Toluene-d8                 | 7.91   | 98    | 134911   | 4.48     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 89.60%  |
| 43) trans-1,3-Dichloropropene- | 8.19   | 79    | 21910    | 4.64     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 55 - 130 | Recovery | =    | 92.80%  |
| 46) 2-Hexanone-d5              | 8.64   | 63    | 114939   | 47.21    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 45 - 130 | Recovery | =    | 94.42%  |
| 57) 1,1,2,2-Tetrachloroethane- | 10.76  | 84    | 48608    | 4.86     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 120 | Recovery | =    | 97.20%  |
| 64) 1,2-Dichlorobenzene-d4     | 12.19  | 152   | 52224    | 5.65     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 80 - 120 | Recovery | =    | 113.00% |


| Target Compounds       |      |    |      |            | Ovalue |
|------------------------|------|----|------|------------|--------|
| 16) Methylene chloride | 3.06 | 84 | 1705 | 0.158 ug/L | 87     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101520\  
Data File : VU040711.D  
Acq On : 15 Oct 2020 11:22  
Operator : SY/MD  
Sample : VU1015WBL01  
Misc : 25.0mL/MSVOA U/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
VBLK29

Quant Time: Oct 16 04:37:21 2020  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Fri Oct 16 04:23:22 2020  
Response via : Initial Calibration

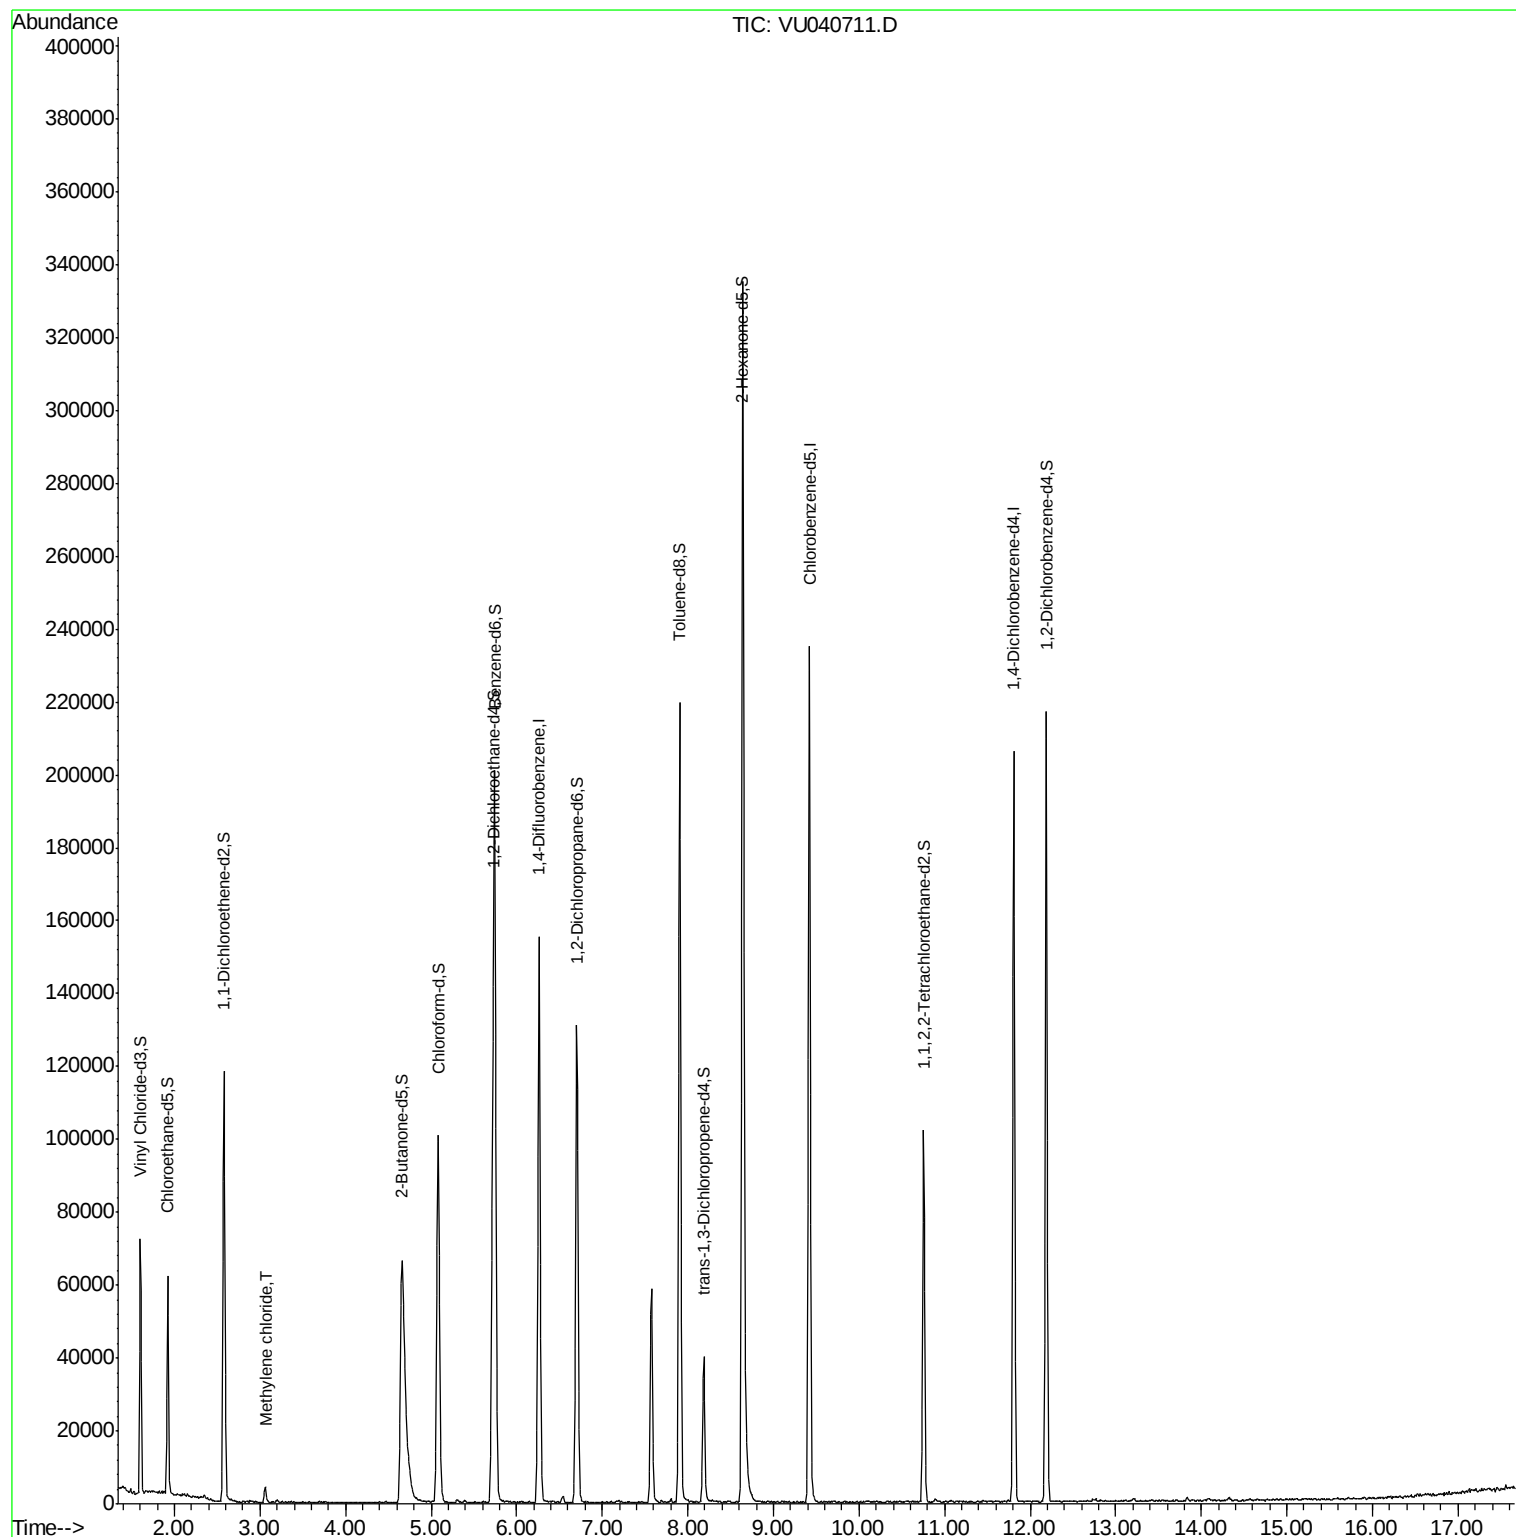

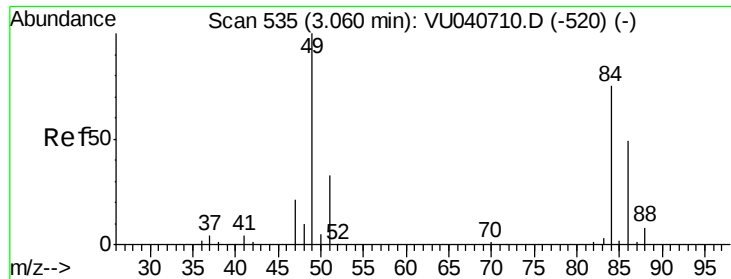

#16  
 Methvlene chloride  
 Concen: 0.158 ug/L  
 RT: 3.06 min Scan# 536  
 Delta R.T. 0.00 min  
 Lab File: VU040711.D  
 Acq: 15 Oct 2020 11:22

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 VBLK29

Tot Ion: 84 Resp: 1705  
 Ion Ratio Lower Upper  
 84 100  
 86 55.6 45.4 84.4  
 49 125.2 99.8 185.3

