

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U101520\
 Data File : VU040724.D
 Acq On : 15 Oct 2020 16:41
 Operator : SY/MD
 Sample : L4421-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFSG7

Quant Time: Oct 16 05:28:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 16 04:23:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	104858	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	111498	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	47650	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	41387	4.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.20%
7) Chloroethane-d5	1.92	69	35462	5.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.80%
11) 1,1-Dichloroethene-d2	2.58	63	61870	3.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.80%
20) 2-Butanone-d5	4.65	46	158559	57.03	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.06%
24) Chloroform-d	5.08	84	85848	5.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.60%
26) 1,2-Dichloroethane-d4	5.72	65	51837	5.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.60%
32) Benzene-d6	5.74	84	152718	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	6.70	67	51253	5.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.60%
41) Toluene-d8	7.91	98	121080	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	8.19	79	19715	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	8.64	63	109534	50.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.52%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	47246	5.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	51698	5.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.00%


Target Compounds					Ovalue
3) Chloromethane	1.53	50	9931	1.118 ug/L	98
13) Acetone	2.66	43	21674	10.057 ug/L	94
14) Carbon disulfide	2.81	76	7628	0.364 ug/L #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101520\
Data File : VU040724.D
Acq On : 15 Oct 2020 16:41
Operator : SY/MD
Sample : L4421-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFSG7

Quant Time: Oct 16 05:28:36 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 16 04:23:22 2020
Response via : Initial Calibration

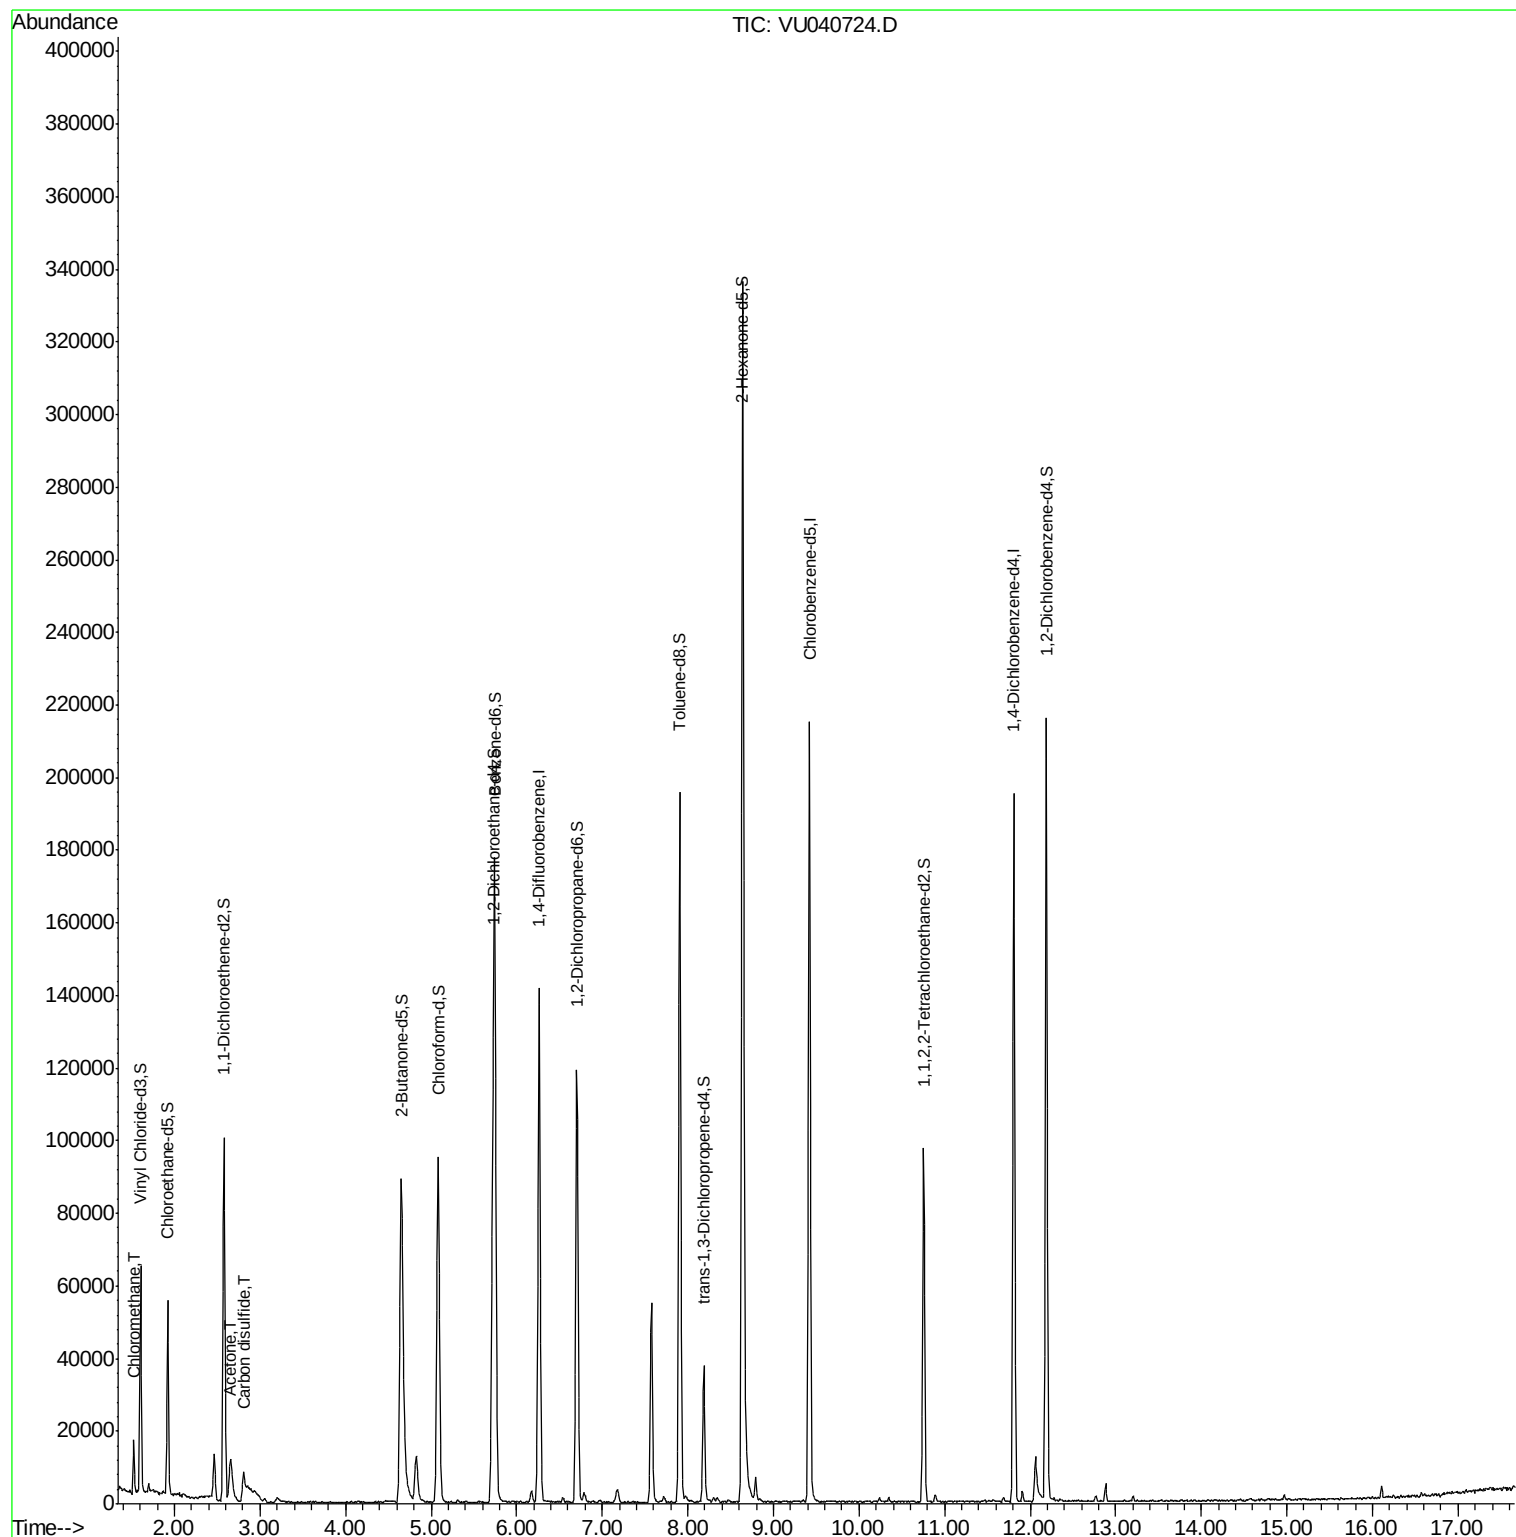

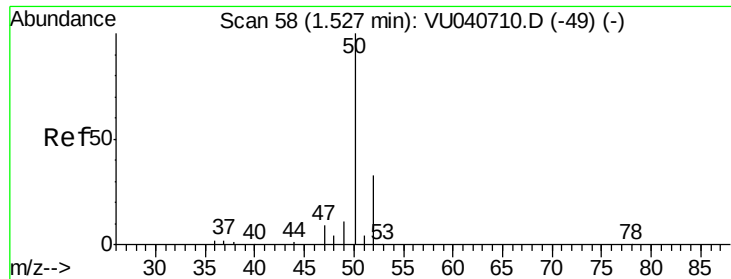

#3

Chloromethane

Concen: 1.118 ug/L

RT: 1.53 min Scan# 58

Delta R.T. -0.00 min

Lab File: VU040724.D

Acq: 15 Oct 2020 16:41

Instrument :

MSVOA_U

ClientSampleId :





BFSG7

Tot Ion: 50 Resp: 9931

Ion Ratio Lower Upper

50 100

52 32.3 21.9 40.7

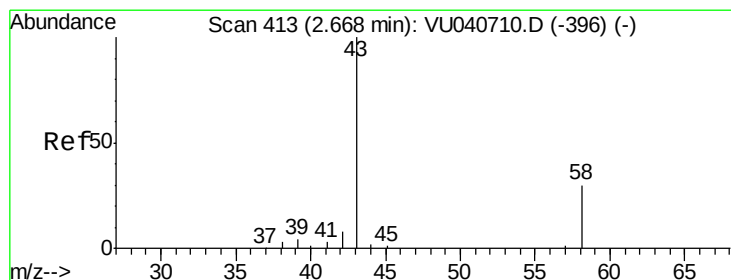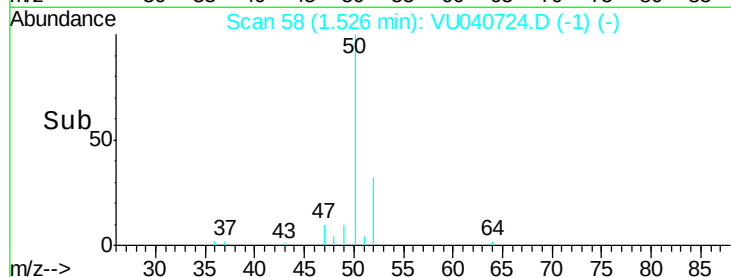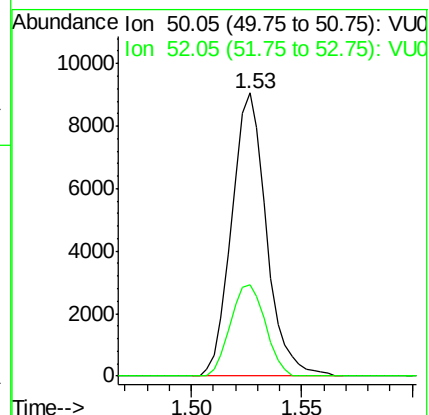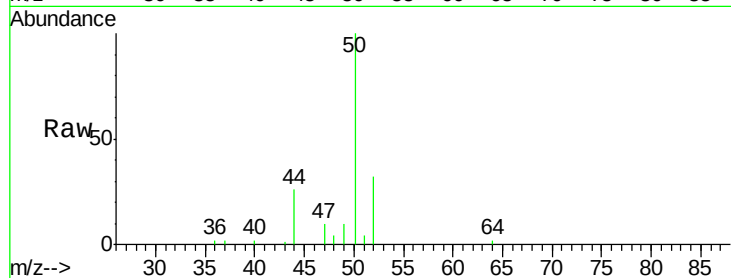

#13

Acetone

Concen: 10.057 ug/L

RT: 2.66 min Scan# 409

Delta R.T. -0.01 min

Lab File: VU040724.D




Acq: 15 Oct 2020 16:41




Tgt Ion: 43 Resp: 21674

Ion Ratio Lower Upper

43 100

58 27.2 0.0 60.6

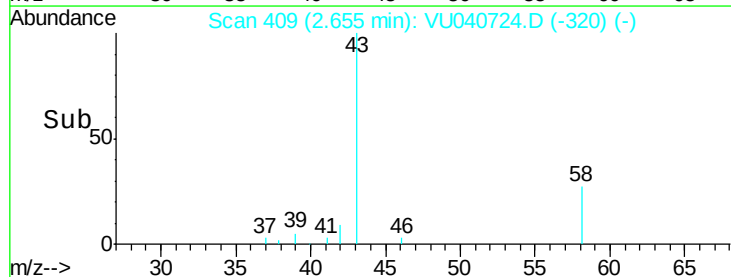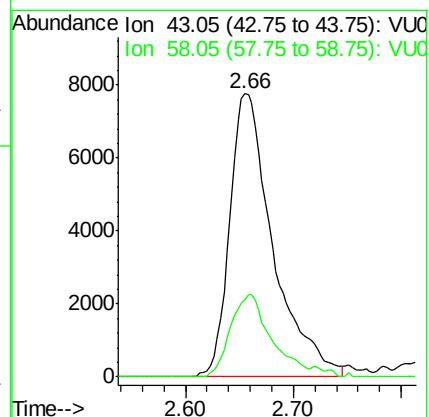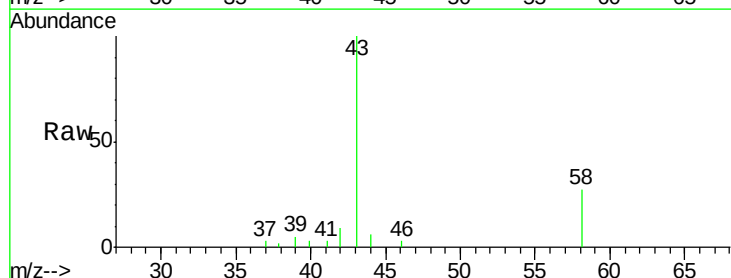

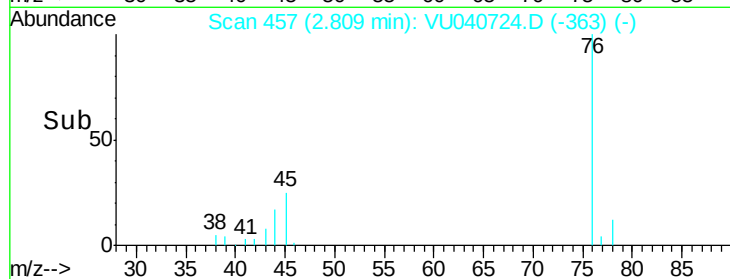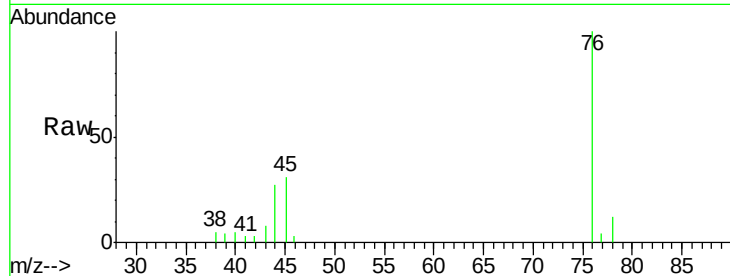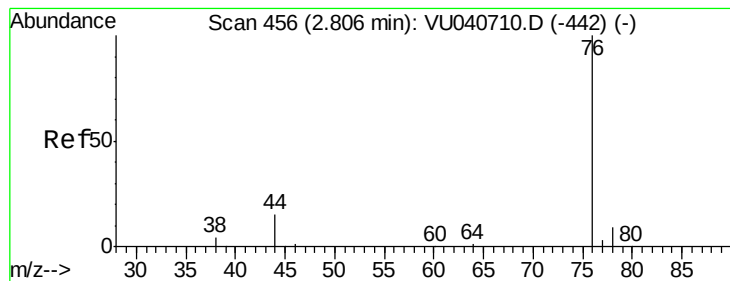

#14

Carbon disulfide

Concen: 0.364 ug/L

RT: 2.81 min Scan# 457

Delta R.T. 0.00 min

Lab File: VU040724.D

Acq: 15 Oct 2020 16:41

Instrument :

MSVOA_U

ClientSampleId :

BFSG7

Tot Ion: 76 Resp: 7628

Ion Ratio Lower Upper

76 100

78 11.7 6.8 10.2#

