

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U101520\
 Data File : VU040728.D
 Acq On : 15 Oct 2020 18:14
 Operator : SY/MD
 Sample : L4421-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFSJ8

Quant Time: Oct 16 05:39:02 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 16 04:23:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	108427	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	116466	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	47690	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	41235	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.92	69	37526	5.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.40%
11) 1,1-Dichloroethene-d2	2.58	63	65392	3.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.40%
20) 2-Butanone-d5	4.66	46	167800	58.36	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.72%
24) Chloroform-d	5.08	84	86119	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.20%
26) 1,2-Dichloroethane-d4	5.72	65	52289	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.80%
32) Benzene-d6	5.74	84	157657	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
36) 1,2-Dichloropropane-d6	6.70	67	53995	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.91	98	121252	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.20%
43) trans-1,3-Dichloropropene-	8.19	79	20847	4.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.40%
46) 2-Hexanone-d5	8.64	63	114384	50.24	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.48%
57) 1,1,2,2-Tetrachloroethane-	10.76	84	49047	5.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.80%
64) 1,2-Dichlorobenzene-d4	12.19	152	51679	5.84	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.80%


Target Compounds					Ovalue
3) Chloromethane	1.53	50	5525	0.601 ug/L	99
13) Acetone	2.66	43	9653	4.331 ug/L	65
47) Tetrachloroethene	8.56	164	14491	2.094 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101520\
Data File : VU040728.D
Acq On : 15 Oct 2020 18:14
Operator : SY/MD
Sample : L4421-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFSJ8

Quant Time: Oct 16 05:39:02 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 16 04:23:22 2020
Response via : Initial Calibration

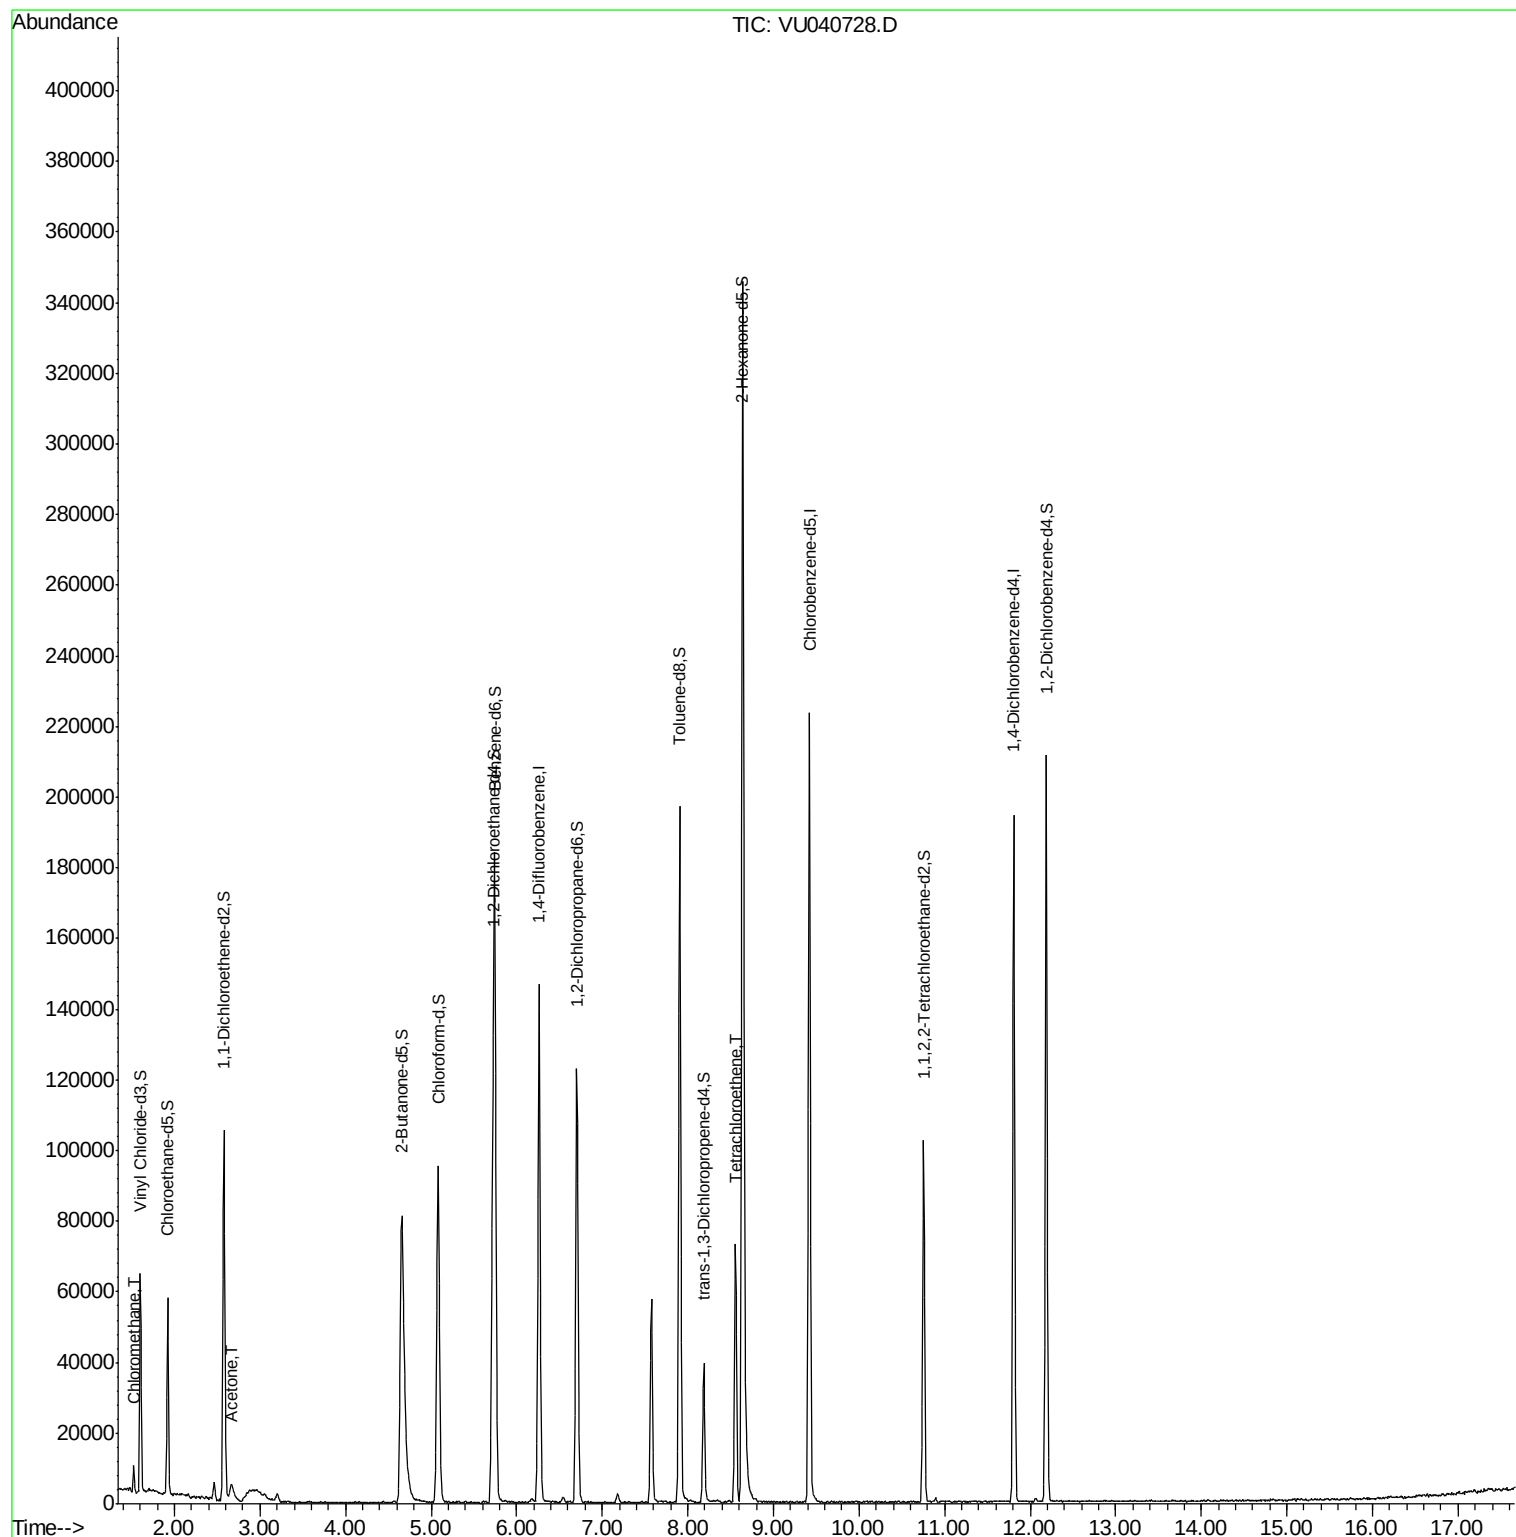

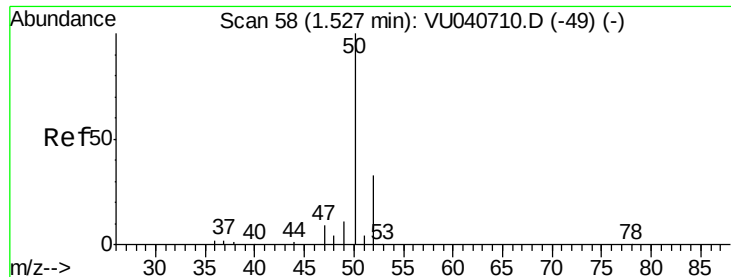

#3

Chloromethane

Concen: 0.601 ug/L

RT: 1.53 min Scan# 58

Delta R.T. 0.00 min

Lab File: VU040728.D

Acq: 15 Oct 2020 18:14

Instrument :

MSVOA_U

ClientSampleId :


BFSJ8

Tot Ion: 50 Resp: 5525

Ion Ratio Lower Upper




50 100

52 30.6 21.9 40.7

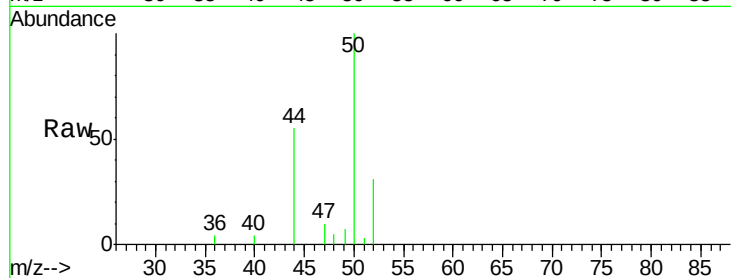

Abundance Ion 50.05 (49.75 to 50.75): VU0

Ion 52.05 (51.75 to 52.75): VU0

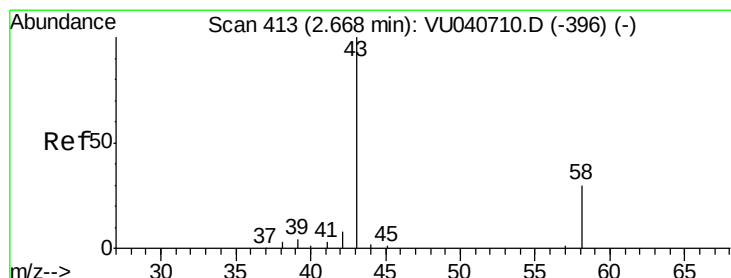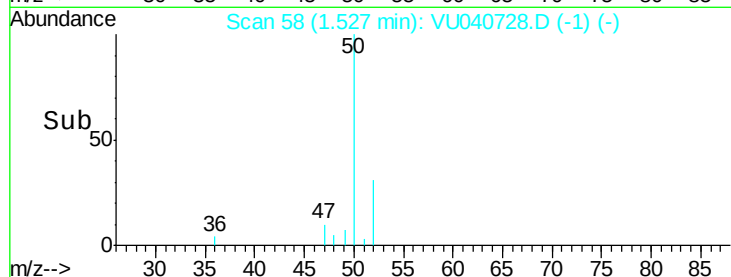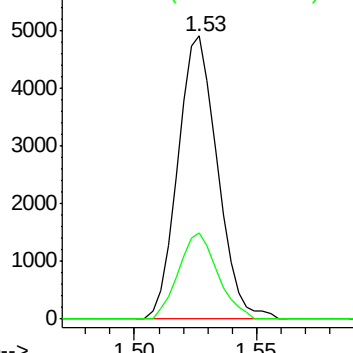

#13

Acetone

Concen: 4.331 ug/L

RT: 2.66 min Scan# 412

Delta R.T. -0.00 min

Lab File: VU040728.D


Acq: 15 Oct 2020 18:14

Tgt Ion: 43 Resp: 9653

Ion Ratio Lower Upper



43 100


58 11.1 0.0 60.6

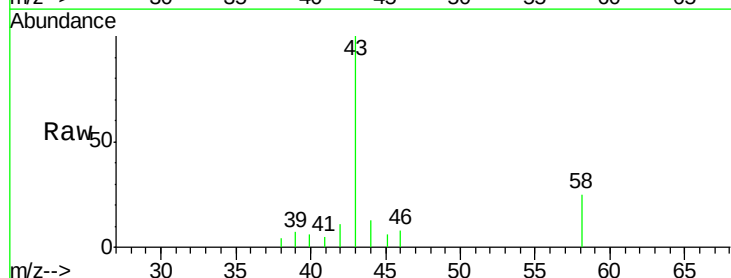

Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

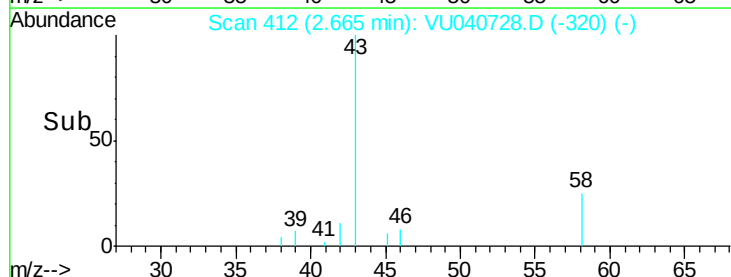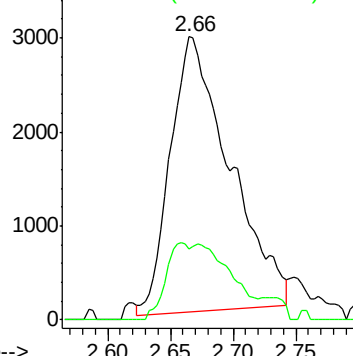

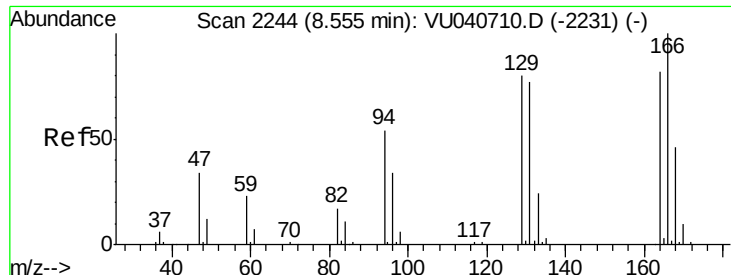

#47

Tetrachloroethene

Concen: 2.094 ug/L

RT: 8.56 min Scan# 2245

Delta R.T. 0.00 min

Lab File: VU040728.D

Acq: 15 Oct 2020 18:14

Instrument :

MSVOA_U

ClientSampleId :

BFSJ8

Tot Ion:164 Resp: 14491


Ion Ratio Lower Upper

164 100

129 101.0 68.8 127.8

131 94.3 66.7 123.9

166 131.0 83.9 155.7

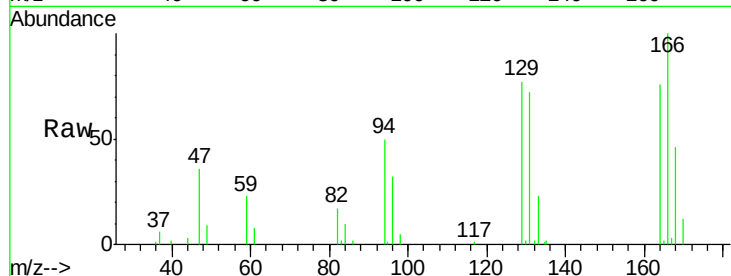

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

