


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101520\
 Data File : VU040709.D
 Acq On : 15 Oct 2020 09:45
 Operator : SY/MD
 Sample : BFB21
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB21

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Oct 16 10:52:06 2020

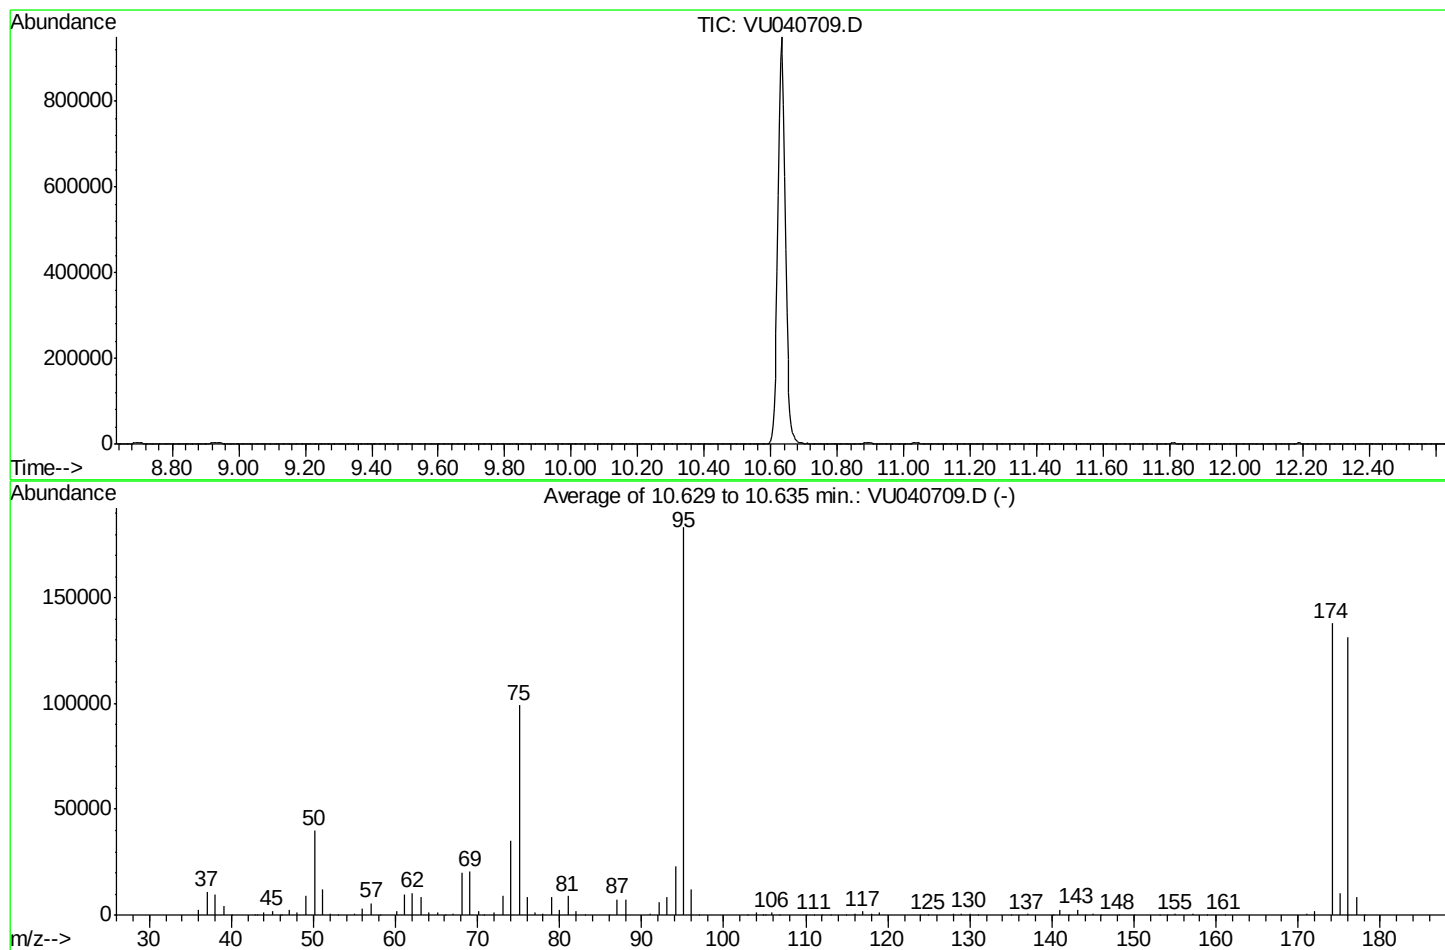

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	39728	PASS
75	95	30	80	54.0	99101	PASS
95	95	100	100	100.0	183445	PASS
96	95	5	9	6.7	12212	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.2	138010	PASS
175	174	5	9	7.7	10594	PASS
176	174	95	101	95.4	131714	PASS
177	176	5	9	6.4	8429	PASS

m/z	Abundance
36.00	2002.0
37.00	10999.0
38.00	9338.0
39.10	4132.0
40.10	383.0
43.20	137.0
44.00	1553.0
45.00	1769.0
46.20	186.0
47.00	2530.0
48.00	1268.0
49.10	8942.0
50.10	39464.0
51.10	12066.0
52.10	527.0
53.00	228.0
55.00	578.0
56.00	3151.0
57.10	5480.0
58.10	153.0
60.10	1756.0
61.10	9707.0
62.10	10548.0
63.10	8697.0
64.00	1433.0
65.10	1656.0
66.10	189.0
67.00	493.0
68.10	20080.0
69.10	20120.0
70.10	1549.0
70.80	105.0
72.00	1138.0
73.10	8662.0
74.10	34192.0
75.10	97160.0
76.10	9170.0
77.10	994.0
77.90	945.0
79.00	8455.0
80.00	2170.0
81.00	8736.0
82.00	2052.0
83.10	251.0
87.00	7263.0
88.00	6863.0
91.00	842.0
92.10	5800.0
93.10	8279.0
94.10	23024.0
95.10	178944.0
96.10	12253.0
97.00	331.0
102.90	126.0
104.00	1000.0
104.80	263.0
105.90	1066.0
106.90	168.0
110.00	161.0
111.10	205.0
112.00	144.0
112.90	247.0
114.90	198.0
116.00	615.0
117.00	1558.0
118.00	820.0
119.00	1202.0
124.90	149.0
128.00	543.0
128.90	364.0
130.00	710.0
130.90	209.0
135.00	332.0
137.00	305.0
140.10	153.0
141.00	2140.0
142.00	214.0
143.00	2636.0
144.00	123.0
145.00	756.0
146.00	187.0
148.10	281.0
150.00	123.0
154.00	142.0
155.00	367.0
157.10	281.0
158.90	209.0
161.00	145.0
171.00	397.0
172.00	1811.0
174.10	131024.0
175.10	10295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

176.10125448.0

177.108062.0

178.10217.0

Instrument :
MSVOA_U

ClientSampleId :
BFB21

m/z	Abundance
36.00	2233.0
37.00	11625.0
38.00	9805.0
39.10	4116.0
40.00	371.0
43.20	128.0
44.00	1523.0
45.00	1916.0
46.10	205.0
47.00	2471.0
48.00	1455.0
49.10	9436.0
50.10	41072.0
51.10	12477.0
52.10	586.0
53.00	197.0
55.00	589.0
56.00	3188.0
57.10	5736.0
58.10	198.0
60.10	1906.0
61.10	10267.0
62.10	10715.0
63.10	8882.0
64.00	1244.0
65.10	1509.0
66.10	170.0
67.00	555.0
68.10	21160.0
69.10	21200.0
70.10	1790.0
72.00	1166.0
73.10	9704.0
74.10	36552.0
75.10	102432.0
76.10	8901.0
77.10	1087.0
77.90	894.0
79.00	8770.0
80.00	2248.0
81.00	9189.0
82.00	2133.0
83.10	263.0
87.00	7758.0
88.00	7367.0
91.00	864.0
92.10	6103.0
93.10	8824.0
94.10	23944.0
95.10	189760.0
96.10	12533.0
97.00	275.0
102.90	119.0
104.00	1034.0
105.10	247.0
105.90	1086.0
106.90	199.0
110.00	153.0
111.00	217.0
112.00	207.0
113.00	243.0
114.90	214.0
116.00	752.0
117.00	1605.0
118.00	838.0
119.00	1207.0
124.00	103.0
125.00	139.0
128.00	673.0
128.90	359.0
130.00	727.0
131.00	233.0
135.10	297.0
137.00	361.0
140.10	169.0
141.00	2330.0
142.00	223.0
143.10	2662.0
144.00	124.0
145.00	747.0
146.00	202.0
148.10	284.0
150.00	149.0
154.10	106.0
155.10	395.0
157.10	373.0
158.90	196.0
161.00	144.0
171.00	380.0
172.00	1913.0
174.10	142912.0
175.10	10990.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

176.10

177.10

178.00

136192.0

8651.0

225.0

Instrument :

MSVOA_U

ClientSampleId :

BFB21

m/z	Abundance
36.00	2214.0
37.00	10895.0
38.00	9260.0
39.00	3659.0
40.00	304.0
42.90	141.0
44.00	1543.0
45.00	1845.0
45.90	245.0
47.10	2120.0
48.00	1384.0
49.10	8681.0
50.10	38648.0
51.10	11536.0
52.10	562.0
53.00	131.0
55.10	611.0
56.00	3028.0
57.10	5486.0
58.20	231.0
60.10	1884.0
61.10	9804.0
62.10	9873.0
63.10	8077.0
64.10	980.0
65.10	1343.0
66.10	131.0
67.10	579.0
68.10	19632.0
69.10	20032.0
70.10	1821.0
72.00	1081.0
73.10	9530.0
74.10	35200.0
75.10	97712.0
76.10	7851.0
77.00	1048.0
77.90	788.0
79.00	8225.0
80.00	2192.0
81.00	8571.0
82.00	1992.0
83.10	206.0
86.00	219.0
87.00	7634.0
88.10	7154.0
91.00	763.0
92.10	5679.0
93.10	8477.0
94.10	22632.0
95.10	181632.0
96.10	11851.0
97.00	319.0
102.90	121.0
104.00	1000.0
105.00	234.0
105.90	955.0
106.80	199.0
110.00	111.0
111.00	227.0
112.00	242.0
112.90	208.0
114.90	240.0
116.00	831.0
117.00	1558.0
118.00	777.0
119.00	1141.0
124.00	117.0
128.00	743.0
128.90	314.0
129.90	627.0
131.00	245.0
135.10	256.0
137.00	395.0
140.10	157.0
141.00	2233.0
142.00	253.0
143.10	2529.0
144.00	105.0
145.00	660.0
146.00	263.0
148.10	266.0
150.00	175.0
153.10	105.0
155.00	415.0
157.10	360.0
158.90	152.0
161.00	163.0
171.00	366.0
172.10	1782.0
174.10	140096.0
175.10	10497.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

176.10133504.0

177.108576.0

178.10195.0

Instrument :
MSVOA_U

ClientSampleId :
BFB21

Scan 2875 (10.584 min): VU040709.D
BFB21

m/z	Abundance
39.90	148.0
44.00	343.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21