


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101521\
 Data File : VU045315.D
 Acq On : 15 Oct 2021 10:39
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101321DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Thu Oct 14 05:46:27 2021

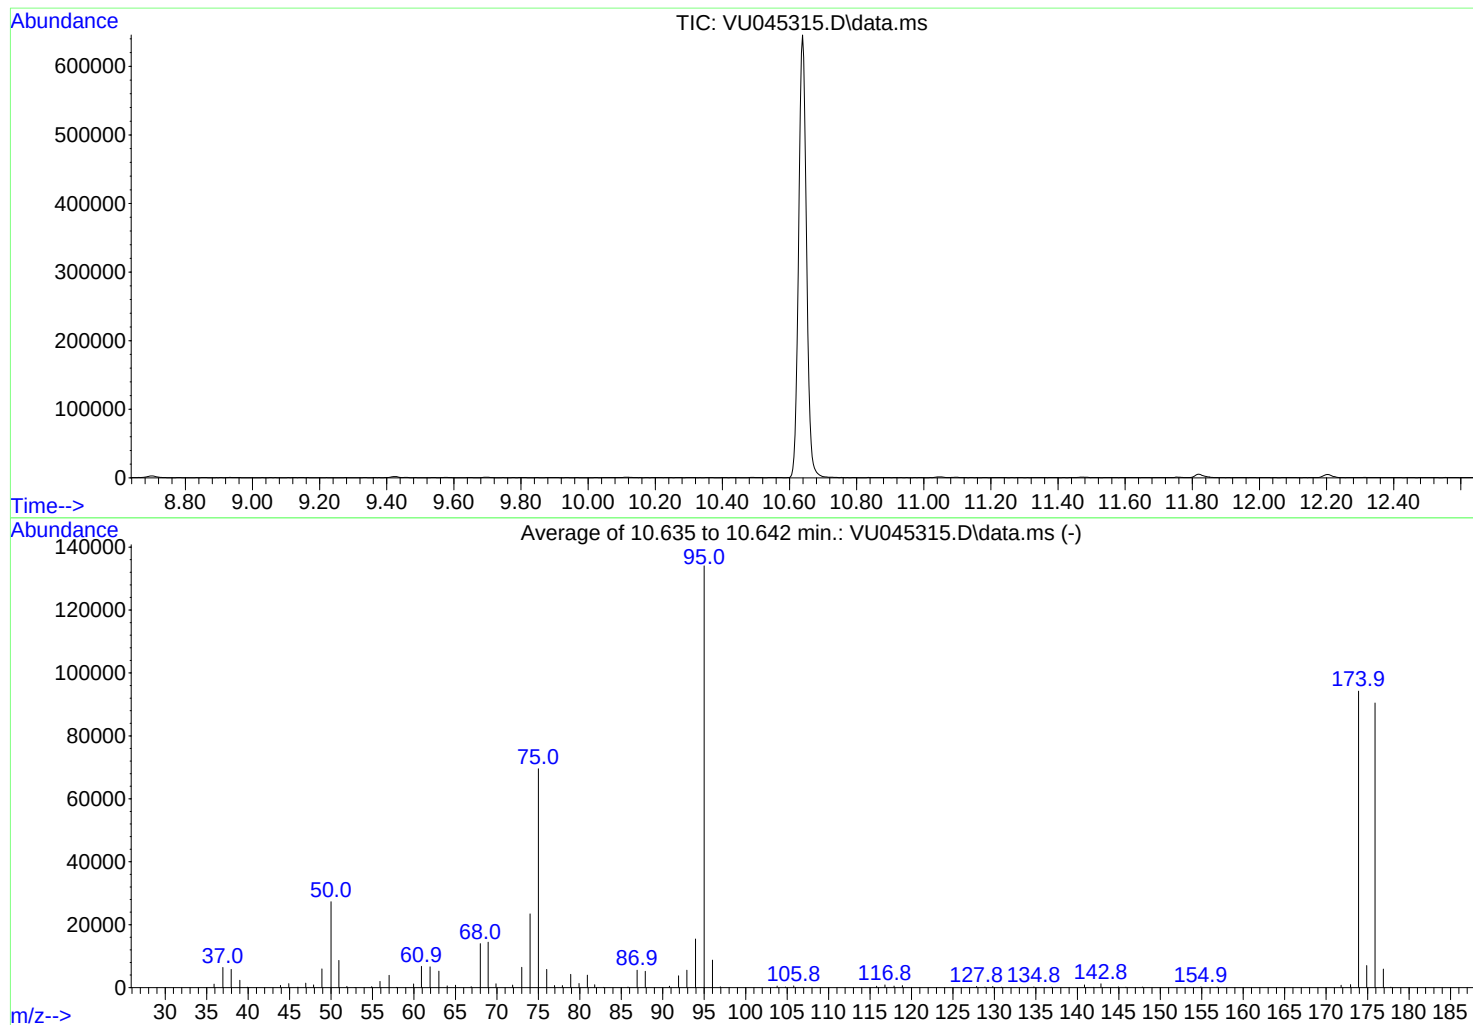

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	27320	PASS
75	95	30	60	51.9	69579	PASS
95	95	100	100	100.0	134056	PASS
96	95	5	9	6.5	8769	PASS
173	174	0.00	2	1.0	977	PASS
174	95	50	100	70.3	94243	PASS
175	174	5	9	7.5	7041	PASS
176	174	95	101	96.0	90464	PASS
177	176	5	9	6.5	5894	PASS