


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101620\
Data File : VU040737.D
Acq On : 16 Oct 2020 09:52
Operator : SY/MD
Sample : BFB22
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB22

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Oct 19 03:08:11 2020

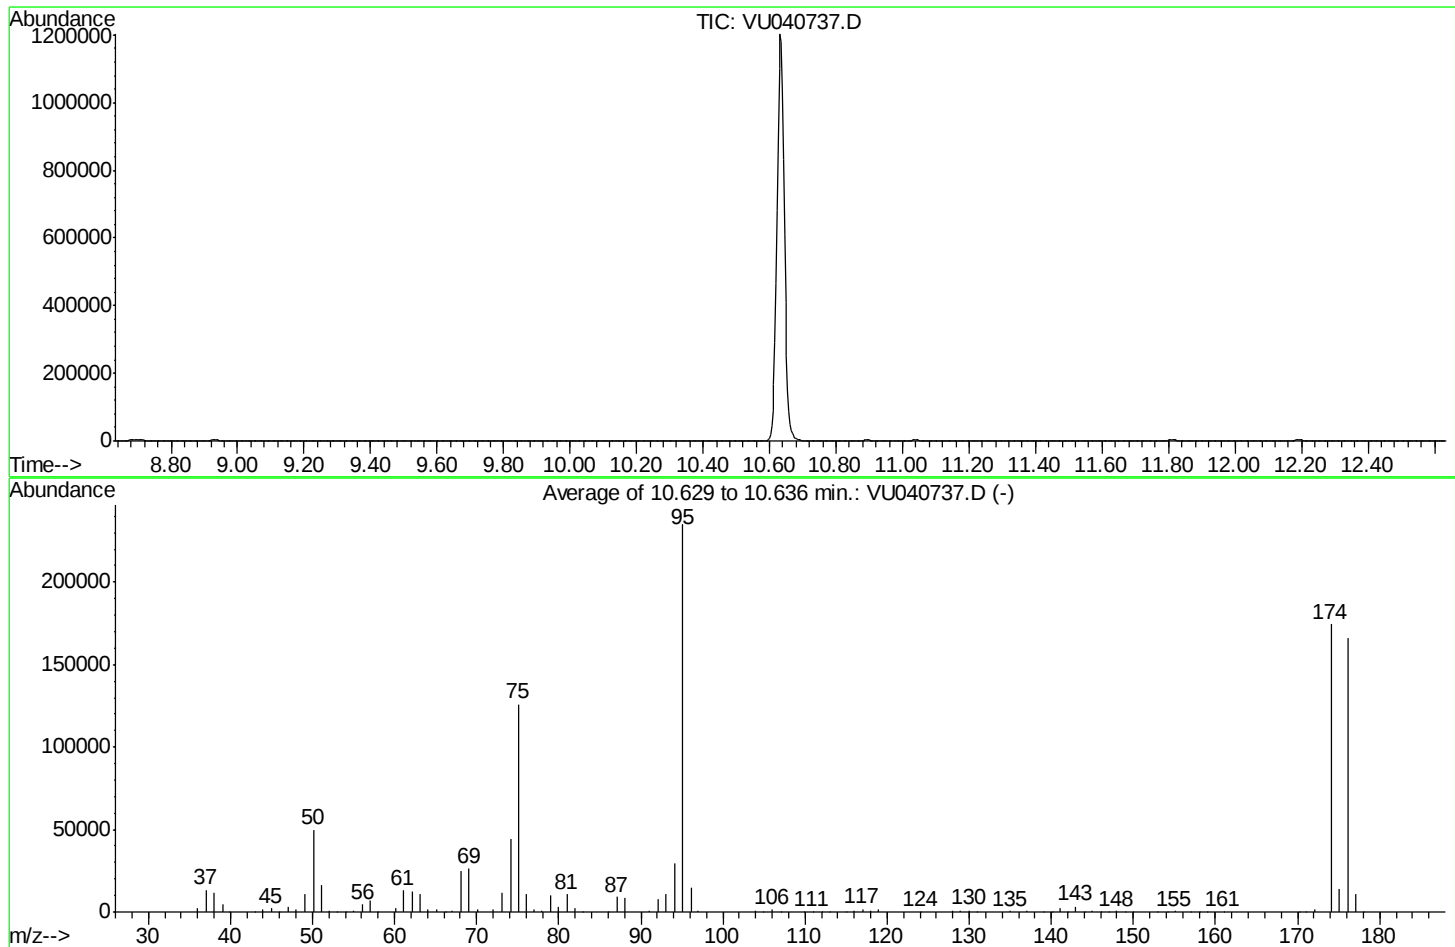

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	49840	PASS
75	95	30	80	53.6	126093	PASS
95	95	100	100	100.0	235050	PASS
96	95	5	9	6.4	14983	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.2	174378	PASS
175	174	5	9	7.9	13751	PASS
176	174	95	101	95.1	165760	PASS
177	176	5	9	6.4	10685	PASS

m/z	Abundance
36.00	2368.0
37.00	12828.0
38.10	11410.0
39.10	4968.0
40.00	358.0
44.10	1976.0
45.00	1950.0
45.90	315.0
47.10	2902.0
48.00	1635.0
49.00	10261.0
50.10	47840.0
51.10	15730.0
52.10	575.0
53.00	207.0
54.00	141.0
55.10	670.0
56.10	4106.0
57.10	6834.0
57.90	399.0
60.10	2516.0
61.00	12990.0
62.10	12258.0
63.10	10457.0
64.10	1795.0
65.10	1873.0
66.20	177.0
67.00	893.0
68.00	24128.0
69.10	25168.0
70.10	1831.0
72.00	1323.0
73.10	11089.0
74.10	41952.0
75.10	119856.0
76.10	10314.0
77.00	1212.0
78.00	948.0
79.00	9738.0
80.00	2898.0
81.00	10253.0
82.00	2200.0
82.90	189.0
86.10	429.0
87.10	8528.0
88.00	8266.0
91.00	1055.0
92.10	7110.0
93.10	10747.0
94.10	27712.0
95.10	223744.0
96.10	14470.0
97.00	355.0
104.00	990.0
104.90	374.0
106.00	1348.0
106.90	145.0
109.90	176.0
111.00	269.0
112.10	240.0
113.10	277.0
114.90	288.0
116.00	962.0
117.00	1771.0
118.00	1025.0
119.00	1728.0
124.10	144.0
128.00	747.0
128.90	490.0
130.00	915.0
130.90	288.0
135.00	528.0
137.00	459.0
139.10	106.0
140.10	161.0
141.00	2446.0
141.90	305.0
143.00	3131.0
144.10	159.0
145.00	799.0
146.00	378.0
147.10	118.0
148.00	454.0
149.10	124.0
149.90	187.0
153.00	124.0
154.10	250.0
155.10	504.0
156.90	316.0
159.00	355.0
160.90	187.0
170.20	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

170.90	385.0
172.10	1966.0
174.10	161216.0
175.10	12933.0
176.10	153088.0
177.10	10042.0
178.00	218.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	2570.0
37.00	13742.0
38.00	12226.0
39.10	5123.0
40.00	357.0
44.00	1982.0
45.00	2170.0
45.90	282.0
47.10	3077.0
48.00	1677.0
49.00	11197.0
50.10	51856.0
51.10	16864.0
52.00	533.0
53.00	162.0
54.00	117.0
55.00	652.0
56.10	4598.0
57.10	7481.0
57.90	404.0
60.10	2730.0
61.10	13377.0
62.10	13348.0
63.10	11080.0
64.10	1800.0
65.10	1671.0
66.20	141.0
67.00	911.0
68.00	25784.0
69.10	27128.0
70.10	2005.0
72.00	1337.0
73.10	11769.0
74.10	46048.0
75.10	130464.0
76.10	11361.0
77.10	1254.0
77.90	1008.0
79.00	10559.0
80.00	2914.0
81.00	11241.0
82.00	2352.0
83.00	220.0
86.10	375.0
87.10	9323.0
88.00	8824.0
91.00	1103.0
92.10	7775.0
93.10	11679.0
94.10	30592.0
95.10	243968.0
96.10	15582.0
97.00	500.0
104.00	1125.0
104.90	398.0
106.00	1543.0
107.00	132.0
110.00	209.0
110.90	330.0
112.10	245.0
113.00	246.0
115.00	291.0
116.00	1090.0
117.00	1884.0
118.00	1167.0
119.00	1659.0
124.10	149.0
128.00	818.0
128.90	555.0
130.00	1062.0
130.90	339.0
135.00	493.0
137.00	443.0
140.10	235.0
141.00	2749.0
142.00	348.0
143.00	3346.0
144.00	143.0
145.00	811.0
146.00	377.0
148.00	549.0
149.00	172.0
149.90	182.0
153.00	134.0
154.10	259.0
155.00	594.0
157.00	384.0
159.00	302.0
160.90	253.0
170.20	127.0
170.90	394.0
172.00	1951.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

174.10	180736.0
175.10	14364.0
176.10	171456.0
177.10	11036.0
178.00	261.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	2554.0
37.00	13051.0
38.00	11790.0
39.10	4865.0
40.00	335.0
43.00	128.0
44.00	1861.0
45.00	2107.0
45.90	257.0
47.10	2849.0
48.00	1589.0
49.10	10932.0
50.10	49824.0
51.10	15642.0
52.00	584.0
53.00	159.0
55.00	659.0
56.10	4767.0
57.10	7204.0
58.00	343.0
60.10	2673.0
61.10	12535.0
62.10	12761.0
63.10	10282.0
64.10	1528.0
65.10	1387.0
66.10	125.0
67.00	807.0
68.10	24912.0
69.10	26592.0
70.10	2064.0
72.00	1357.0
73.10	11384.0
74.10	45144.0
75.10	127960.0
76.10	11022.0
77.10	1273.0
78.00	936.0
79.00	10395.0
80.00	2693.0
81.00	10961.0
82.00	2227.0
83.00	226.0
86.10	319.0
87.00	9238.0
88.00	8747.0
91.00	1084.0
92.00	7375.0
93.10	11314.0
94.10	29784.0
95.10	237440.0
96.10	14897.0
97.00	535.0
104.00	1184.0
104.90	410.0
106.00	1534.0
107.10	148.0
110.00	226.0
110.90	326.0
112.10	230.0
113.00	251.0
115.00	319.0
116.00	1099.0
117.00	1876.0
118.00	1164.0
119.00	1469.0
124.10	102.0
128.00	841.0
128.90	568.0
130.00	1032.0
130.90	331.0
135.00	454.0
137.00	390.0
140.00	282.0
141.00	2735.0
142.10	369.0
143.00	3228.0
143.90	153.0
145.00	787.0
146.00	373.0
147.00	108.0
147.90	588.0
149.00	198.0
149.90	183.0
152.90	153.0
154.10	239.0
155.00	589.0
157.00	418.0
158.00	116.0
158.90	255.0
161.00	315.0
171.00	318.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

172.00	1884.0
174.10	181184.0
175.10	13956.0
176.10	172736.0
177.10	10979.0
178.00	271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

Scan 2875 (10.584 min): VU040737.D
BFB22

m/z	Abundance
39.80	173.0
44.00	385.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22