

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055775.D
 Acq On : 16 Oct 2023 16:25
 Operator : MD/SY
 Sample : 04874-03 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Oct 17 05:09:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 17 05:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	463112	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	475647	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	218141	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	149049	35.881	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	71.760%	
7) Chloroethane-d5	1.888	69	134550	39.626	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.260%	
11) 1,1-Dichloroethene-d2	2.557	63	208052	28.090	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	56.180%#	
21) 2-Butanone-d5	4.615	46	200657	65.191	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	65.190%	
24) Chloroform-d	5.055	84	299370	37.593	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	75.180%	
26) 1,2-Dichloroethane-d4	5.695	65	217571	44.387	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.780%	
32) Benzene-d6	5.721	84	637349	41.880	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	83.760%	
36) 1,2-Dichloropropane-d6	6.685	67	202979	42.130	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	84.260%	
41) Toluene-d8	7.894	98	554430	40.346	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	80.700%	
43) trans-1,3-Dichloroprop...	8.174	79	92343	39.900	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	79.800%	
47) 2-Hexanone-d5	8.631	63	111442	58.838	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	58.840%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	321458	43.347	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	86.700%	
66) 1,2-Dichlorobenzene-d4	12.190	152	206307	47.658	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.320%	
Target Compounds						
					Qvalue	
60) 1,2,3-Trichloropropane	11.811	75	26163	5.526	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055775.D
Acq On : 16 Oct 2023 16:25
Operator : MD/SY
Sample : 04874-03 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Oct 17 05:09:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 17 05:06:35 2023
Response via : Initial Calibration

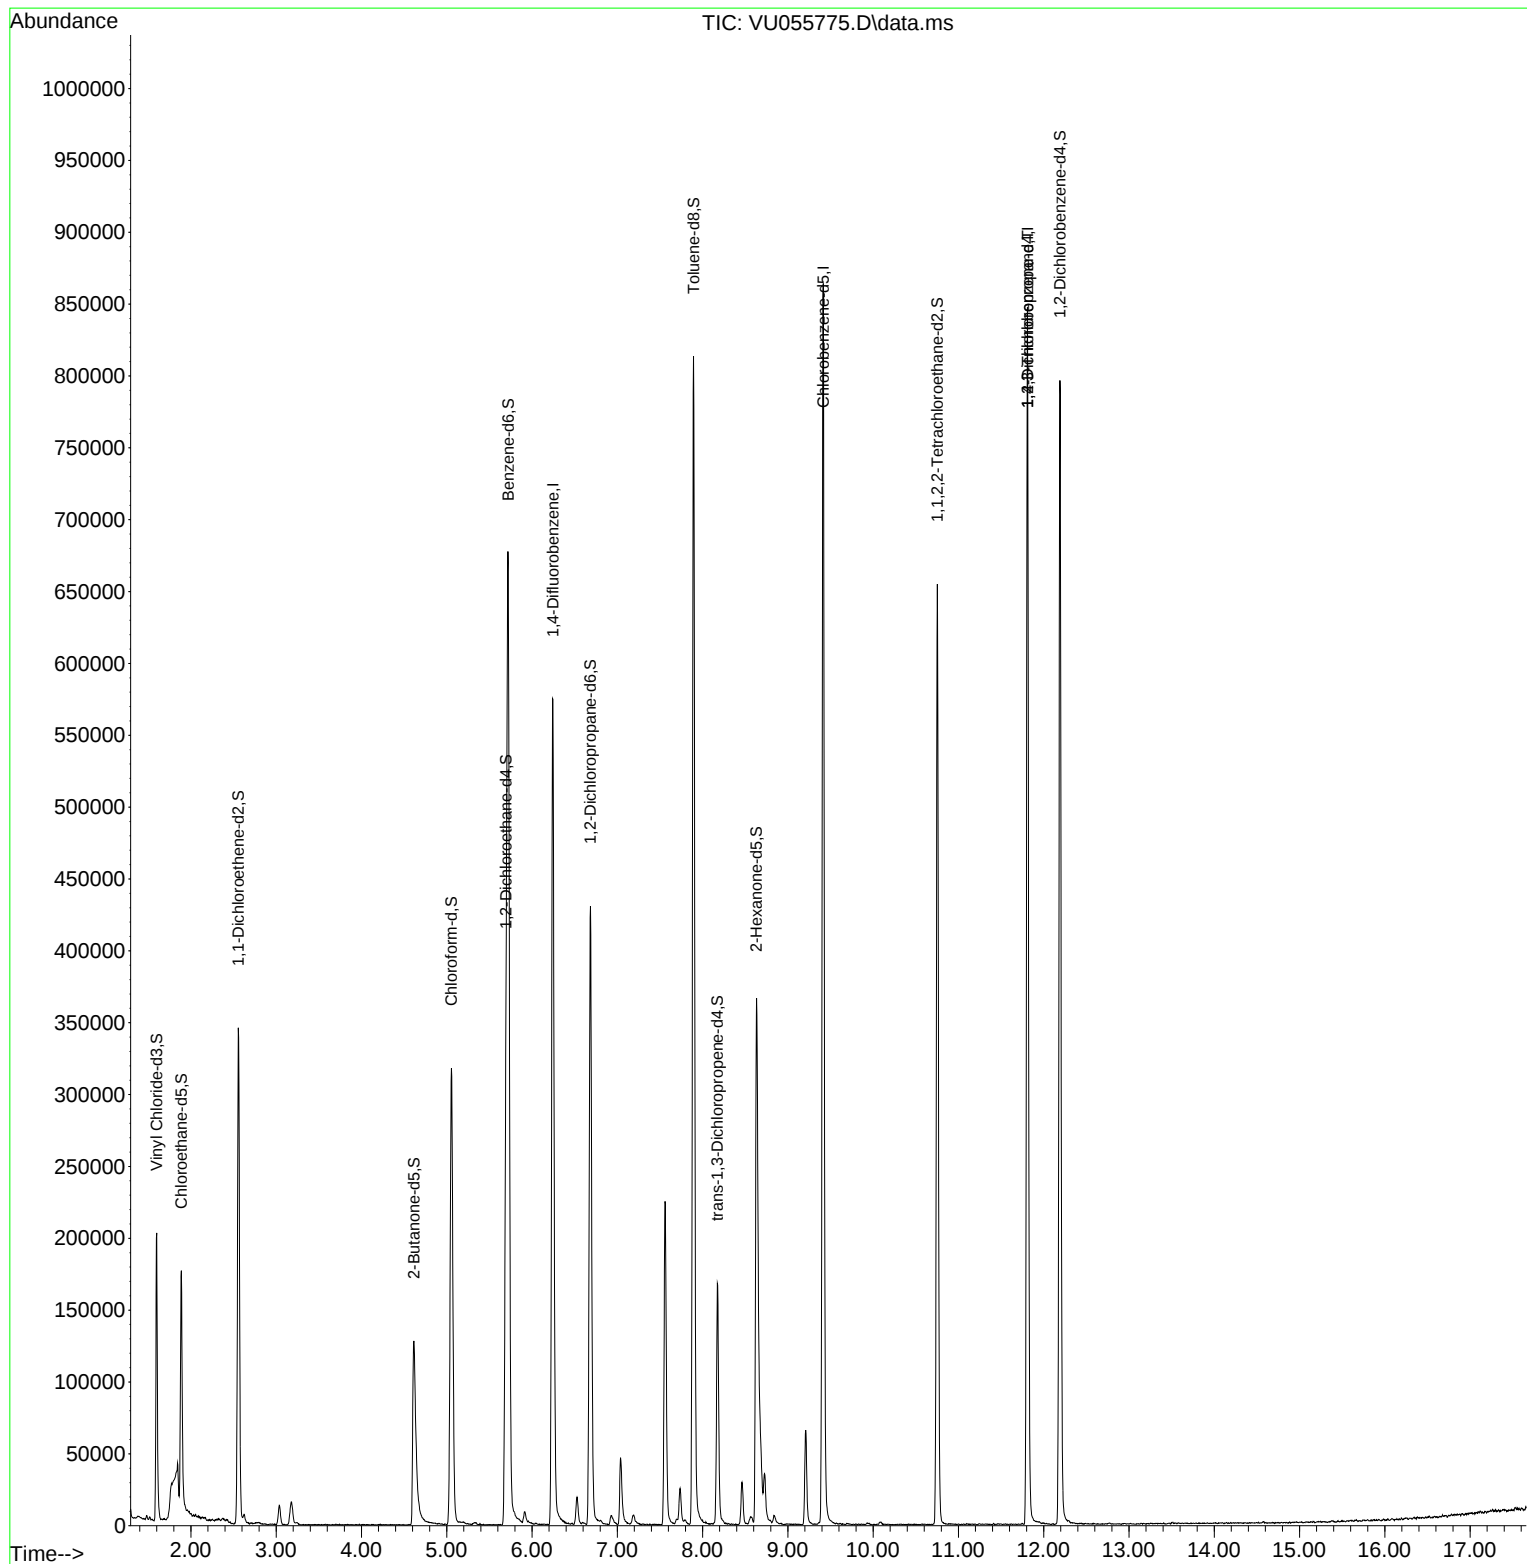

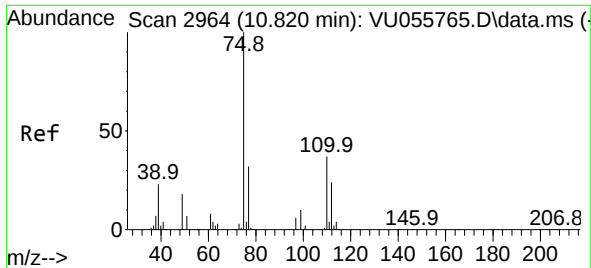

#60
 1,2,3-Trichloropropane
 Concen: 5.526 ug/L
 RT: 11.811 min Scan# 31
 Delta R.T. 0.990 min
 Lab File: VU055775.D
 Acq: 16 Oct 2023 16:25

Instrument :
 MSVOA_U
 ClientSampleId :

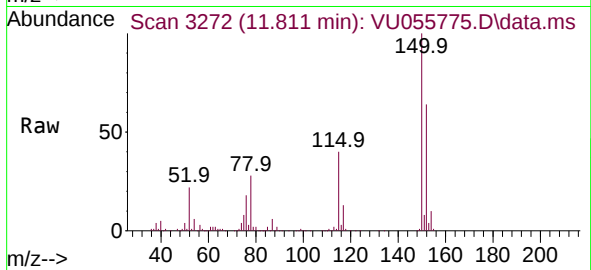

Tgt Ion:	75	Resp:	26163
Ion	Ratio	Lower	Upper
75	100		
77	37.3	25.8	38.8
110	2.9	28.5	42.7#

