

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055767.D
 Acq On : 16 Oct 2023 13:11
 Operator : MD/SY
 Sample : VU1016WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	114	rVB	264710	298735	14.07%	1.946%
2	1.769	139	149	160	rBV5	13032	23832	1.12%	0.155%
3	1.911	184	193	207	rBV	218538	286057	13.48%	1.864%
4	2.496	373	375	379	rVB2	802	500	0.02%	0.003%
5	2.567	381	397	418	rBV	429516	708221	33.37%	4.614%
6	2.904	499	502	508	rBV2	368	405	0.02%	0.003%
7	2.956	512	518	519	rBV3	328	333	0.02%	0.002%
8	3.004	529	533	536	rBV	365	252	0.01%	0.002%
9	3.046	536	546	563	rVB5	3460	6616	0.31%	0.043%
10	3.181	583	588	589	rBV2	654	525	0.02%	0.003%
11	3.316	625	630	635	rBV2	237	241	0.01%	0.002%
12	3.341	635	638	640	rBV2	388	231	0.01%	0.002%
13	3.354	640	642	646	rBV2	345	273	0.01%	0.002%
14	3.419	656	662	666	rBV3	460	450	0.02%	0.003%
15	3.570	706	709	712	rBV3	419	236	0.01%	0.002%
16	3.798	778	780	786	rVV2	497	356	0.02%	0.002%
17	3.885	803	807	813	rBV	274	242	0.01%	0.002%
18	3.959	825	830	834	rVB2	261	271	0.01%	0.002%
19	4.116	875	879	883	rVB2	321	270	0.01%	0.002%
20	4.165	890	894	900	rVV2	183	238	0.01%	0.002%
21	4.615	1023	1034	1070	rBV	149545	401749	18.93%	2.617%
22	4.933	1129	1133	1135	rBV3	482	352	0.02%	0.002%
23	4.988	1148	1150	1153	rVB2	344	223	0.01%	0.001%
24	5.058	1154	1172	1199	rBV	387837	871132	41.04%	5.675%
25	5.287	1239	1243	1244	rBV2	562	398	0.02%	0.003%
26	5.322	1251	1254	1255	rBV2	429	229	0.01%	0.001%
27	5.402	1277	1279	1286	rVB2	418	337	0.02%	0.002%
28	5.724	1357	1379	1406	rBV2	761229	2122584	100.00%	13.828%
29	5.952	1447	1450	1453	rBV3	438	278	0.01%	0.002%
30	5.972	1454	1456	1459	rVB	558	225	0.01%	0.001%
31	6.248	1528	1542	1572	rBV	567143	1123607	52.94%	7.320%
32	6.531	1618	1630	1644	rBV2	25545	52435	2.47%	0.342%
33	6.621	1656	1658	1662	rBV3	621	409	0.02%	0.003%
34	6.689	1662	1679	1703	rBV	471197	958860	45.17%	6.246%
35	6.933	1751	1755	1756	rBV	387	254	0.01%	0.002%
36	6.994	1771	1774	1776	rBV	412	232	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055767.D
 Acq On : 16 Oct 2023 13:11
 Operator : MD/SY
 Sample : VU1016WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.190	1823	1835	1848	rBV4	5485	11548	0.54%	0.075%
38	7.473	1914	1923	1929	rBV2	295	464	0.02%	0.003%
39	7.563	1938	1951	1970	rBV	246330	454865	21.43%	2.963%
40	7.746	2006	2008	2010	rBV3	627	304	0.01%	0.002%
41	7.788	2018	2021	2023	rVB2	413	221	0.01%	0.001%
42	7.804	2023	2026	2032	rVB3	1188	1032	0.05%	0.007%
43	7.898	2041	2055	2090	rBV	927846	1667261	78.55%	10.861%
44	8.116	2121	2123	2130	rVB5	702	646	0.03%	0.004%
45	8.177	2130	2142	2162	rBV	172838	312072	14.70%	2.033%
46	8.316	2182	2185	2190	rBV2	685	629	0.03%	0.004%
47	8.373	2199	2203	2207	rBV2	288	295	0.01%	0.002%
48	8.396	2207	2210	2213	rVB2	499	236	0.01%	0.002%
49	8.470	2230	2233	2236	rVB2	647	424	0.02%	0.003%
50	8.553	2251	2259	2261	rBV4	908	761	0.04%	0.005%
51	8.634	2272	2284	2323	rBV4	294340	795304	37.47%	5.181%
52	8.930	2371	2376	2379	rVB3	795	676	0.03%	0.004%
53	8.955	2379	2384	2388	rBV3	643	556	0.03%	0.004%
54	8.981	2388	2392	2394	rBV	513	419	0.02%	0.003%
55	9.164	2446	2449	2452	rVV3	501	307	0.01%	0.002%
56	9.209	2459	2463	2469	rBV4	1200	1168	0.06%	0.008%
57	9.415	2513	2527	2561	rBV	858974	1446047	68.13%	9.420%
58	9.573	2574	2576	2581	rVB3	899	656	0.03%	0.004%
59	9.605	2584	2586	2588	rVB	552	225	0.01%	0.001%
60	9.637	2588	2596	2597	rBV3	433	481	0.02%	0.003%
61	9.682	2606	2610	2611	rBV	617	329	0.02%	0.002%
62	9.785	2639	2642	2645	rBV2	487	252	0.01%	0.002%
63	9.817	2648	2652	2655	rVB3	486	396	0.02%	0.003%
64	9.952	2691	2694	2698	rBV2	279	264	0.01%	0.002%
65	10.010	2710	2712	2715	rBV	335	269	0.01%	0.002%
66	10.174	2758	2763	2766	rBV2	513	441	0.02%	0.003%
67	10.357	2818	2820	2824	rVV2	457	300	0.01%	0.002%
68	10.380	2824	2827	2830	rVV	397	254	0.01%	0.002%
69	10.489	2856	2861	2864	rBV3	560	487	0.02%	0.003%
70	10.602	2892	2896	2903	rBV2	391	333	0.02%	0.002%
71	10.753	2928	2943	2967	rBV	627465	1038335	48.92%	6.764%
72	11.213	3081	3086	3089	rBV3	384	298	0.01%	0.002%
73	11.367	3132	3134	3139	rVB	293	221	0.01%	0.001%
74	11.486	3169	3171	3175	rVB	760	453	0.02%	0.003%
75	11.508	3175	3178	3180	rBV	378	270	0.01%	0.002%
76	11.595	3201	3205	3206	rBV2	305	219	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055767.D
 Acq On : 16 Oct 2023 13:11
 Operator : MD/SY
 Sample : VU1016WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.701	3235	3238	3241	rBV	440	246	0.01%	0.002%
78	11.727	3243	3246	3250	rVB2	466	345	0.02%	0.002%
79	11.753	3250	3254	3259	rBV3	503	473	0.02%	0.003%
80	11.811	3259	3272	3296	rBV	790283	1318026	62.10%	8.586%
81	11.987	3323	3327	3329	rVB2	567	391	0.02%	0.003%
82	12.004	3329	3332	3333	rBV2	559	263	0.01%	0.002%
83	12.068	3350	3352	3355	rBV2	411	260	0.01%	0.002%
84	12.190	3377	3390	3412	rBV	842057	1422289	67.01%	9.265%
85	12.389	3450	3452	3456	rBV3	603	386	0.02%	0.003%
86	12.467	3473	3476	3482	rVB4	559	476	0.02%	0.003%
87	12.495	3482	3485	3487	rBV	393	226	0.01%	0.001%
88	12.624	3520	3525	3527	rBV3	471	430	0.02%	0.003%
89	12.682	3539	3543	3547	rBV3	600	593	0.03%	0.004%
90	12.730	3554	3558	3560	rBV	251	221	0.01%	0.001%
91	12.849	3592	3595	3597	rBV2	442	299	0.01%	0.002%
92	12.910	3611	3614	3617	rVB	608	397	0.02%	0.003%
93	13.016	3645	3647	3653	rVB2	619	514	0.02%	0.003%
94	13.081	3664	3667	3670	rBV2	524	395	0.02%	0.003%
95	13.222	3708	3711	3714	rBV3	464	400	0.02%	0.003%
96	13.769	3878	3881	3882	rBV	482	222	0.01%	0.001%
97	13.817	3893	3896	3898	rBV	500	295	0.01%	0.002%
98	13.868	3909	3912	3916	rBV2	1161	1041	0.05%	0.007%
99	13.910	3923	3925	3929	rBV3	419	245	0.01%	0.002%
100	15.537	4429	4431	4434	rBV2	880	676	0.03%	0.004%


Sum of corrected areas: 15350415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055767.D
Acq On : 16 Oct 2023 13:11
Operator : MD/SY
Sample : VU1016WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

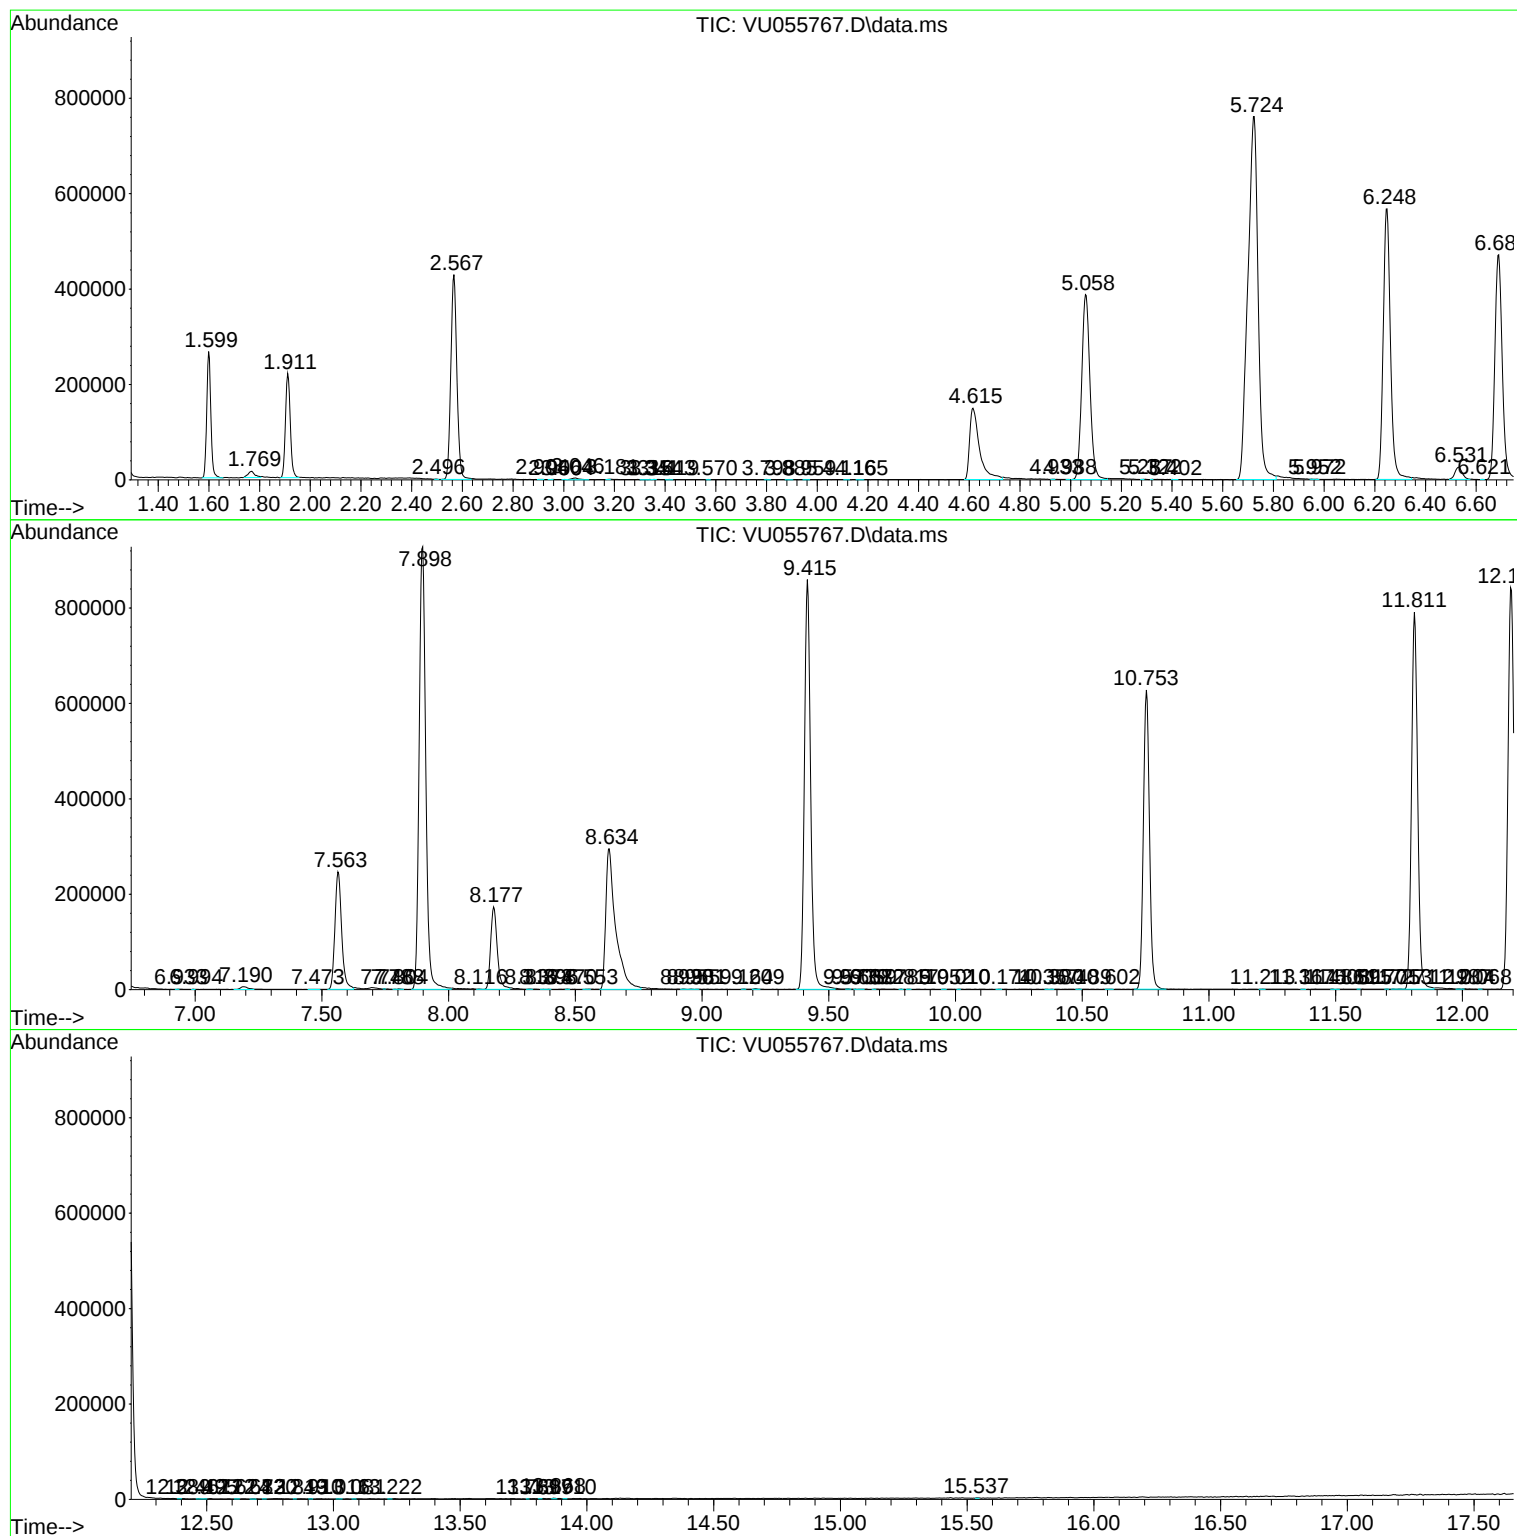

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055767.D
Acq On : 16 Oct 2023 13:11
Operator : MD/SY
Sample : VU1016WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055767.D
Acq On : 16 Oct 2023 13:11
Operator : MD/SY
Sample : VU1016WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK108

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------