

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055776.D
 Acq On : 16 Oct 2023 16:49
 Operator : MD/SY
 Sample : 04874-04 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.480	55	59	66	rVB4	4238	4618	0.24%	0.031%
2	1.512	67	69	76	rBV4	1879	2050	0.11%	0.014%
3	1.599	87	96	110	rBV	213121	260646	13.54%	1.762%
4	1.792	144	156	159	rBV6	17442	37411	1.94%	0.253%
5	1.891	179	187	204	rVB	181236	267306	13.89%	1.807%
6	2.480	367	370	375	rVB4	973	718	0.04%	0.005%
7	2.560	382	395	408	rBV	380540	622283	32.33%	4.206%
8	2.843	481	483	487	rVB2	658	429	0.02%	0.003%
9	2.940	509	513	516	rBV3	896	827	0.04%	0.006%
10	3.039	533	544	554	rBV2	13709	25755	1.34%	0.174%
11	3.178	573	587	601	rBV2	19971	46394	2.41%	0.314%
12	3.316	626	630	634	rBV2	382	389	0.02%	0.003%
13	3.702	745	750	753	rVV2	456	492	0.03%	0.003%
14	3.821	784	787	793	rBV2	331	381	0.02%	0.003%
15	4.232	908	915	918	rBV	372	449	0.02%	0.003%
16	4.271	923	927	928	rBV	471	361	0.02%	0.002%
17	4.403	963	968	972	rVB2	393	407	0.02%	0.003%
18	4.615	1018	1034	1064	rBV	148342	405554	21.07%	2.741%
19	5.055	1155	1171	1203	rBV	348706	784445	40.75%	5.302%
20	5.386	1270	1274	1280	rVB3	627	599	0.03%	0.004%
21	5.634	1347	1351	1356	rBV	640	516	0.03%	0.003%
22	5.718	1356	1377	1406	rBV2	693561	1924933	100.00%	13.010%
23	5.911	1430	1437	1452	rVB2	5702	10902	0.57%	0.074%
24	6.004	1464	1466	1470	rVB2	632	467	0.02%	0.003%
25	6.023	1470	1472	1476	rBV2	741	352	0.02%	0.002%
26	6.100	1493	1496	1499	rBV2	530	440	0.02%	0.003%
27	6.123	1499	1503	1508	rVV3	728	643	0.03%	0.004%
28	6.168	1514	1517	1522	rBV3	502	504	0.03%	0.003%
29	6.242	1527	1540	1566	rBV	554494	1079708	56.09%	7.297%
30	6.531	1618	1630	1642	rBV4	20697	41101	2.14%	0.278%
31	6.595	1646	1650	1654	rVB4	727	604	0.03%	0.004%
32	6.611	1654	1655	1659	rVB2	958	525	0.03%	0.004%
33	6.685	1662	1678	1705	rBV	437165	872784	45.34%	5.899%
34	6.865	1732	1734	1740	rVB3	764	672	0.03%	0.005%
35	6.930	1743	1754	1769	rBV	7144	14843	0.77%	0.100%
36	6.994	1772	1774	1780	rVB3	901	589	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055776.D
 Acq On : 16 Oct 2023 16:49
 Operator : MD/SY
 Sample : 04874-04 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.046	1780	1790	1806	rBV	14990	29421	1.53%	0.199%
38	7.119	1811	1813	1818	rVB2	516	423	0.02%	0.003%
39	7.152	1820	1823	1825	rVB2	674	363	0.02%	0.002%
40	7.187	1825	1834	1841	rBV5	6573	12061	0.63%	0.082%
41	7.274	1859	1861	1867	rVB3	528	372	0.02%	0.003%
42	7.367	1887	1890	1895	rBV2	548	437	0.02%	0.003%
43	7.393	1895	1898	1906	rVB2	620	548	0.03%	0.004%
44	7.560	1938	1950	1977	rBV	232090	417270	21.68%	2.820%
45	7.695	1986	1992	1996	rBV5	3193	4247	0.22%	0.029%
46	7.737	1997	2005	2016	rVB2	15039	25926	1.35%	0.175%
47	7.782	2017	2019	2020	rBV2	1021	496	0.03%	0.003%
48	7.894	2040	2054	2086	rBV	830739	1475121	76.63%	9.970%
49	8.100	2113	2118	2121	rBV4	640	474	0.02%	0.003%
50	8.174	2129	2141	2163	rBV	159502	282649	14.68%	1.910%
51	8.460	2219	2230	2247	rVV3	22024	38022	1.98%	0.257%
52	8.560	2252	2261	2271	rBV8	3922	8202	0.43%	0.055%
53	8.634	2272	2284	2310	rBV4	374140	908400	47.19%	6.139%
54	8.824	2341	2343	2345	rBV3	749	348	0.02%	0.002%
55	9.010	2395	2401	2404	rBV2	683	732	0.04%	0.005%
56	9.123	2434	2436	2440	rVB3	644	400	0.02%	0.003%
57	9.158	2443	2447	2450	rBV2	529	419	0.02%	0.003%
58	9.209	2453	2463	2478	rVV3	35226	60895	3.16%	0.412%
59	9.309	2489	2494	2498	rVB2	437	417	0.02%	0.003%
60	9.364	2504	2511	2514	rBV4	1364	1654	0.09%	0.011%
61	9.412	2514	2526	2554	rBV	823869	1392368	72.33%	9.410%
62	9.570	2572	2575	2578	rVB3	718	443	0.02%	0.003%
63	9.682	2605	2610	2612	rBV3	733	566	0.03%	0.004%
64	9.923	2679	2685	2686	rBV3	851	760	0.04%	0.005%
65	10.174	2755	2763	2769	rBV2	621	1078	0.06%	0.007%
66	10.595	2888	2894	2896	rBV	474	376	0.02%	0.003%
67	10.753	2930	2943	2967	rBV	670983	1082710	56.25%	7.317%
68	10.971	3006	3011	3014	rBV	416	388	0.02%	0.003%
69	11.036	3026	3031	3035	rBV2	435	424	0.02%	0.003%
70	11.235	3089	3093	3097	rVB2	699	628	0.03%	0.004%
71	11.315	3111	3118	3119	rBV	503	473	0.02%	0.003%
72	11.811	3259	3272	3297	rBV	783210	1287692	66.90%	8.703%
73	12.020	3333	3337	3339	rBV2	547	481	0.02%	0.003%
74	12.090	3354	3359	3362	rBV4	841	808	0.04%	0.005%
75	12.190	3377	3390	3414	rBV	798559	1331158	69.15%	8.997%
76	12.438	3460	3467	3468	rBV4	738	720	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055776.D
 Acq On : 16 Oct 2023 16:49
 Operator : MD/SY
 Sample : 04874-04 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	12.537	3495	3498	3500	rBV2	551	382	0.02%	0.003%
78	12.579	3507	3511	3514	rBV2	529	417	0.02%	0.003%
79	12.814	3581	3584	3590	rBV4	572	632	0.03%	0.004%
80	12.907	3610	3613	3619	rBV3	480	531	0.03%	0.004%
81	12.962	3626	3630	3633	rBV2	484	461	0.02%	0.003%
82	12.978	3633	3635	3639	rVB	709	479	0.02%	0.003%
83	13.007	3639	3644	3648	rBV2	1009	1001	0.05%	0.007%
84	13.032	3649	3652	3655	rBV2	757	554	0.03%	0.004%
85	13.174	3694	3696	3701	rVB3	608	517	0.03%	0.003%
86	13.261	3719	3723	3727	rBV3	417	422	0.02%	0.003%
87	13.338	3745	3747	3754	rVB3	743	701	0.04%	0.005%
88	13.376	3754	3759	3762	rBV2	528	487	0.03%	0.003%
89	13.402	3762	3767	3772	rVV4	711	756	0.04%	0.005%
90	13.434	3774	3777	3783	rVB2	581	418	0.02%	0.003%
91	13.512	3796	3801	3802	rBV3	456	367	0.02%	0.002%
92	13.557	3811	3815	3819	rBV3	675	719	0.04%	0.005%
93	14.106	3982	3986	3989	rBV2	606	591	0.03%	0.004%
94	14.222	4020	4022	4026	rVB2	914	484	0.03%	0.003%
95	14.274	4037	4038	4045	rBV4	473	379	0.02%	0.003%
96	14.560	4124	4127	4134	rVV7	1007	1114	0.06%	0.008%
97	14.884	4226	4228	4230	rBV	730	366	0.02%	0.002%
98	15.161	4309	4314	4316	rBV5	1191	1007	0.05%	0.007%
99	15.341	4366	4370	4375	rBV3	981	1100	0.06%	0.007%
100	15.473	4408	4411	4414	rBV2	1083	980	0.05%	0.007%


Sum of corrected areas: 14796332

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055776.D
Acq On : 16 Oct 2023 16:49
Operator : MD/SY
Sample : 04874-04 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

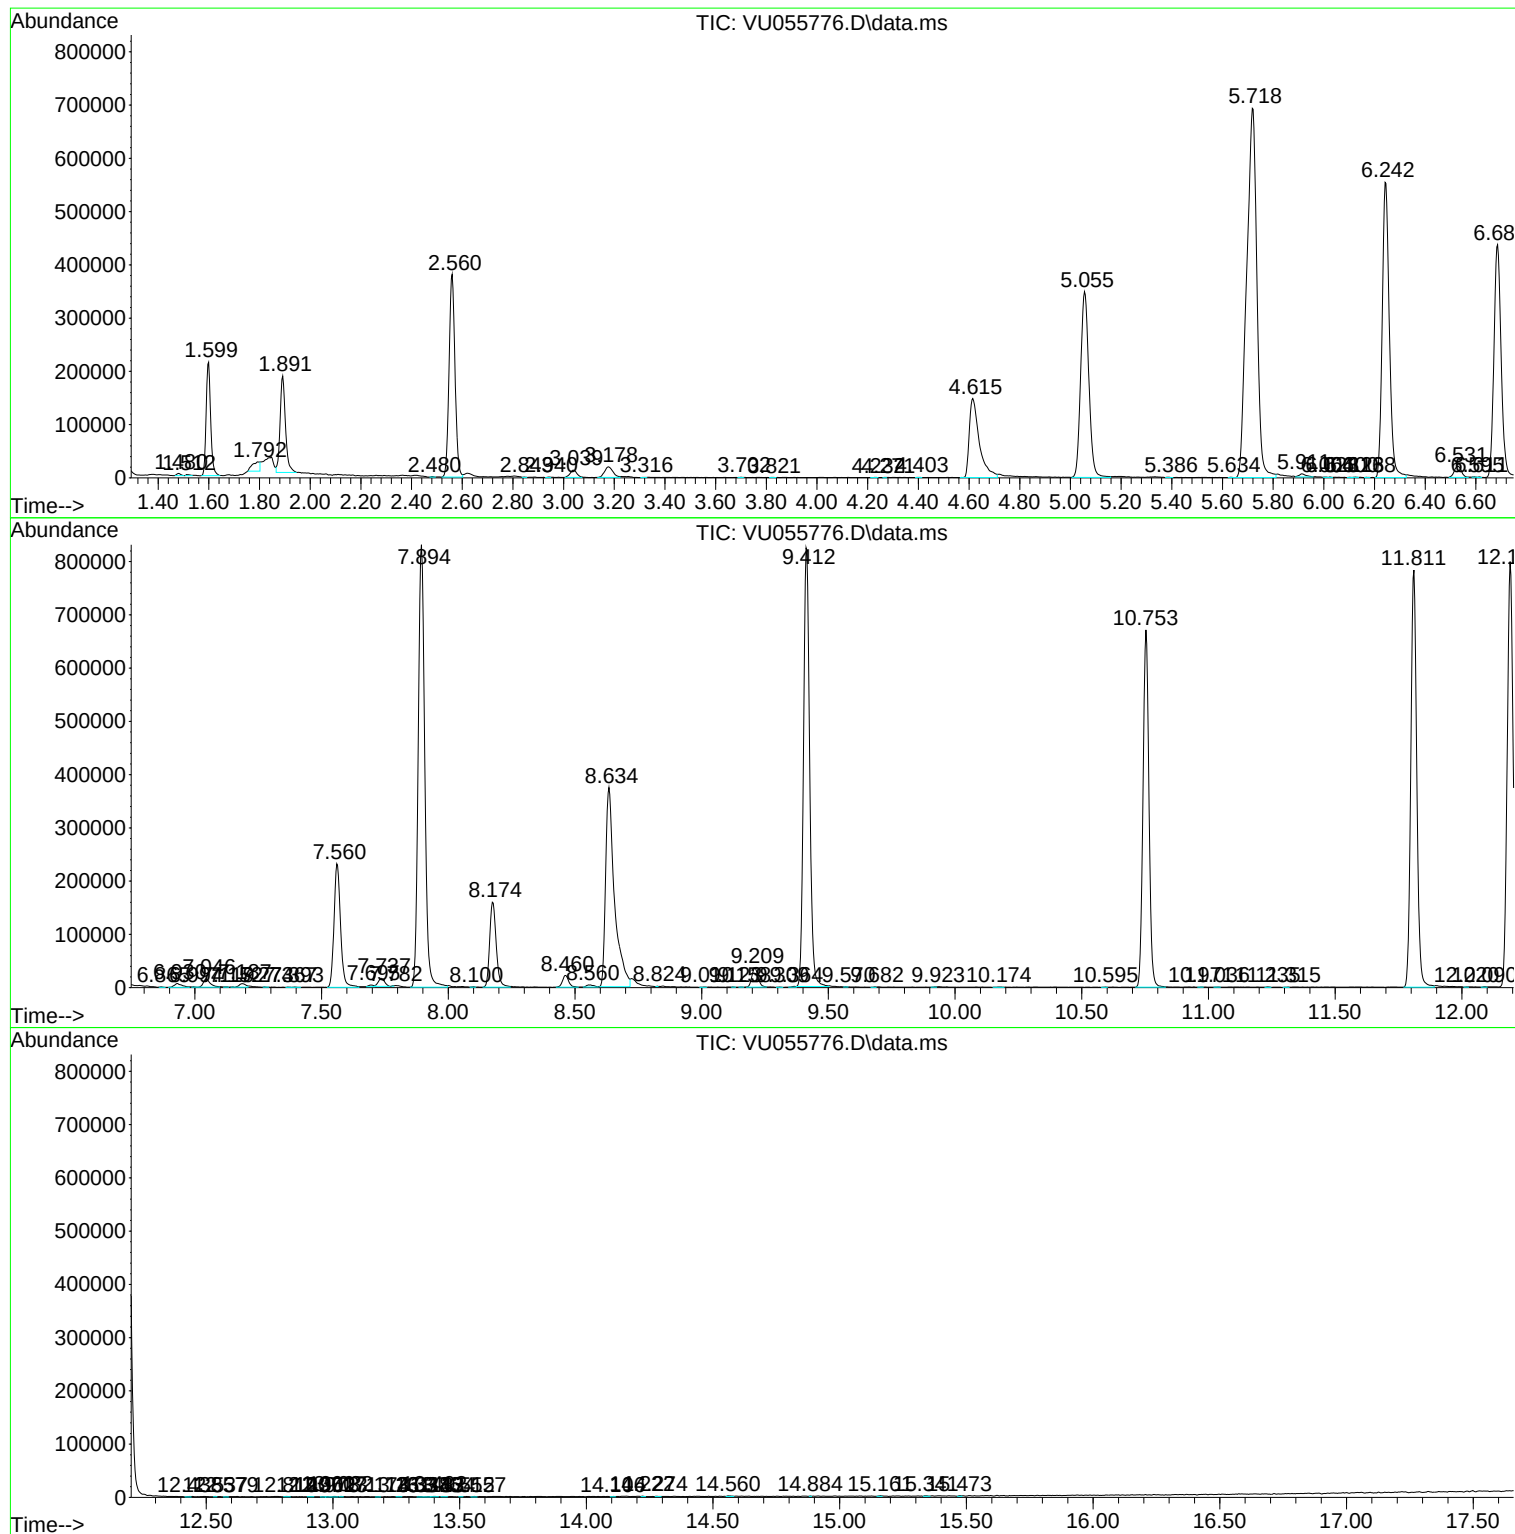

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055776.D
Acq On : 16 Oct 2023 16:49
Operator : MD/SY
Sample : 04874-04 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055776.D
Acq On : 16 Oct 2023 16:49
Operator : MD/SY
Sample : 04874-04 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0M28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc