

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055777.D
 Acq On : 16 Oct 2023 17:13
 Operator : MD/SY
 Sample : 04874-05 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055777.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	118	rBV	220047	260725	13.75%	1.824%
2	1.772	140	150	152	rBV6	18449	27954	1.47%	0.196%
3	1.891	180	187	207	rVB	178350	259881	13.71%	1.818%
4	2.464	364	365	369	rBV2	431	346	0.02%	0.002%
5	2.560	383	395	412	rBV	383073	624296	32.93%	4.368%
6	2.846	480	484	487	rBV3	588	403	0.02%	0.003%
7	2.952	513	517	522	rVB2	632	589	0.03%	0.004%
8	3.039	534	544	554	rBV2	8713	15422	0.81%	0.108%
9	3.107	562	565	570	rVB2	378	292	0.02%	0.002%
10	3.177	573	587	611	rBV	17841	45511	2.40%	0.318%
11	3.316	627	630	636	rVB3	394	395	0.02%	0.003%
12	3.579	709	712	716	rVB2	387	318	0.02%	0.002%
13	3.631	725	728	733	rVB3	500	379	0.02%	0.003%
14	3.669	737	740	744	rBV2	289	277	0.01%	0.002%
15	3.743	759	763	766	rBV	382	286	0.02%	0.002%
16	3.791	773	778	779	rBV2	370	286	0.02%	0.002%
17	3.853	792	797	802	rVV2	334	419	0.02%	0.003%
18	3.878	802	805	810	rVV	480	337	0.02%	0.002%
19	3.904	810	813	816	rVV2	698	465	0.02%	0.003%
20	4.010	843	846	849	rBV	277	265	0.01%	0.002%
21	4.274	923	928	931	rBV2	314	278	0.01%	0.002%
22	4.293	931	934	942	rVB2	234	269	0.01%	0.002%
23	4.332	942	946	951	rVB2	458	369	0.02%	0.003%
24	4.492	991	996	1001	rBV2	260	292	0.02%	0.002%
25	4.615	1023	1034	1066	rBV	136997	379052	19.99%	2.652%
26	4.888	1116	1119	1122	rBV2	526	359	0.02%	0.003%
27	5.004	1152	1155	1156	rBV3	559	344	0.02%	0.002%
28	5.055	1156	1171	1195	rVV	347689	775177	40.88%	5.423%
29	5.264	1234	1236	1242	rVB2	511	372	0.02%	0.003%
30	5.290	1242	1244	1249	rBV4	635	478	0.03%	0.003%
31	5.325	1249	1255	1257	rBV4	903	1061	0.06%	0.007%
32	5.531	1314	1319	1321	rBV3	443	365	0.02%	0.003%
33	5.640	1348	1353	1356	rBV2	365	346	0.02%	0.002%
34	5.721	1356	1378	1408	rBV2	681757	1895995	100.00%	13.264%
35	5.968	1450	1455	1458	rBV3	686	681	0.04%	0.005%
36	6.004	1464	1466	1469	rVB4	583	307	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055777.D
 Acq On : 16 Oct 2023 17:13
 Operator : MD/SY
 Sample : 04874-05 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.074	1485	1488	1493	rBV3	402	256	0.01%	0.002%
38	6.106	1493	1498	1499	rBV3	497	349	0.02%	0.002%
39	6.245	1526	1541	1564	rBV	544036	1059840	55.90%	7.415%
40	6.460	1605	1608	1612	rBV3	729	656	0.03%	0.005%
41	6.524	1618	1628	1643	rBV3	23584	45022	2.37%	0.315%
42	6.685	1664	1678	1705	rBV	427537	859153	45.31%	6.011%
43	6.881	1736	1739	1741	rVB3	497	292	0.02%	0.002%
44	7.004	1772	1777	1779	rBV	296	270	0.01%	0.002%
45	7.100	1803	1807	1811	rBV2	334	266	0.01%	0.002%
46	7.190	1824	1835	1850	rBV4	6179	14442	0.76%	0.101%
47	7.245	1850	1852	1857	rVB4	738	586	0.03%	0.004%
48	7.486	1923	1927	1931	rBV3	506	384	0.02%	0.003%
49	7.563	1938	1951	1976	rBV	222248	405332	21.38%	2.836%
50	7.698	1985	1993	1996	rBV5	2821	3421	0.18%	0.024%
51	7.798	2023	2024	2028	rVB	463	265	0.01%	0.002%
52	7.894	2038	2054	2085	rBV	830442	1460512	77.03%	10.218%
53	8.174	2130	2141	2170	rVV	157451	273125	14.41%	1.911%
54	8.389	2204	2208	2210	rBV	318	274	0.01%	0.002%
55	8.463	2226	2231	2235	rBV3	605	640	0.03%	0.004%
56	8.486	2235	2238	2242	rVV3	324	270	0.01%	0.002%
57	8.634	2272	2284	2327	rBV3	327729	836902	44.14%	5.855%
58	8.830	2342	2345	2347	rBV2	695	484	0.03%	0.003%
59	8.897	2364	2366	2370	rVB3	719	476	0.03%	0.003%
60	8.917	2370	2372	2375	rBV3	539	293	0.02%	0.002%
61	9.010	2398	2401	2402	rBV2	440	290	0.02%	0.002%
62	9.048	2411	2413	2416	rVB2	619	282	0.01%	0.002%
63	9.212	2454	2464	2467	rBV4	1384	1789	0.09%	0.013%
64	9.415	2514	2527	2553	rBV	810831	1379608	72.76%	9.652%
65	9.569	2572	2575	2576	rBV2	618	328	0.02%	0.002%
66	10.023	2712	2716	2719	rVV2	555	533	0.03%	0.004%
67	10.103	2738	2741	2744	rBV2	384	307	0.02%	0.002%
68	10.132	2747	2750	2754	rVB3	463	373	0.02%	0.003%
69	10.174	2759	2763	2766	rVV2	490	344	0.02%	0.002%
70	10.216	2771	2776	2783	rVB2	384	505	0.03%	0.004%
71	10.450	2844	2849	2852	rVV	560	484	0.03%	0.003%
72	10.528	2871	2873	2880	rVB2	371	288	0.02%	0.002%
73	10.618	2899	2901	2910	rVB2	420	543	0.03%	0.004%
74	10.753	2928	2943	2963	rBV	635198	1038055	54.75%	7.262%
75	10.904	2987	2990	2994	rVB2	458	326	0.02%	0.002%
76	10.942	2998	3002	3005	rBV2	417	409	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055777.D
 Acq On : 16 Oct 2023 17:13
 Operator : MD/SY
 Sample : 04874-05 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.032	3027	3030	3033	rBV2	385	330	0.02%	0.002%
78	11.364	3130	3133	3136	rBV2	347	332	0.02%	0.002%
79	11.566	3192	3196	3198	rBV	858	347	0.02%	0.002%
80	11.675	3226	3230	3231	rBV	361	267	0.01%	0.002%
81	11.730	3242	3247	3250	rBV2	508	405	0.02%	0.003%
82	11.753	3251	3254	3258	rBV2	335	320	0.02%	0.002%
83	11.810	3259	3272	3299	rBV	780415	1272573	67.12%	8.903%
84	12.026	3337	3339	3343	rVB3	557	335	0.02%	0.002%
85	12.103	3359	3363	3367	rBV4	512	534	0.03%	0.004%
86	12.190	3375	3390	3419	rBV	786462	1328838	70.09%	9.296%
87	12.376	3446	3448	3451	rVB2	767	394	0.02%	0.003%
88	12.399	3451	3455	3459	rBV4	466	486	0.03%	0.003%
89	12.708	3548	3551	3553	rBV	475	318	0.02%	0.002%
90	12.769	3568	3570	3572	rVB2	777	374	0.02%	0.003%
91	12.852	3592	3596	3601	rBV3	577	673	0.04%	0.005%
92	13.138	3682	3685	3687	rVB2	522	281	0.01%	0.002%
93	13.238	3713	3716	3718	rBV2	489	324	0.02%	0.002%
94	13.277	3724	3728	3730	rBV3	399	376	0.02%	0.003%
95	13.833	3897	3901	3904	rBV3	690	710	0.04%	0.005%
96	14.235	4022	4026	4028	rBV2	462	357	0.02%	0.002%
97	14.518	4111	4114	4116	rBV2	936	504	0.03%	0.004%
98	15.132	4301	4305	4309	rBV5	1044	1099	0.06%	0.008%
99	15.228	4333	4335	4339	rVB2	1146	666	0.04%	0.005%
100	15.576	4441	4443	4446	rBV3	926	628	0.03%	0.004%


Sum of corrected areas: 14294036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055777.D
Acq On : 16 Oct 2023 17:13
Operator : MD/SY
Sample : 04874-05 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

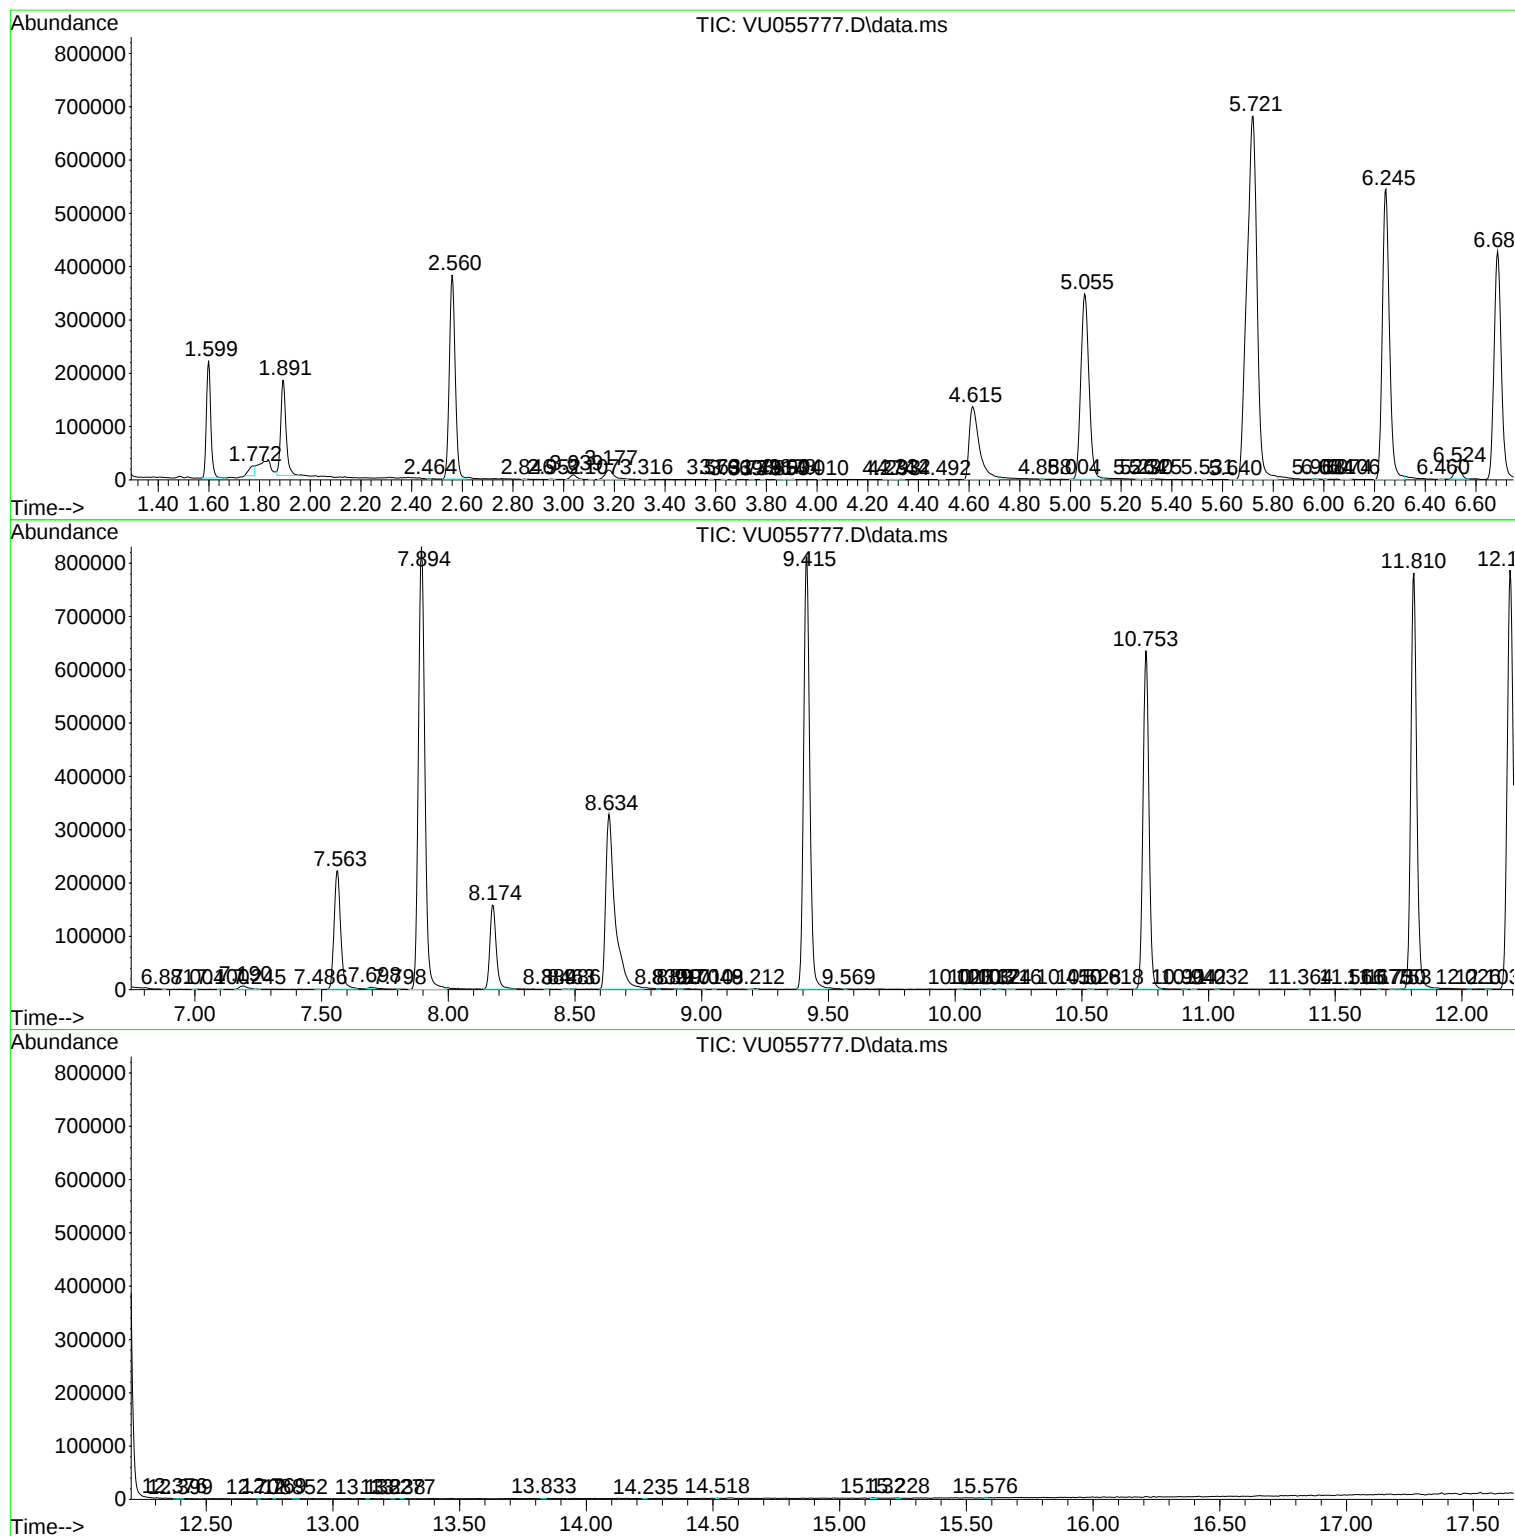

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055777.D
Acq On : 16 Oct 2023 17:13
Operator : MD/SY
Sample : 04874-05 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055777.D
Acq On : 16 Oct 2023 17:13
Operator : MD/SY
Sample : 04874-05 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------