

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055779.D
 Acq On : 16 Oct 2023 18:02
 Operator : MD/SY
 Sample : 04874-07 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.483	55	60	66	rBV3	3717	3884	0.21%	0.028%
2	1.599	88	96	114	rBV	207763	245241	13.54%	1.786%
3	1.788	140	155	156	rBV4	21806	45293	2.50%	0.330%
4	1.891	179	187	202	rVB	174193	248178	13.70%	1.808%
5	2.489	371	373	378	rVB3	565	421	0.02%	0.003%
6	2.560	382	395	419	rBV	364494	597941	33.00%	4.356%
7	2.734	447	449	453	rBV4	415	295	0.02%	0.002%
8	2.782	459	464	465	rBV4	631	536	0.03%	0.004%
9	2.856	484	487	493	rVB3	416	429	0.02%	0.003%
10	2.920	503	507	513	rBV3	344	467	0.03%	0.003%
11	3.039	534	544	557	rVB3	7075	12993	0.72%	0.095%
12	3.097	560	562	566	rBV3	603	350	0.02%	0.003%
13	3.177	573	587	610	rBV	19006	46808	2.58%	0.341%
14	3.386	650	652	657	rVV	327	310	0.02%	0.002%
15	3.531	693	697	700	rBV2	400	358	0.02%	0.003%
16	3.583	710	713	717	rVV2	397	283	0.02%	0.002%
17	3.718	752	755	764	rVB	502	574	0.03%	0.004%
18	3.766	764	770	772	rBV	350	379	0.02%	0.003%
19	4.091	867	871	874	rBV2	324	277	0.02%	0.002%
20	4.341	946	949	956	rBV2	247	267	0.01%	0.002%
21	4.570	1014	1020	1021	rBV	300	298	0.02%	0.002%
22	4.615	1022	1034	1068	rBV	134621	369623	20.40%	2.692%
23	5.055	1154	1171	1195	rBV	333139	748966	41.34%	5.456%
24	5.332	1246	1257	1259	rBV6	1254	2226	0.12%	0.016%
25	5.592	1334	1338	1343	rVB2	426	366	0.02%	0.003%
26	5.618	1343	1346	1351	rBV	411	410	0.02%	0.003%
27	5.718	1356	1377	1398	rBV2	656883	1811869	100.00%	13.198%
28	6.036	1473	1476	1486	rVB4	742	1093	0.06%	0.008%
29	6.132	1504	1506	1511	rVB2	455	388	0.02%	0.003%
30	6.242	1527	1540	1566	rBV	527766	1034626	57.10%	7.537%
31	6.528	1618	1629	1645	rVB4	22637	45958	2.54%	0.335%
32	6.595	1645	1650	1653	rBV6	1097	792	0.04%	0.006%
33	6.685	1663	1678	1698	rBV	416835	821121	45.32%	5.981%
34	6.878	1734	1738	1740	rBV2	654	298	0.02%	0.002%
35	6.907	1744	1747	1751	rVB	395	289	0.02%	0.002%
36	7.020	1778	1782	1785	rVB2	366	281	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055779.D
 Acq On : 16 Oct 2023 18:02
 Operator : MD/SY
 Sample : 04874-07 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.187	1824	1834	1846	rBV4	5505	11947	0.66%	0.087%
38	7.261	1852	1857	1861	rBV3	387	361	0.02%	0.003%
39	7.473	1918	1923	1927	rBV2	395	349	0.02%	0.003%
40	7.560	1938	1950	1980	rBV	212682	384527	21.22%	2.801%
41	7.692	1984	1991	2003	rVB6	2647	4967	0.27%	0.036%
42	7.782	2015	2019	2021	rBV2	474	274	0.02%	0.002%
43	7.811	2024	2028	2031	rVB4	712	537	0.03%	0.004%
44	7.894	2040	2054	2092	rBV	780840	1390545	76.75%	10.129%
45	8.132	2121	2128	2129	rBV3	500	481	0.03%	0.004%
46	8.174	2130	2141	2163	rVV	151144	257832	14.23%	1.878%
47	8.319	2183	2186	2188	rBV2	626	335	0.02%	0.002%
48	8.386	2201	2207	2209	rBV2	478	360	0.02%	0.003%
49	8.553	2255	2259	2263	rVB3	534	412	0.02%	0.003%
50	8.576	2263	2266	2270	rBV3	899	657	0.04%	0.005%
51	8.634	2270	2284	2321	rBV3	314067	813299	44.89%	5.924%
52	9.161	2446	2448	2450	rBV2	536	297	0.02%	0.002%
53	9.216	2462	2465	2470	rBV2	472	295	0.02%	0.002%
54	9.242	2470	2473	2480	rVB3	333	430	0.02%	0.003%
55	9.315	2492	2496	2501	rBV2	343	363	0.02%	0.003%
56	9.412	2513	2526	2553	rBV	762177	1313820	72.51%	9.570%
57	9.766	2634	2636	2643	rVB2	601	493	0.03%	0.004%
58	9.833	2653	2657	2660	rBV2	295	289	0.02%	0.002%
59	9.875	2664	2670	2675	rBV	556	629	0.03%	0.005%
60	9.997	2703	2708	2712	rBV2	518	480	0.03%	0.003%
61	10.020	2712	2715	2718	rBV	371	292	0.02%	0.002%
62	10.168	2757	2761	2766	rBV3	448	382	0.02%	0.003%
63	10.203	2768	2772	2776	rBV	293	278	0.02%	0.002%
64	10.550	2875	2880	2883	rBV2	487	479	0.03%	0.003%
65	10.592	2890	2893	2897	rVB3	404	315	0.02%	0.002%
66	10.627	2897	2904	2907	rBV2	510	655	0.04%	0.005%
67	10.753	2930	2943	2968	rBV	601661	984378	54.33%	7.171%
68	10.891	2984	2986	2993	rVB3	659	549	0.03%	0.004%
69	11.122	3056	3058	3065	rVV3	334	272	0.02%	0.002%
70	11.290	3107	3110	3114	rBV	387	302	0.02%	0.002%
71	11.399	3141	3144	3145	rVV	426	268	0.01%	0.002%
72	11.409	3145	3147	3151	rVB2	503	334	0.02%	0.002%
73	11.592	3201	3204	3210	rBV2	423	373	0.02%	0.003%
74	11.631	3212	3216	3219	rVV3	550	392	0.02%	0.003%
75	11.811	3259	3272	3292	rBV	736486	1220865	67.38%	8.893%
76	11.952	3313	3316	3317	rBV2	623	294	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055779.D
 Acq On : 16 Oct 2023 18:02
 Operator : MD/SY
 Sample : 04874-07 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COM31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	12.055	3346	3348	3355	rVB6	969	1000	0.06%	0.007%
78	12.090	3355	3359	3363	rBV3	474	548	0.03%	0.004%
79	12.190	3376	3390	3410	rBV	757625	1275358	70.39%	9.290%
80	12.396	3452	3454	3459	rVB3	782	559	0.03%	0.004%
81	12.479	3474	3480	3484	rBV4	684	931	0.05%	0.007%
82	12.630	3525	3527	3532	rVB	476	312	0.02%	0.002%
83	12.688	3540	3545	3548	rBV3	680	717	0.04%	0.005%
84	12.862	3593	3599	3606	rBV3	490	726	0.04%	0.005%
85	12.997	3638	3641	3644	rBV2	602	508	0.03%	0.004%
86	13.087	3664	3669	3671	rBV2	497	471	0.03%	0.003%
87	13.100	3671	3673	3677	rVB2	634	438	0.02%	0.003%
88	13.167	3692	3694	3698	rVB2	513	269	0.01%	0.002%
89	13.261	3719	3723	3725	rBV2	486	406	0.02%	0.003%
90	13.335	3743	3746	3748	rBV3	463	312	0.02%	0.002%
91	13.470	3785	3788	3789	rBV	691	369	0.02%	0.003%
92	13.573	3817	3820	3823	rBV2	612	405	0.02%	0.003%
93	14.232	4023	4025	4030	rVB3	593	467	0.03%	0.003%
94	14.267	4033	4036	4039	rBV	474	380	0.02%	0.003%
95	14.499	4104	4108	4110	rBV3	686	479	0.03%	0.003%
96	14.576	4120	4132	4135	rBV4	1510	2561	0.14%	0.019%
97	14.666	4157	4160	4162	rBV	664	455	0.03%	0.003%
98	15.055	4278	4281	4285	rBV5	984	626	0.03%	0.005%
99	15.154	4310	4312	4319	rVB2	918	808	0.04%	0.006%
100	15.489	4413	4416	4418	rBV3	840	648	0.04%	0.005%




Sum of corrected areas: 13728048

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055779.D
Acq On : 16 Oct 2023 18:02
Operator : MD/SY
Sample : 04874-07 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

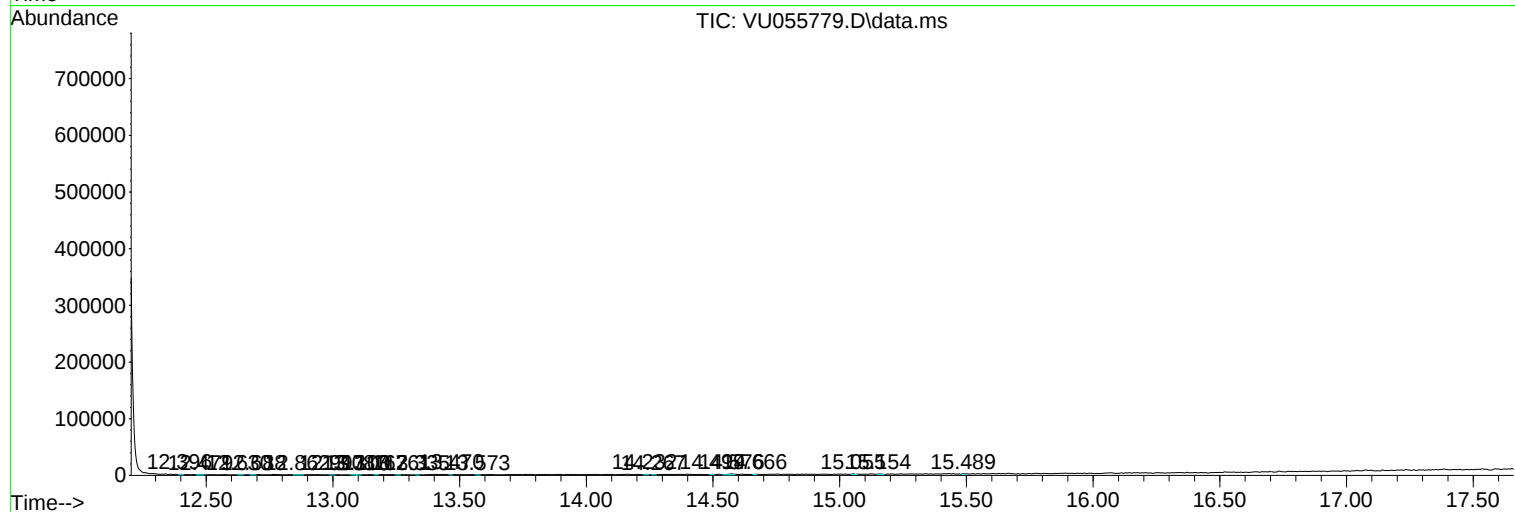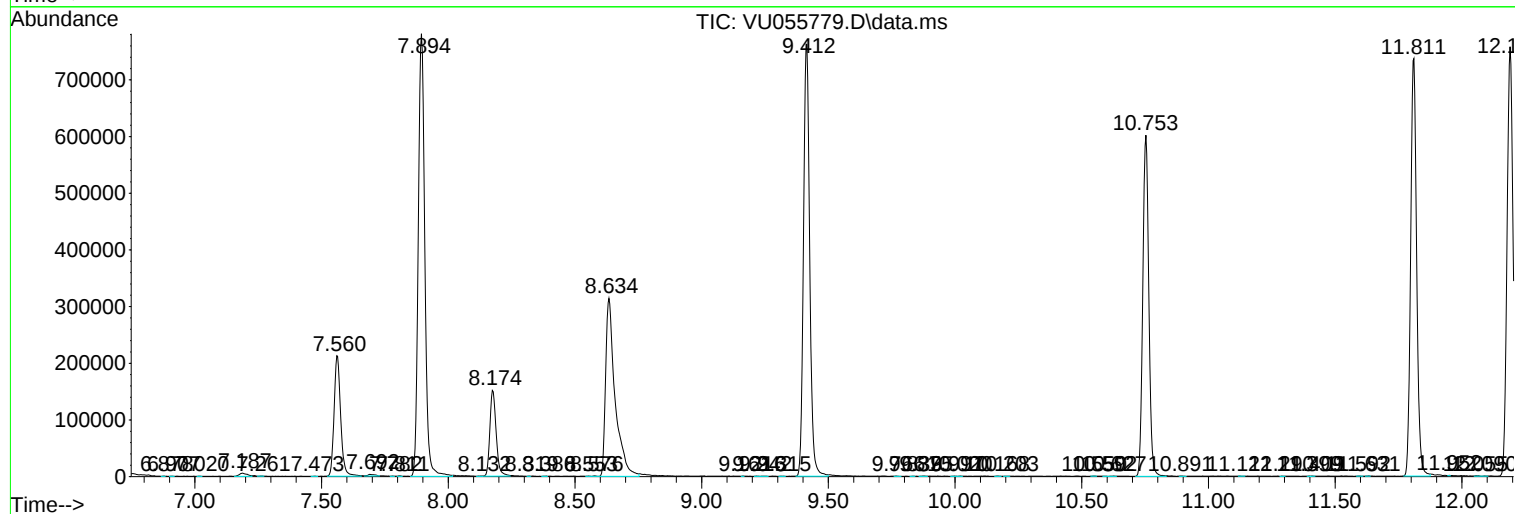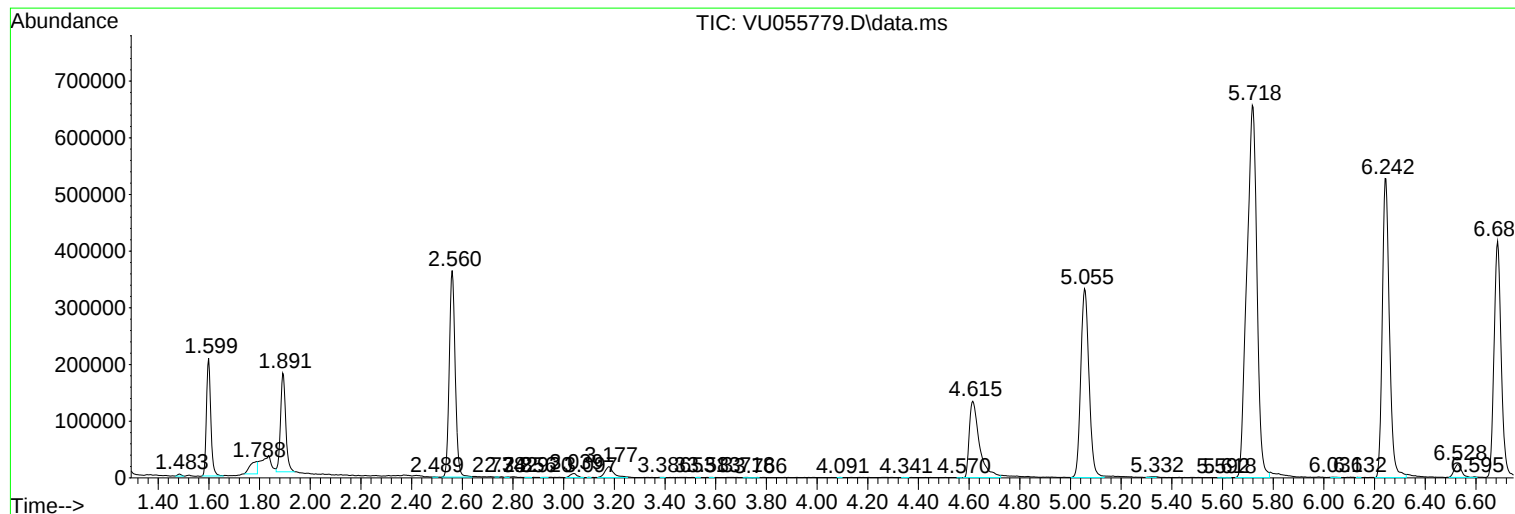

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055779.D
Acq On : 16 Oct 2023 18:02
Operator : MD/SY
Sample : 04874-07 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055779.D
Acq On : 16 Oct 2023 18:02
Operator : MD/SY
Sample : 04874-07 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COM31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc