

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055781.D
 Acq On : 16 Oct 2023 18:50
 Operator : MD/SY
 Sample : 04824-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	112	rBV	223001	273912	13.78%	1.897%
2	2.557	382	394	412	rBV	402613	652271	32.81%	4.516%
3	3.039	533	544	554	rBV5	4792	8735	0.44%	0.060%
4	3.094	559	561	564	rBV2	394	229	0.01%	0.002%
5	3.113	564	567	569	rVB	466	224	0.01%	0.002%
6	3.155	576	580	581	rBV2	666	431	0.02%	0.003%
7	3.377	647	649	653	rBV	344	197	0.01%	0.001%
8	3.467	673	677	680	rBV3	578	466	0.02%	0.003%
9	3.528	691	696	701	rBV2	401	318	0.02%	0.002%
10	3.628	725	727	729	rBV	334	163	0.01%	0.001%
11	3.856	795	798	800	rVB	135	71	0.00%	0.000%
12	3.927	817	820	821	rBV	267	141	0.01%	0.001%
13	3.962	827	831	832	rBV	280	179	0.01%	0.001%
14	4.107	873	876	878	rBV	200	109	0.01%	0.001%
15	4.168	893	895	900	rVB	274	210	0.01%	0.001%
16	4.190	900	902	903	rBV	159	77	0.00%	0.001%
17	4.232	912	915	916	rBV	114	61	0.00%	0.000%
18	4.367	954	957	958	rBV2	118	66	0.00%	0.000%
19	4.486	989	994	998	rBV	251	275	0.01%	0.002%
20	4.509	998	1001	1002	rVV	241	134	0.01%	0.001%
21	4.534	1006	1009	1010	rBV2	297	168	0.01%	0.001%
22	4.567	1017	1019	1020	rBV	238	69	0.00%	0.000%
23	4.615	1023	1034	1072	rBV	142245	399500	20.09%	2.766%
24	5.055	1150	1171	1191	rBV	366426	810640	40.77%	5.613%
25	5.312	1248	1251	1252	rBV2	715	466	0.02%	0.003%
26	5.399	1276	1278	1280	rBV	256	126	0.01%	0.001%
27	5.422	1281	1285	1289	rVB2	393	309	0.02%	0.002%
28	5.467	1297	1299	1304	rBV2	111	99	0.00%	0.001%
29	5.528	1315	1318	1319	rBV2	333	189	0.01%	0.001%
30	5.718	1355	1377	1406	rBV2	723850	1988243	100.00%	13.766%
31	6.033	1471	1475	1478	rBV4	612	551	0.03%	0.004%
32	6.110	1497	1499	1501	rBV3	297	113	0.01%	0.001%
33	6.123	1501	1503	1507	rVV2	664	366	0.02%	0.003%
34	6.165	1513	1516	1519	rBV2	233	193	0.01%	0.001%
35	6.242	1526	1540	1571	rBV	553972	1077237	54.18%	7.459%
36	6.464	1607	1609	1611	rBV2	601	292	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055781.D
 Acq On : 16 Oct 2023 18:50
 Operator : MD/SY
 Sample : 04824-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.528	1618	1629	1642	rBV3	21587	41940	2.11%	0.290%
38	6.685	1662	1678	1701	rBV	447897	893565	44.94%	6.187%
39	6.878	1736	1738	1740	rBV	275	101	0.01%	0.001%
40	6.911	1746	1748	1751	rVB2	442	187	0.01%	0.001%
41	6.939	1755	1757	1760	rBV2	426	272	0.01%	0.002%
42	6.981	1767	1770	1775	rBV	439	381	0.02%	0.003%
43	7.062	1792	1795	1801	rVB2	764	443	0.02%	0.003%
44	7.139	1818	1819	1823	rVB	283	109	0.01%	0.001%
45	7.190	1823	1835	1852	rBV4	6798	16388	0.82%	0.113%
46	7.367	1886	1890	1893	rBV2	242	187	0.01%	0.001%
47	7.422	1902	1907	1911	rBV	321	380	0.02%	0.003%
48	7.560	1938	1950	1984	rBV	234425	425535	21.40%	2.946%
49	7.788	2019	2021	2025	rBV2	483	334	0.02%	0.002%
50	7.894	2039	2054	2079	rBV	864085	1533736	77.14%	10.619%
51	8.174	2130	2141	2164	rBV	162842	286914	14.43%	1.987%
52	8.341	2191	2193	2197	rBB3	623	365	0.02%	0.003%
53	8.364	2197	2200	2201	rBV	441	224	0.01%	0.002%
54	8.390	2207	2208	2210	rBV	330	130	0.01%	0.001%
55	8.492	2237	2240	2243	rBV2	326	290	0.01%	0.002%
56	8.525	2248	2250	2253	rBV2	323	172	0.01%	0.001%
57	8.541	2253	2255	2256	rBV	398	174	0.01%	0.001%
58	8.573	2263	2265	2267	rVB	401	187	0.01%	0.001%
59	8.592	2267	2271	2272	rBV2	220	133	0.01%	0.001%
60	8.637	2272	2285	2321	rBV3	340945	880258	44.27%	6.095%
61	9.013	2400	2402	2406	rVB3	392	230	0.01%	0.002%
62	9.197	2456	2459	2460	rBV	557	256	0.01%	0.002%
63	9.312	2493	2495	2497	rBV	343	178	0.01%	0.001%
64	9.412	2514	2526	2553	rBV	823155	1397211	70.27%	9.674%
65	9.689	2606	2612	2613	rBV2	624	490	0.02%	0.003%
66	9.766	2633	2636	2641	rVB4	627	468	0.02%	0.003%
67	9.817	2651	2652	2654	rBV	270	129	0.01%	0.001%
68	9.830	2654	2656	2658	rVV	494	228	0.01%	0.002%
69	10.090	2735	2737	2740	rBV	217	140	0.01%	0.001%
70	10.148	2752	2755	2757	rBV2	376	222	0.01%	0.002%
71	10.161	2757	2759	2762	rVV	347	162	0.01%	0.001%
72	10.209	2772	2774	2777	rBV	338	180	0.01%	0.001%
73	10.364	2820	2822	2824	rBV	323	204	0.01%	0.001%
74	10.457	2849	2851	2856	rVB	320	125	0.01%	0.001%
75	10.698	2922	2926	2930	rBV2	345	312	0.02%	0.002%
76	10.753	2930	2943	2969	rBV	661551	1095760	55.11%	7.587%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055781.D
Acq On : 16 Oct 2023 18:50
Operator : MD/SY
Sample : 04824-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Title : VOC Analysis

77	11.727	3243	3246	3250	rBV	551	401	0.02%	0.003%
78	11.811	3255	3272	3299	rBV	781639	1277138	64.23%	8.843%
79	12.190	3377	3390	3412	rBV	823432	1369564	68.88%	9.483%
80	12.537	3496	3498	3501	rBV	454	304	0.02%	0.002%




Sum of corrected areas: 14442937

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055781.D
Acq On : 16 Oct 2023 18:50
Operator : MD/SY
Sample : 04824-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

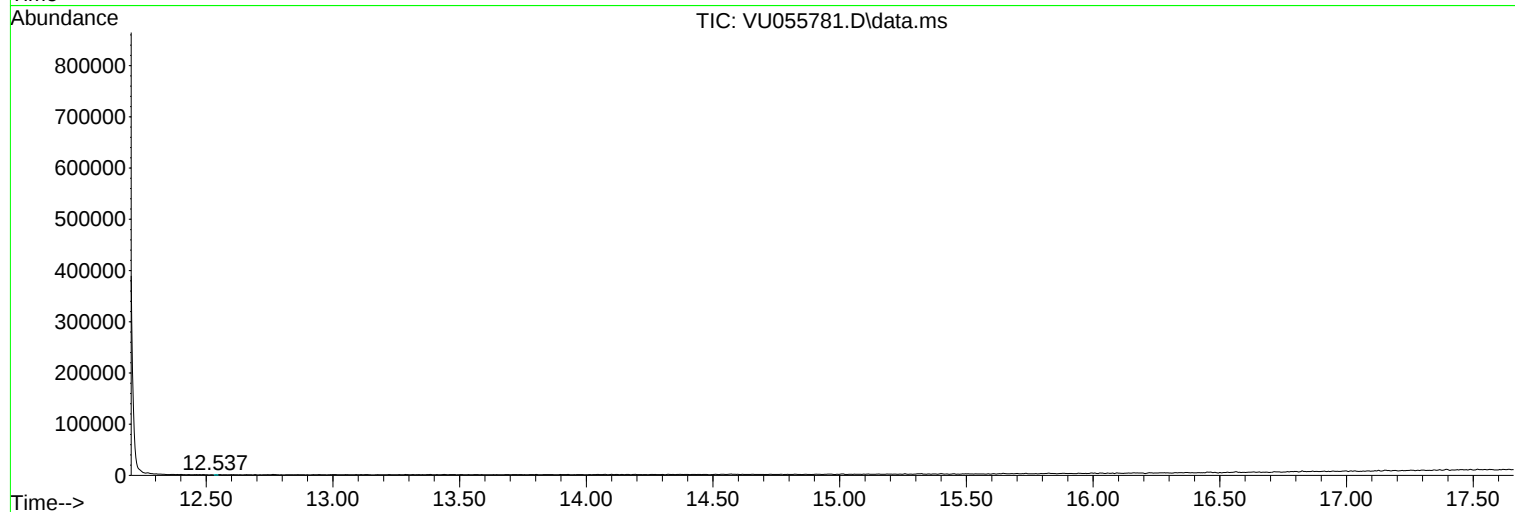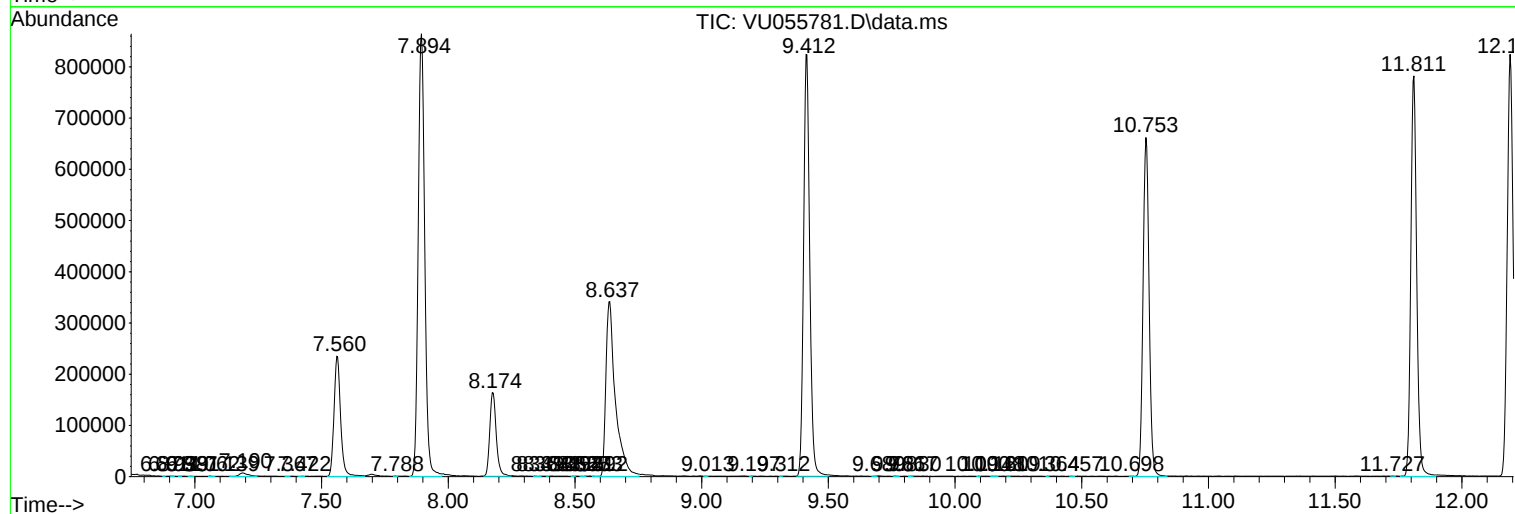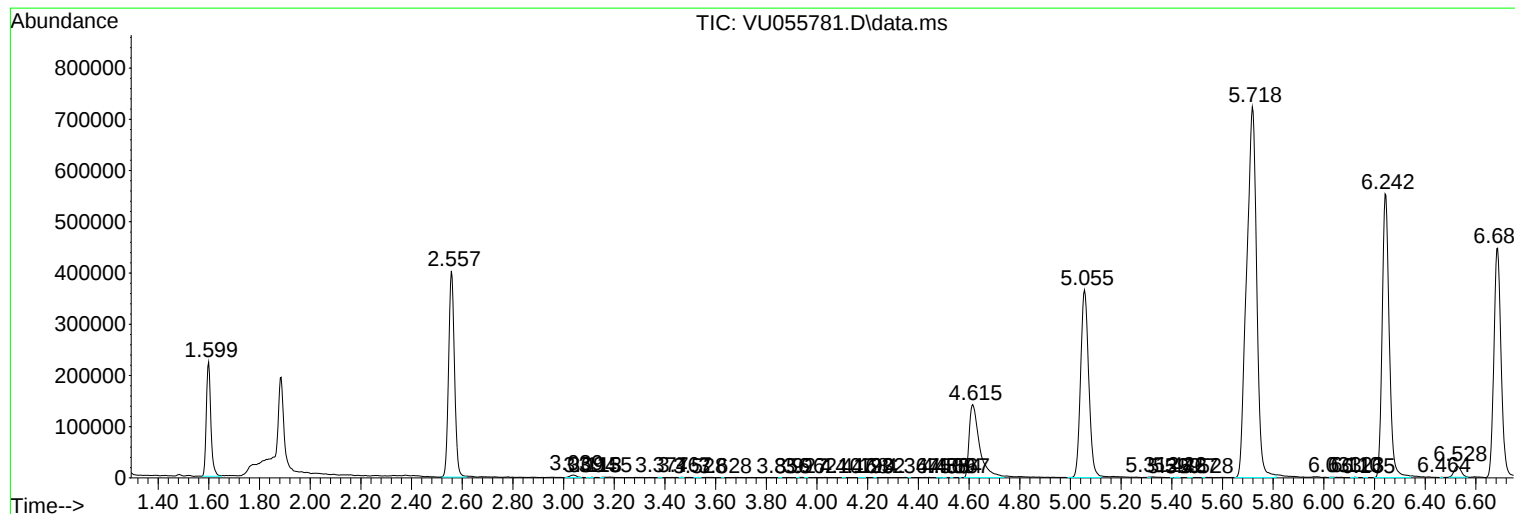

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055781.D
Acq On : 16 Oct 2023 18:50
Operator : MD/SY
Sample : 04824-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055781.D
Acq On : 16 Oct 2023 18:50
Operator : MD/SY
Sample : 04824-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------