

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055782.D
 Acq On : 16 Oct 2023 19:14
 Operator : MD/SY
 Sample : 04852-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055782.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	116	rBV	213856	257840	13.56%	1.826%
2	1.888	180	186	204	rVB	177446	258363	13.59%	1.829%
3	2.560	383	395	413	rBV	379529	624277	32.83%	4.420%
4	3.007	530	534	535	rBV2	571	365	0.02%	0.003%
5	3.039	537	544	555	rVB2	4745	7818	0.41%	0.055%
6	3.145	574	577	579	rBV	456	330	0.02%	0.002%
7	3.242	604	607	609	rBV2	444	274	0.01%	0.002%
8	3.267	613	615	618	rBV	194	102	0.01%	0.001%
9	3.345	638	639	640	rBV	171	53	0.00%	0.000%
10	3.367	643	646	648	rVV2	149	91	0.00%	0.001%
11	3.422	659	663	666	rVB2	270	176	0.01%	0.001%
12	3.444	666	670	671	rBV	216	140	0.01%	0.001%
13	3.515	690	692	694	rBV	177	94	0.00%	0.001%
14	3.531	694	697	698	rBV2	346	171	0.01%	0.001%
15	3.685	743	745	746	rBV	351	116	0.01%	0.001%
16	3.766	767	770	773	rVB2	207	126	0.01%	0.001%
17	3.830	786	790	792	rBV	238	151	0.01%	0.001%
18	3.859	797	799	802	rVB2	530	261	0.01%	0.002%
19	3.875	802	804	808	rBV	162	112	0.01%	0.001%
20	3.939	822	824	826	rBV	241	135	0.01%	0.001%
21	4.017	842	848	853	rBV2	264	335	0.02%	0.002%
22	4.139	883	886	888	rBV2	223	164	0.01%	0.001%
23	4.190	899	902	905	rVB	453	229	0.01%	0.002%
24	4.209	905	908	912	rBV2	153	79	0.00%	0.001%
25	4.290	930	933	937	rVB2	272	156	0.01%	0.001%
26	4.309	937	939	943	rVB2	151	84	0.00%	0.001%
27	4.332	943	946	950	rBV3	341	309	0.02%	0.002%
28	4.357	952	954	959	rVB2	381	256	0.01%	0.002%
29	4.422	970	974	977	rVB2	378	231	0.01%	0.002%
30	4.447	980	982	984	rBV2	210	112	0.01%	0.001%
31	4.499	992	998	1000	rBV2	170	193	0.01%	0.001%
32	4.525	1003	1006	1008	rBV2	164	97	0.01%	0.001%
33	4.615	1023	1034	1070	rBV	141762	399095	20.99%	2.826%
34	4.949	1136	1138	1142	rVB2	595	343	0.02%	0.002%
35	4.988	1147	1150	1151	rBV	385	172	0.01%	0.001%
36	5.055	1156	1171	1196	rBV	349497	777017	40.86%	5.502%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055782.D
 Acq On : 16 Oct 2023 19:14
 Operator : MD/SY
 Sample : 04852-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	5.280	1240	1241	1245	rBV2	205	119	0.01%	0.001%
38	5.303	1246	1248	1250	rBV	563	256	0.01%	0.002%
39	5.425	1284	1286	1289	rBV2	261	190	0.01%	0.001%
40	5.463	1295	1298	1299	rBV	389	162	0.01%	0.001%
41	5.499	1305	1309	1310	rBV	299	215	0.01%	0.002%
42	5.602	1339	1341	1344	rVB	188	74	0.00%	0.001%
43	5.615	1344	1345	1346	rBV	358	102	0.01%	0.001%
44	5.717	1356	1377	1404	rBV2	690861	1901717	100.00%	13.466%
45	6.004	1464	1466	1468	rVB2	524	206	0.01%	0.001%
46	6.100	1493	1496	1497	rBV2	405	165	0.01%	0.001%
47	6.113	1497	1500	1502	rBV3	286	234	0.01%	0.002%
48	6.193	1521	1525	1527	rBV2	435	303	0.02%	0.002%
49	6.242	1527	1540	1585	rVV	518281	1030763	54.20%	7.299%
50	6.528	1618	1629	1644	rBV2	22797	44083	2.32%	0.312%
51	6.685	1663	1678	1700	rBV	435025	856523	45.04%	6.065%
52	6.891	1738	1742	1745	rVB2	455	309	0.02%	0.002%
53	6.907	1745	1747	1748	rBV	212	85	0.00%	0.001%
54	6.930	1752	1754	1758	rVB2	309	194	0.01%	0.001%
55	6.952	1758	1761	1763	rBV	188	131	0.01%	0.001%
56	6.965	1763	1765	1767	rVB	328	146	0.01%	0.001%
57	7.039	1785	1788	1792	rBV2	259	169	0.01%	0.001%
58	7.097	1805	1806	1807	rBV2	184	67	0.00%	0.000%
59	7.187	1825	1834	1841	rBV4	6448	11490	0.60%	0.081%
60	7.312	1868	1873	1874	rBV	258	159	0.01%	0.001%
61	7.332	1875	1879	1882	rVB2	480	292	0.02%	0.002%
62	7.351	1883	1885	1888	rVB	294	140	0.01%	0.001%
63	7.370	1888	1891	1893	rBV2	208	90	0.00%	0.001%
64	7.396	1897	1899	1900	rBV2	243	96	0.01%	0.001%
65	7.441	1910	1913	1915	rBV2	203	156	0.01%	0.001%
66	7.508	1933	1934	1937	rBV	246	150	0.01%	0.001%
67	7.560	1939	1950	1983	rVV	223731	408791	21.50%	2.895%
68	7.804	2024	2026	2027	rBV	180	67	0.00%	0.000%
69	7.836	2034	2036	2038	rVB2	341	140	0.01%	0.001%
70	7.894	2038	2054	2087	rBV	832750	1458624	76.70%	10.328%
71	8.126	2124	2126	2128	rBV	353	171	0.01%	0.001%
72	8.174	2130	2141	2165	rVV	156808	277177	14.58%	1.963%
73	8.338	2189	2192	2196	rBV2	511	501	0.03%	0.004%
74	8.396	2208	2210	2213	rBV	274	174	0.01%	0.001%
75	8.457	2224	2229	2231	rBV	385	364	0.02%	0.003%
76	8.586	2266	2269	2271	rBV	459	232	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
 Data File : VU055782.D
 Acq On : 16 Oct 2023 19:14
 Operator : MD/SY
 Sample : 04852-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	8.634	2273	2284	2323	rVV2	335843	871451	45.82%	6.171%
78	8.946	2377	2381	2385	rBV4	806	609	0.03%	0.004%
79	9.248	2472	2475	2481	rVB2	433	422	0.02%	0.003%
80	9.322	2495	2498	2499	rBV	323	152	0.01%	0.001%
81	9.412	2514	2526	2572	rBV	775498	1333279	70.11%	9.441%
82	9.582	2576	2579	2581	rBV3	553	284	0.01%	0.002%
83	9.692	2610	2613	2616	rBV2	679	576	0.03%	0.004%
84	9.733	2623	2626	2627	rBV	260	111	0.01%	0.001%
85	9.794	2642	2645	2648	rVV2	338	191	0.01%	0.001%
86	9.811	2648	2650	2653	rVB2	264	79	0.00%	0.001%
87	10.142	2747	2753	2757	rBV2	512	497	0.03%	0.004%
88	10.190	2766	2768	2772	rBV2	288	195	0.01%	0.001%
89	10.248	2784	2786	2787	rBV	289	81	0.00%	0.001%
90	10.306	2802	2804	2805	rBV	180	72	0.00%	0.001%
91	10.338	2812	2814	2817	rBV2	234	114	0.01%	0.001%
92	10.753	2927	2943	2962	rBV	650391	1063126	55.90%	7.528%
93	10.923	2994	2996	3001	rVB2	563	326	0.02%	0.002%
94	10.946	3001	3003	3005	rBV	219	114	0.01%	0.001%
95	11.065	3038	3040	3044	rBV2	238	113	0.01%	0.001%
96	11.138	3059	3063	3067	rBV2	498	479	0.03%	0.003%
97	11.158	3067	3069	3072	rVB	403	170	0.01%	0.001%
98	11.810	3259	3272	3289	rBV	741827	1207506	63.50%	8.550%
99	12.190	3377	3390	3414	rBV	790923	1317164	69.26%	9.327%
100	13.196	3701	3703	3706	rBV2	511	355	0.02%	0.003%




Sum of corrected areas: 14122360

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055782.D
Acq On : 16 Oct 2023 19:14
Operator : MD/SY
Sample : 04852-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

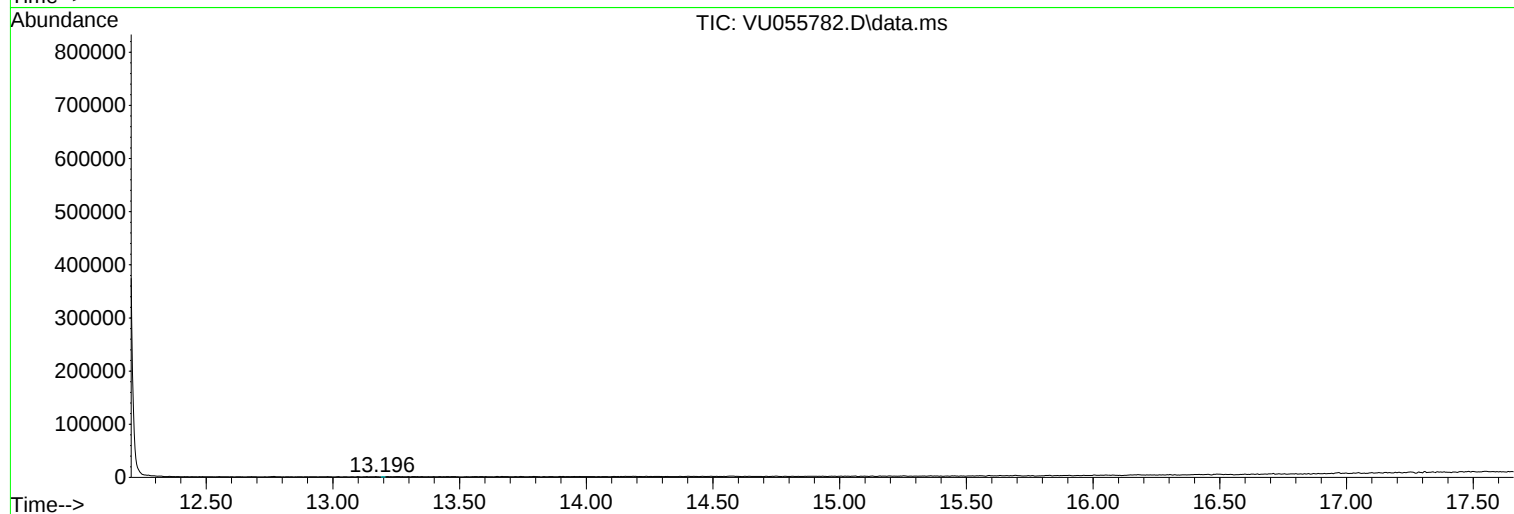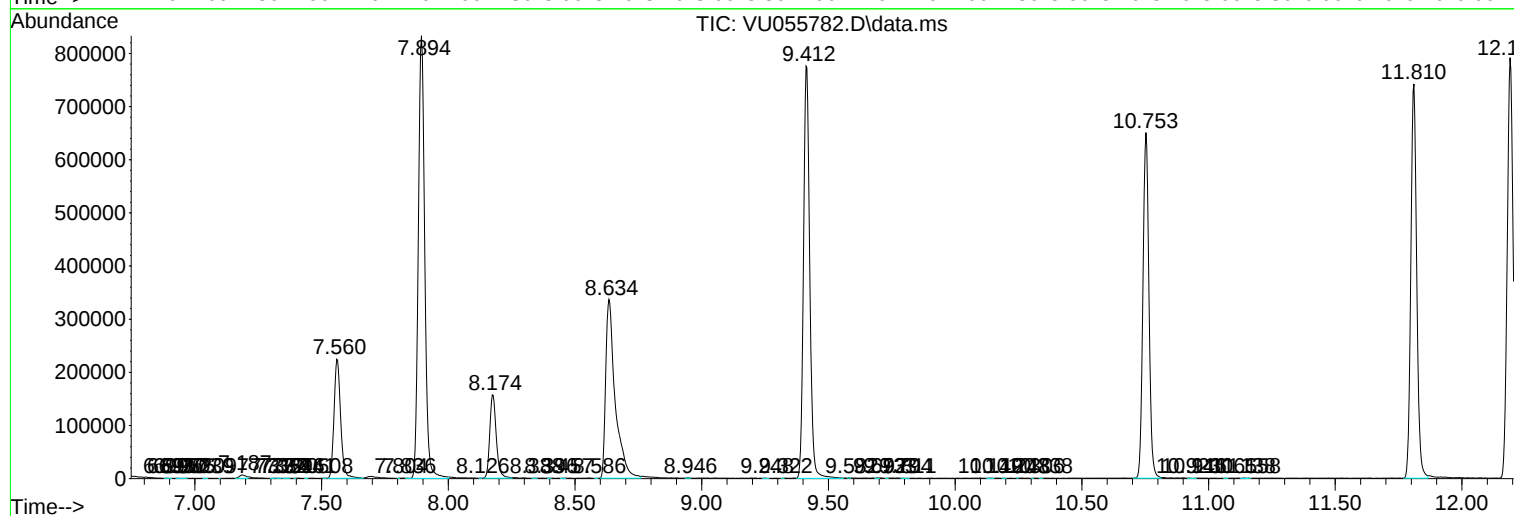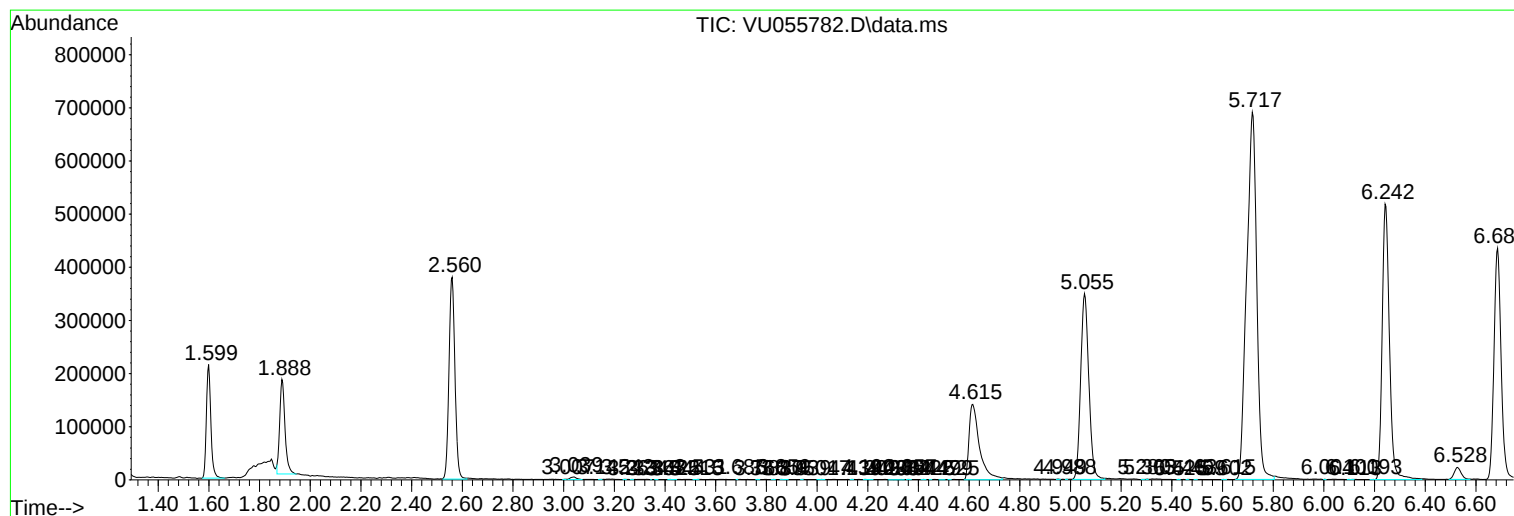

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055782.D
Acq On : 16 Oct 2023 19:14
Operator : MD/SY
Sample : 04852-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055782.D
Acq On : 16 Oct 2023 19:14
Operator : MD/SY
Sample : 04852-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------