


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101623\
Data File : VU055764.D
Acq On : 16 Oct 2023 08:32
Operator : MD/SY
Sample : BFB023
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB023

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Title : VOC Analysis
Last Update : Tue Oct 17 05:06:35 2023

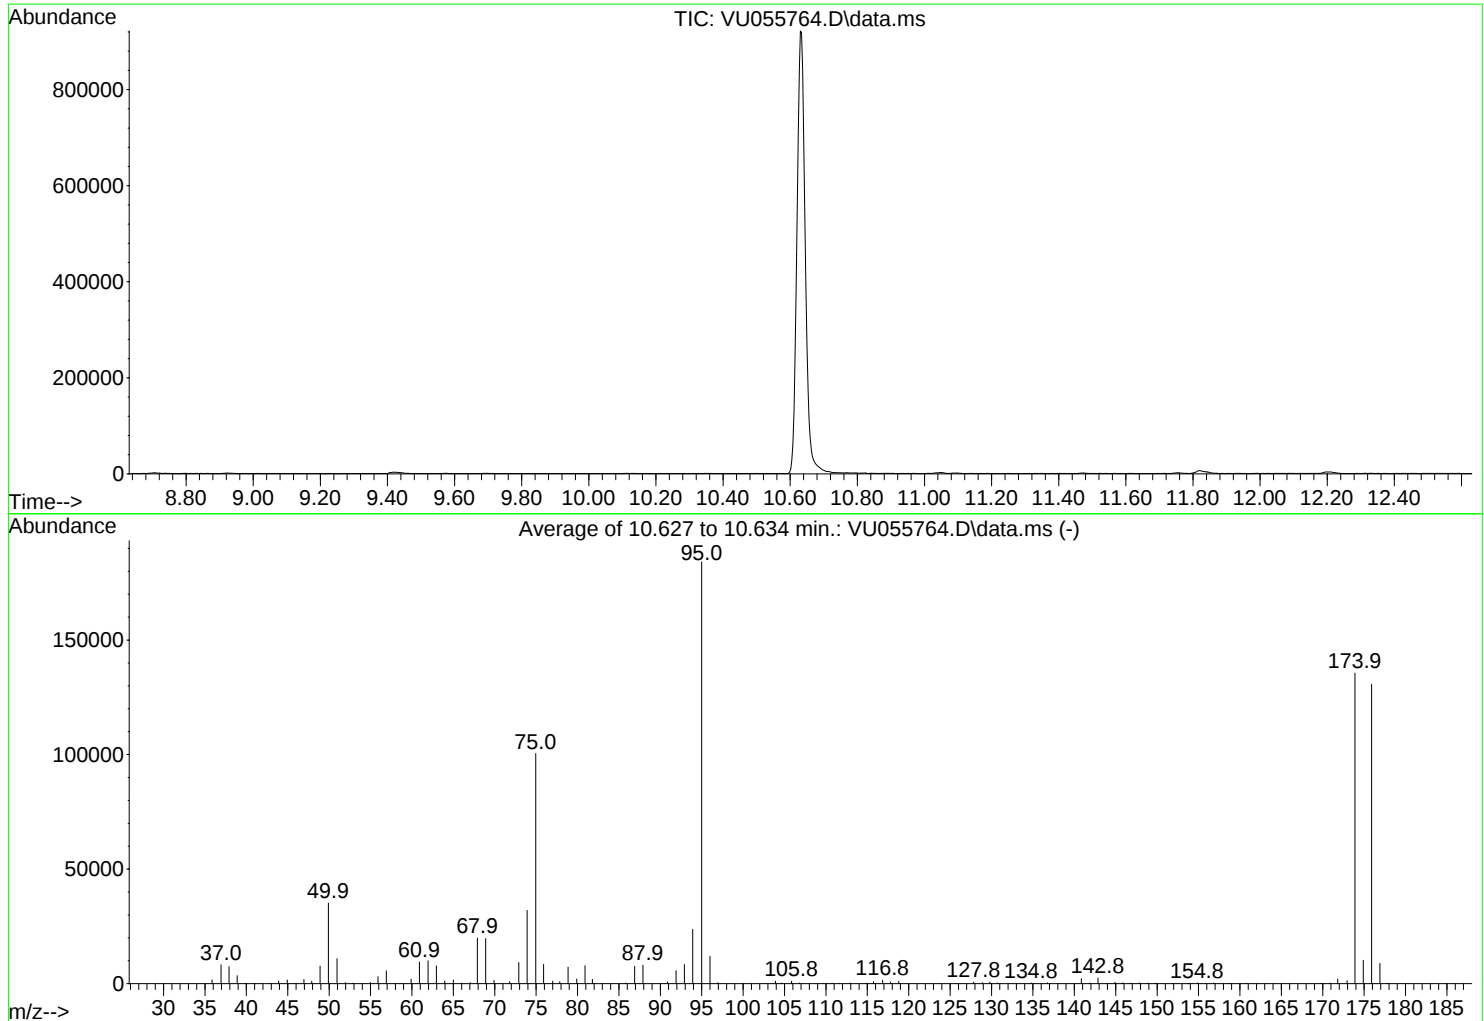

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	35232	PASS
75	95	30	80	54.5	100437	PASS
95	95	100	100	100.0	184149	PASS
96	95	5	9	6.5	11964	PASS
173	174	0.00	2	1.0	1330	PASS
174	95	50	120	73.6	135576	PASS
175	174	5	9	7.5	10189	PASS
176	174	95	101	96.4	130712	PASS
177	176	5	9	6.8	8863	PASS

m/z	Abundance
39.90	214.0
43.90	365.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
35.90	1531.0
37.00	7887.0
37.90	7212.0
38.90	3480.0
39.90	398.0
43.90	1288.0
45.00	1518.0
45.90	159.0
46.90	1596.0
47.90	1241.0
48.90	7373.0
49.90	34192.0
50.90	10570.0
52.00	567.0
52.80	290.0
55.00	446.0
55.90	2929.0
56.90	5452.0
57.90	175.0
59.90	1779.0
60.90	8935.0
62.00	9805.0
62.90	7463.0
63.90	1042.0
65.00	1554.0
66.00	209.0
67.00	536.0
67.90	19240.0
68.90	19000.0
69.90	1396.0
71.80	867.0
72.90	8661.0
73.90	30296.0
74.90	95832.0
75.90	8181.0
77.00	1209.0
77.80	731.0
78.80	7013.0
79.90	1860.0
80.90	7232.0
81.80	1738.0
83.00	187.0
85.80	230.0
86.90	7207.0
87.90	7360.0
90.80	638.0
91.90	5702.0
92.90	7654.0
93.90	22552.0
95.00	174848.0
96.00	11617.0
96.90	380.0
102.80	107.0
103.90	887.0
104.60	191.0
105.00	184.0
105.80	969.0
106.80	200.0
109.70	151.0
110.70	143.0
111.70	110.0
112.90	235.0
114.80	170.0
115.70	696.0
116.80	1446.0
117.80	698.0
118.80	1038.0
127.90	582.0
128.90	438.0
129.80	660.0
130.70	279.0
134.80	331.0
136.70	311.0
140.90	1947.0
141.80	313.0
142.90	2271.0
144.00	137.0
144.90	651.0
145.90	348.0
146.80	182.0
147.80	272.0
148.90	221.0
149.80	192.0
151.80	177.0
152.60	122.0
154.90	357.0
156.90	265.0
158.60	216.0
160.80	207.0
169.80	119.0
170.90	242.0
171.80	1866.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

172.90	1289.0
173.90	125960.0
174.90	9274.0
175.90	122568.0
176.90	8019.0
177.80	213.0

Instrument :

MSVOA_U

ClientSampleId :

BFB023

m/z	Abundance
35.80	1612.0
36.90	8389.0
37.90	7548.0
38.90	3679.0
39.90	386.0
40.90	100.0
42.80	119.0
43.90	1462.0
44.90	1689.0
45.80	161.0
47.00	1799.0
47.90	1091.0
48.90	7868.0
49.90	36168.0
51.00	11157.0
51.90	529.0
52.80	224.0
54.00	103.0
55.00	535.0
55.90	3224.0
56.90	5778.0
57.90	170.0
58.60	122.0
59.90	2033.0
60.90	9719.0
62.00	10248.0
62.90	7884.0
63.90	1098.0
65.00	1641.0
66.00	173.0
67.10	562.0
67.90	20536.0
68.90	20256.0
69.90	1490.0
71.80	930.0
72.90	9557.0
73.90	32680.0
75.00	103400.0
75.90	8612.0
77.00	1208.0
77.80	874.0
78.90	7284.0
79.90	2083.0
80.90	8121.0
81.80	1888.0
82.90	164.0
85.80	292.0
86.90	7956.0
87.90	8353.0
90.90	732.0
91.90	5870.0
92.90	8409.0
93.90	24616.0
95.00	189440.0
96.00	12160.0
97.00	456.0
102.70	111.0
103.90	1063.0
104.70	269.0
105.80	1063.0
106.80	273.0
109.70	193.0
110.70	214.0
111.60	112.0
112.90	327.0
114.80	189.0
115.80	808.0
116.80	1515.0
117.80	713.0
118.80	1121.0
123.70	149.0
125.70	103.0
127.90	701.0
128.90	481.0
129.80	679.0
130.70	282.0
134.80	293.0
136.70	337.0
140.80	2228.0
141.90	314.0
142.90	2544.0
144.00	153.0
144.90	655.0
145.90	384.0
146.80	195.0
147.90	347.0
148.80	204.0
149.80	242.0
154.90	375.0
156.80	316.0
158.90	192.0
160.70	190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

169.70	165.0
170.90	283.0
171.80	2111.0
173.00	1354.0
173.90	139392.0
174.90	10478.0
175.90	134656.0
176.90	9210.0
178.00	252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

m/z	Abundance
35.90	1654.0
36.90	8416.0
37.90	7470.0
38.90	3433.0
40.00	352.0
40.80	101.0
42.80	181.0
43.90	1623.0
45.00	1636.0
45.70	136.0
47.00	1970.0
47.90	930.0
48.90	7823.0
49.90	35336.0
51.00	11030.0
51.90	444.0
52.90	194.0
54.00	105.0
55.00	523.0
55.90	3031.0
56.90	5663.0
58.00	174.0
58.60	100.0
59.90	1997.0
60.90	9670.0
61.90	10033.0
63.00	8006.0
64.00	1156.0
65.00	1640.0
66.00	175.0
67.10	460.0
67.90	20072.0
68.90	19920.0
69.90	1494.0
71.80	948.0
72.90	9433.0
73.90	32936.0
75.00	102080.0
75.90	8393.0
77.00	1052.0
77.90	862.0
78.90	7230.0
79.90	2192.0
80.90	8235.0
81.80	1960.0
82.90	170.0
85.80	354.0
86.90	7434.0
87.90	8322.0
90.90	807.0
91.90	5485.0
92.90	8841.0
93.90	24192.0
95.00	188160.0
96.00	12114.0
97.00	477.0
102.60	112.0
103.90	1098.0
104.70	305.0
105.90	1057.0
106.80	301.0
109.70	175.0
110.80	259.0
111.60	129.0
112.90	332.0
114.90	197.0
115.80	961.0
116.90	1447.0
117.80	711.0
118.80	1096.0
123.70	191.0
125.70	127.0
127.80	685.0
128.90	395.0
129.80	624.0
130.70	285.0
134.80	313.0
136.80	329.0
140.80	2235.0
141.80	221.0
142.80	2587.0
143.90	149.0
144.90	695.0
145.80	421.0
146.70	205.0
147.90	469.0
148.80	164.0
149.80	245.0
153.70	116.0
154.80	436.0
156.80	357.0
158.90	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023

160.70	154.0
169.80	139.0
170.80	306.0
171.80	2059.0
173.00	1346.0
173.90	141376.0
174.90	10814.0
175.90	134912.0
176.90	9359.0
178.00	273.0

Instrument :
MSVOA_U
ClientSampleId :
BFB023