


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101624\
Data File : VU061131.D
Acq On : 16 Oct 2024 08:21
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101624DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Oct 17 13:52:51 2024

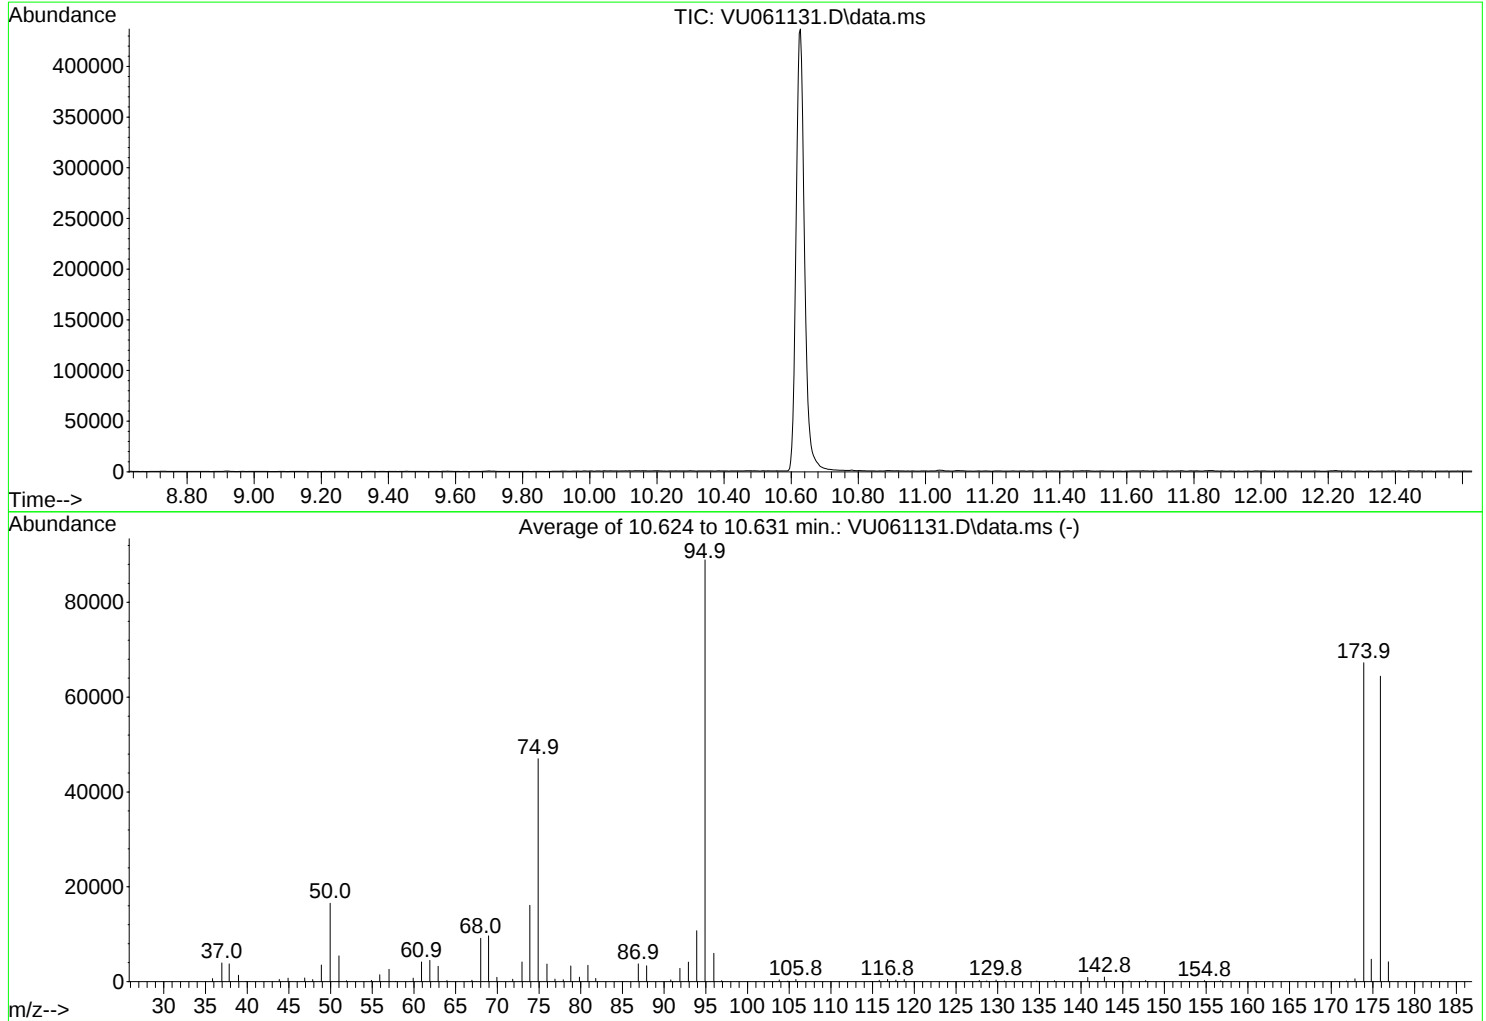

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	16522	PASS
75	95	30	60	52.9	47021	PASS
95	95	100	100	100.0	88960	PASS
96	95	5	9	6.7	5978	PASS
173	174	0.00	2	0.9	619	PASS
174	95	50	100	75.6	67243	PASS
175	174	5	9	7.0	4726	PASS
176	174	95	101	95.8	64429	PASS
177	176	5	9	6.5	4172	PASS