

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101718\
 Data File : VU027676.D
 Acq On : 17 Oct 2018 14:20
 Operator : MD/SY
 Sample : J5463-01 250X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JB2

Quant Time: Oct 19 07:11:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 19 06:41:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	83736	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	78289	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	38998	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	30176	4.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.80%
7) Chloroethane-d5	1.68	69	23456	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.28	63	41338	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	4.21	46	88216	46.62	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.24%
24) Chloroform-d	4.65	84	50186	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.31	65	28108	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.34	84	107632	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.33	67	38288	5.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.80%
41) Toluene-d8	7.57	98	104854	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
43) trans-1,3-Dichloropropene-	7.85	79	15120	4.61	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.20%
46) 2-Hexanone-d5	8.32	63	80995	50.35	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.70%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	26998	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	37868	5.18	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.60%

Target Compounds


					Ovalue
5) Vinyl chloride	1.40	62	44417	5.436 ug/L #	81
18) trans-1,2-Dichloroethene	2.99	96	1197	0.199 ug/L #	73
22) cis-1,2-Dichloroethene	4.23	96	126585	18.985 ug/L #	97
34) Trichloroethene	6.19	95	63210	9.531 ug/L	98
47) Tetrachloroethene	8.23	164	1768	0.334 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101718\
Data File : VU027676.D
Acq On : 17 Oct 2018 14:20
Operator : MD/SY
Sample : J5463-01 250X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JB2

Quant Time: Oct 19 07:11:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 19 06:41:15 2018
Response via : Initial Calibration

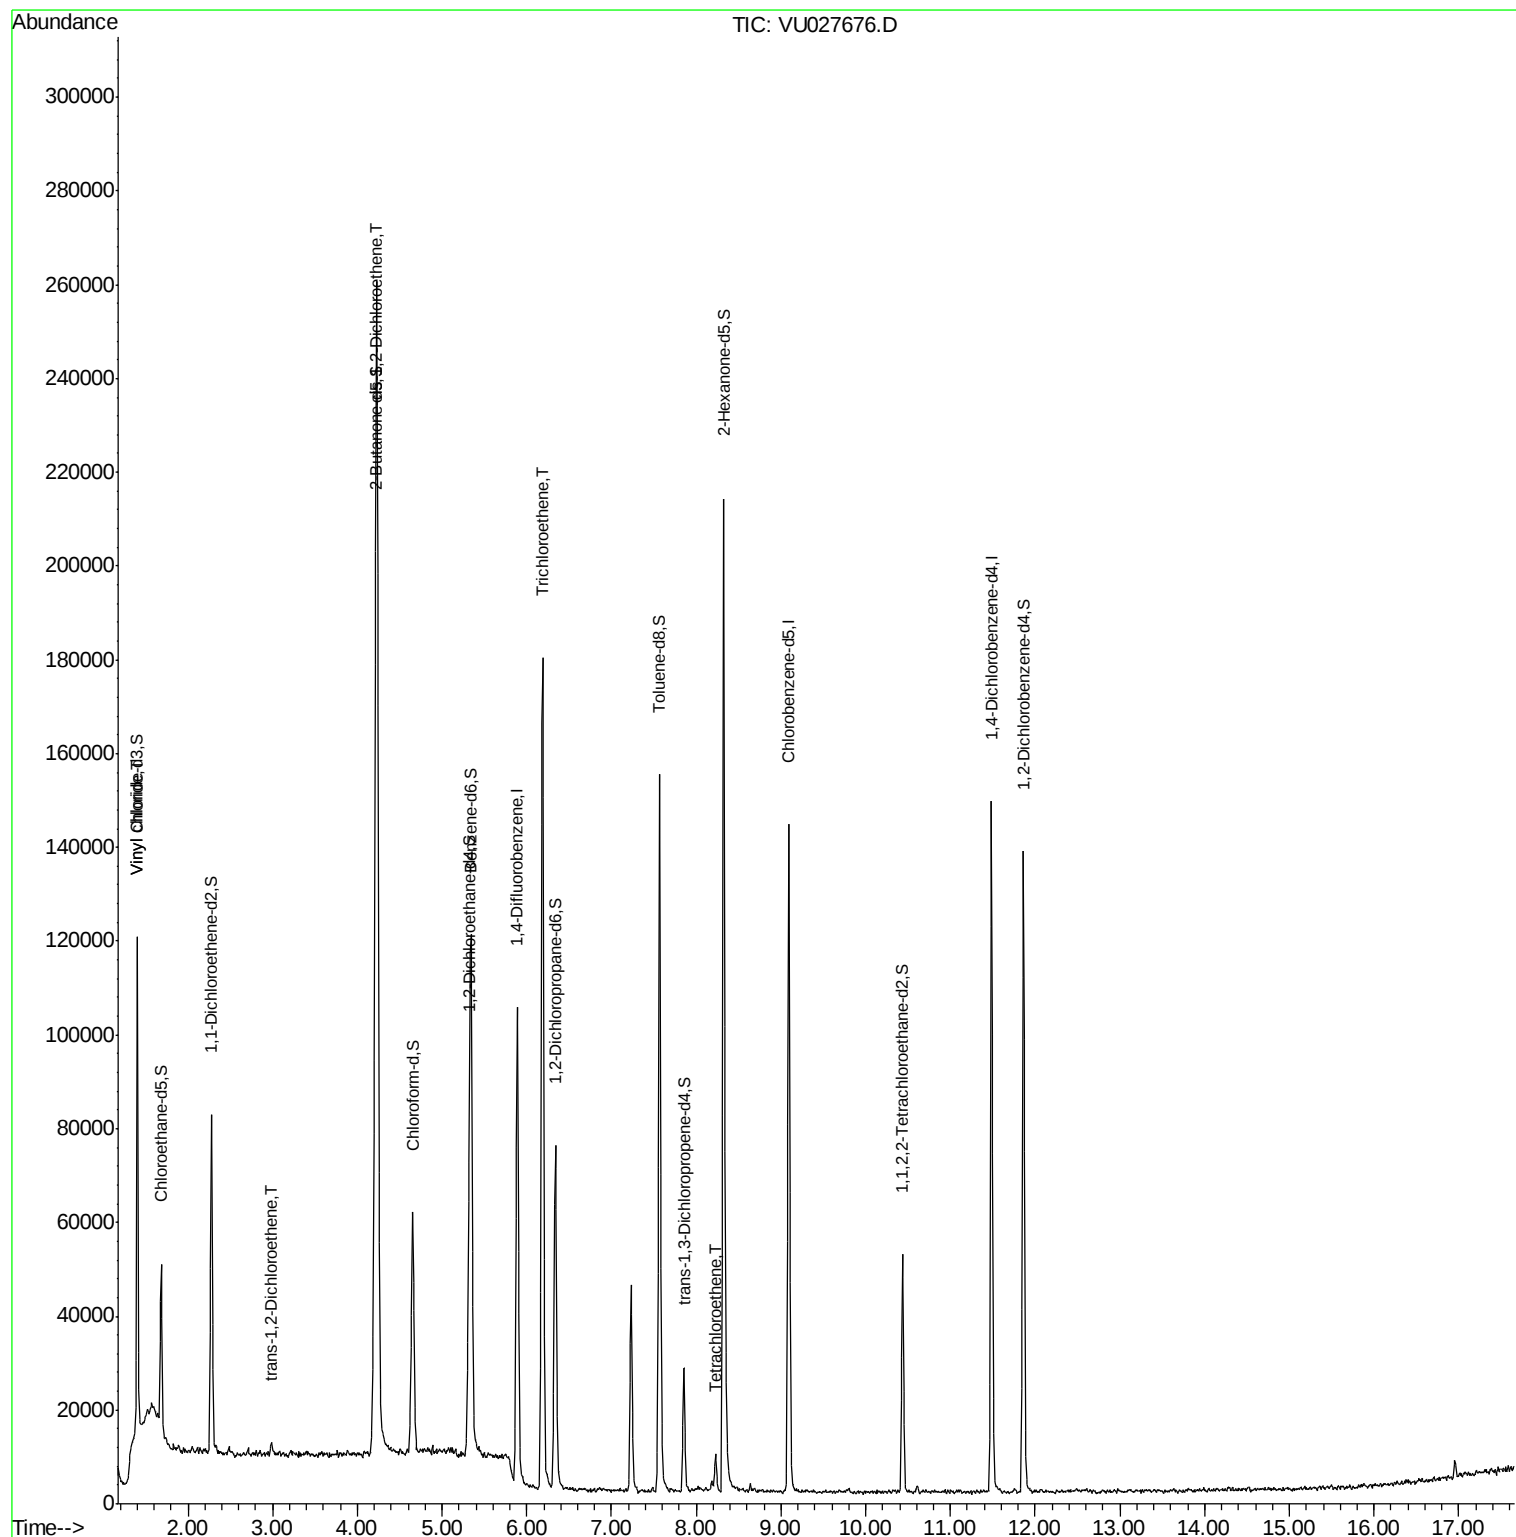

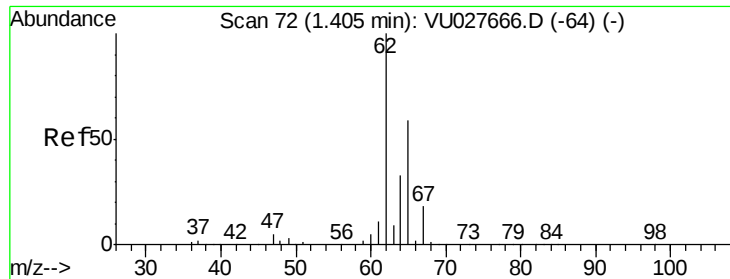

#5

Vinyl chloride

Concen: 5.436 ug/L

RT: 1.40 min Scan# 72

Delta R.T. 0.00 min

Lab File: VU027676.D

Acq: 17 Oct 2018 14:20

Instrument :

MSVOA_U

ClientSampleId :


C0JB2

Tot Ion: 62 Resp: 44417

Ion Ratio Lower Upper




62 100

64 43.3 22.9 42.5#

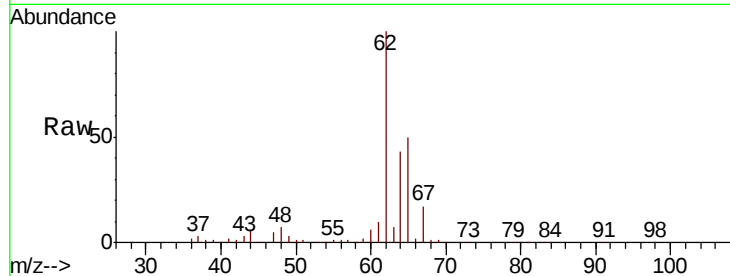

Abundance Ion 62.00 (61.70 to 62.70): VU0

Ion 64.10 (63.80 to 64.80): VU0

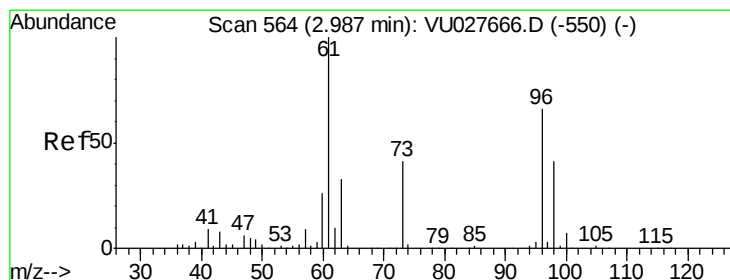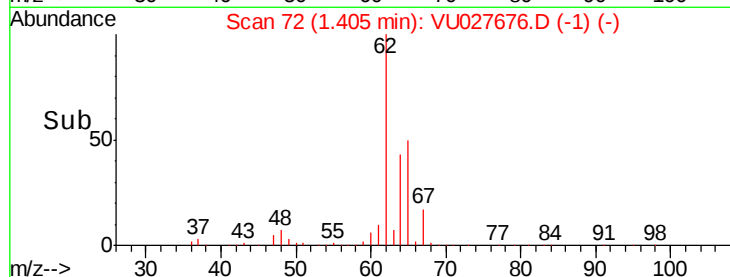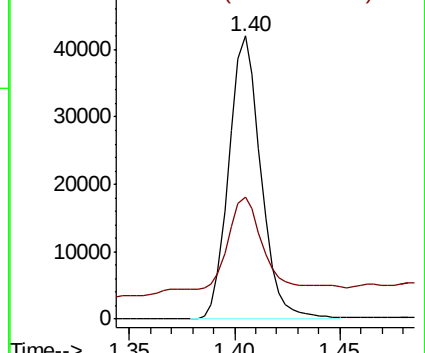

#18

trans-1,2-Dichloroethene

Concen: 0.199 ug/L

RT: 2.99 min Scan# 564

Delta R.T. 0.00 min

Lab File: VU027676.D

Acq: 17 Oct 2018 14:20


Tgt Ion: 96 Resp: 1197

Ion Ratio Lower Upper

96 100

61 137.0 105.8 196.4



98 111.8 43.6 81.0#

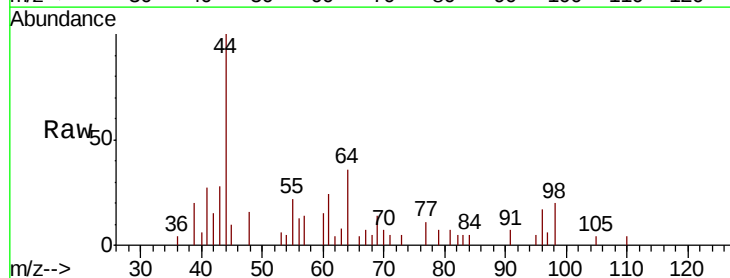


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 97.95 (97.65 to 98.65): VU0

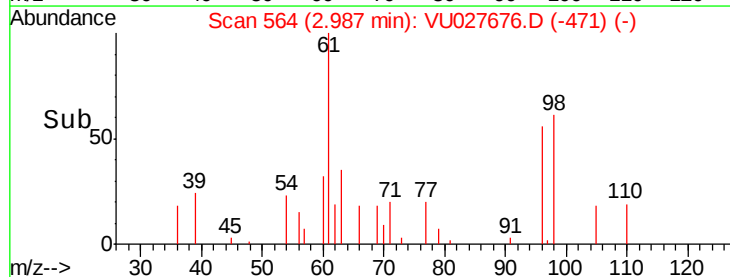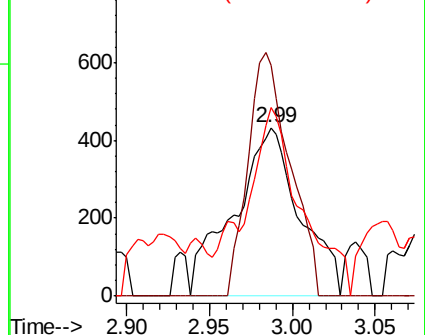

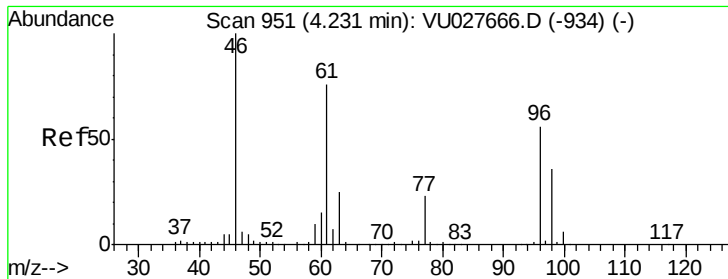


#22




cis-1,2-Dichloroethene
Concen: 18.985 ug/L
RT: 4.23 min Scan# 950
Delta R.T. -0.00 min
Lab File: VU027676.D
Acq: 17 Oct 2018 14:20

Instrument :
MSVOA_U
ClientSampleId :
C0JB2

Tot Ion: 96 Resp: 126585
Ion Ratio Lower Upper
96 100
61 139.5 95.3 176.9
68 0.3 1.1 2.1#

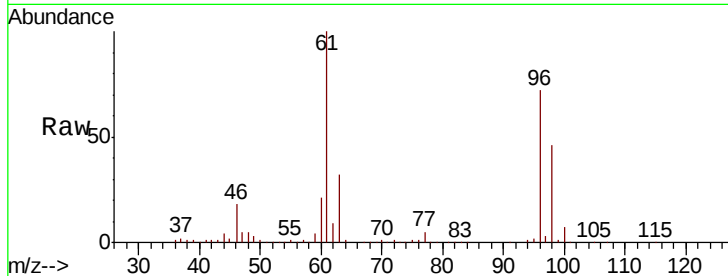


Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.05 (60.75 to 61.75): VU0
Ion 68.15 (67.85 to 68.85): VU0

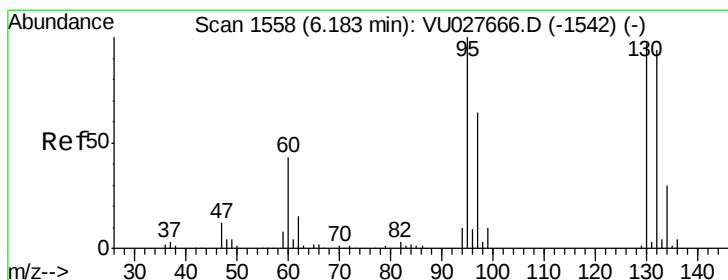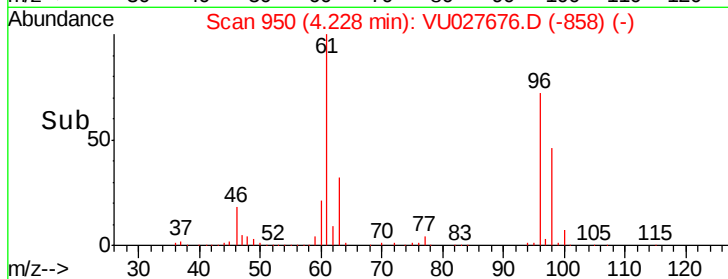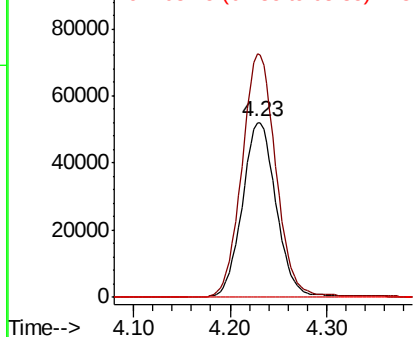



#34


Trichloroethene
Concen: 9.531 ug/L
RT: 6.19 min Scan# 1559
Delta R.T. 0.00 min
Lab File: VU027676.D
Acq: 17 Oct 2018 14:20

Tgt Ion: 95 Resp: 63210
Ion Ratio Lower Upper
95 100
97 65.7 44.7 83.1
132 96.8 65.9 122.5
130 99.2 67.9 126.1

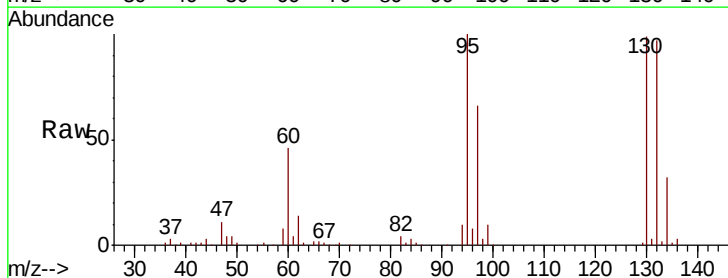

Abundance Ion 95.00 (94.70 to 95.70): VU0
Ion 96.95 (96.65 to 97.65): VU0
Ion 131.95 (131.65 to 132.65): V
Ion 129.95 (129.65 to 130.65): V

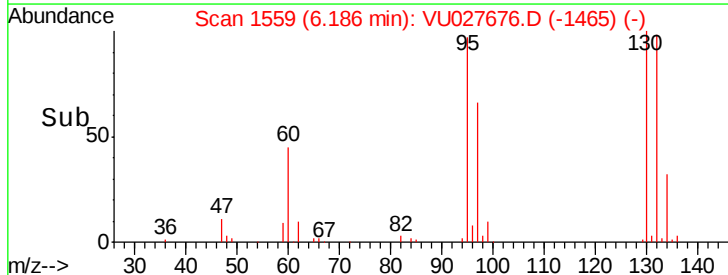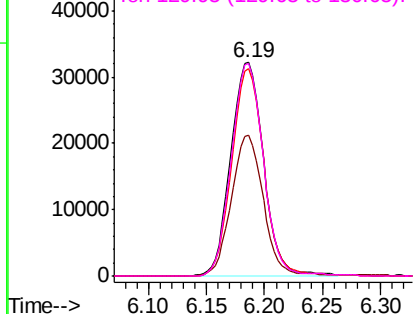

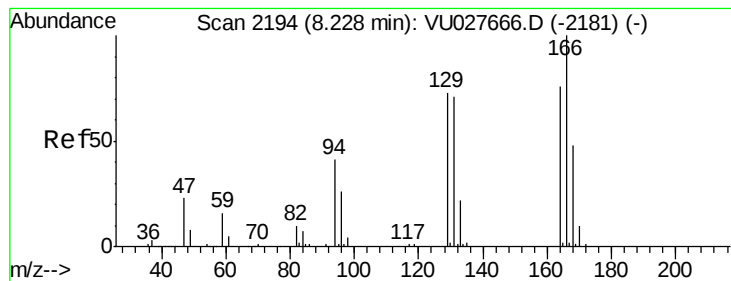

#47

Tetrachloroethene

Concen: 0.334 ug/L

RT: 8.23 min Scan# 2194

Delta R.T. 0.00 min

Lab File: VU027676.D


Acq: 17 Oct 2018 14:20

Instrument :

MSVOA_U

ClientSampleId :

C0JB2

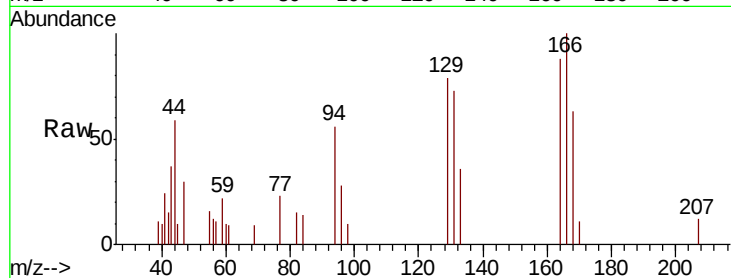

Tot Ion:164 Resp: 1768


Ion Ratio Lower Upper

164 100

129 89.5 67.3 124.9

131 83.1 64.8 120.3

166 113.3 91.8 170.4

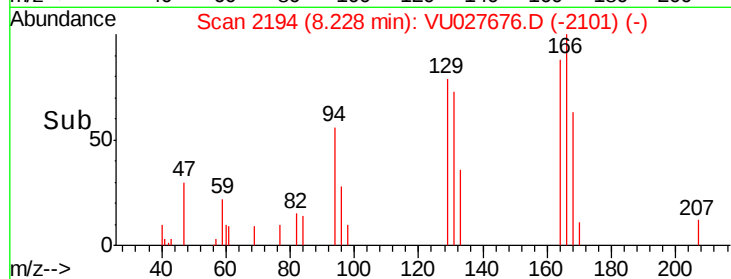

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

