

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101718\
 Data File : VU027686.D
 Acq On : 17 Oct 2018 18:56
 Operator : MD/SY
 Sample : J5463-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JC0

Quant Time: Oct 19 07:47:18 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 17 10:16:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	78956	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	73048	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	36503	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	26474	4.22	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.40%
7) Chloroethane-d5	1.68	69	21209	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.80%
11) 1,1-Dichloroethene-d2	2.28	63	36648	3.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.80%
20) 2-Butanone-d5	4.20	46	86762	48.63	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.26%
24) Chloroform-d	4.65	84	46117	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.31	65	25419	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
32) Benzene-d6	5.34	84	98300	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.33	67	34829	5.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.40%
41) Toluene-d8	7.57	98	91436	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
43) trans-1,3-Dichloropropene-	7.85	79	13598	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
46) 2-Hexanone-d5	8.31	63	73579	49.03	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.06%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	25040	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	33877	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds					Ovalue
13) Acetone	2.33	43	4474	3.921 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101718\
Data File : VU027686.D
Acq On : 17 Oct 2018 18:56
Operator : MD/SY
Sample : J5463-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JC0

Quant Time: Oct 19 07:47:18 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 17 10:16:06 2018
Response via : Initial Calibration

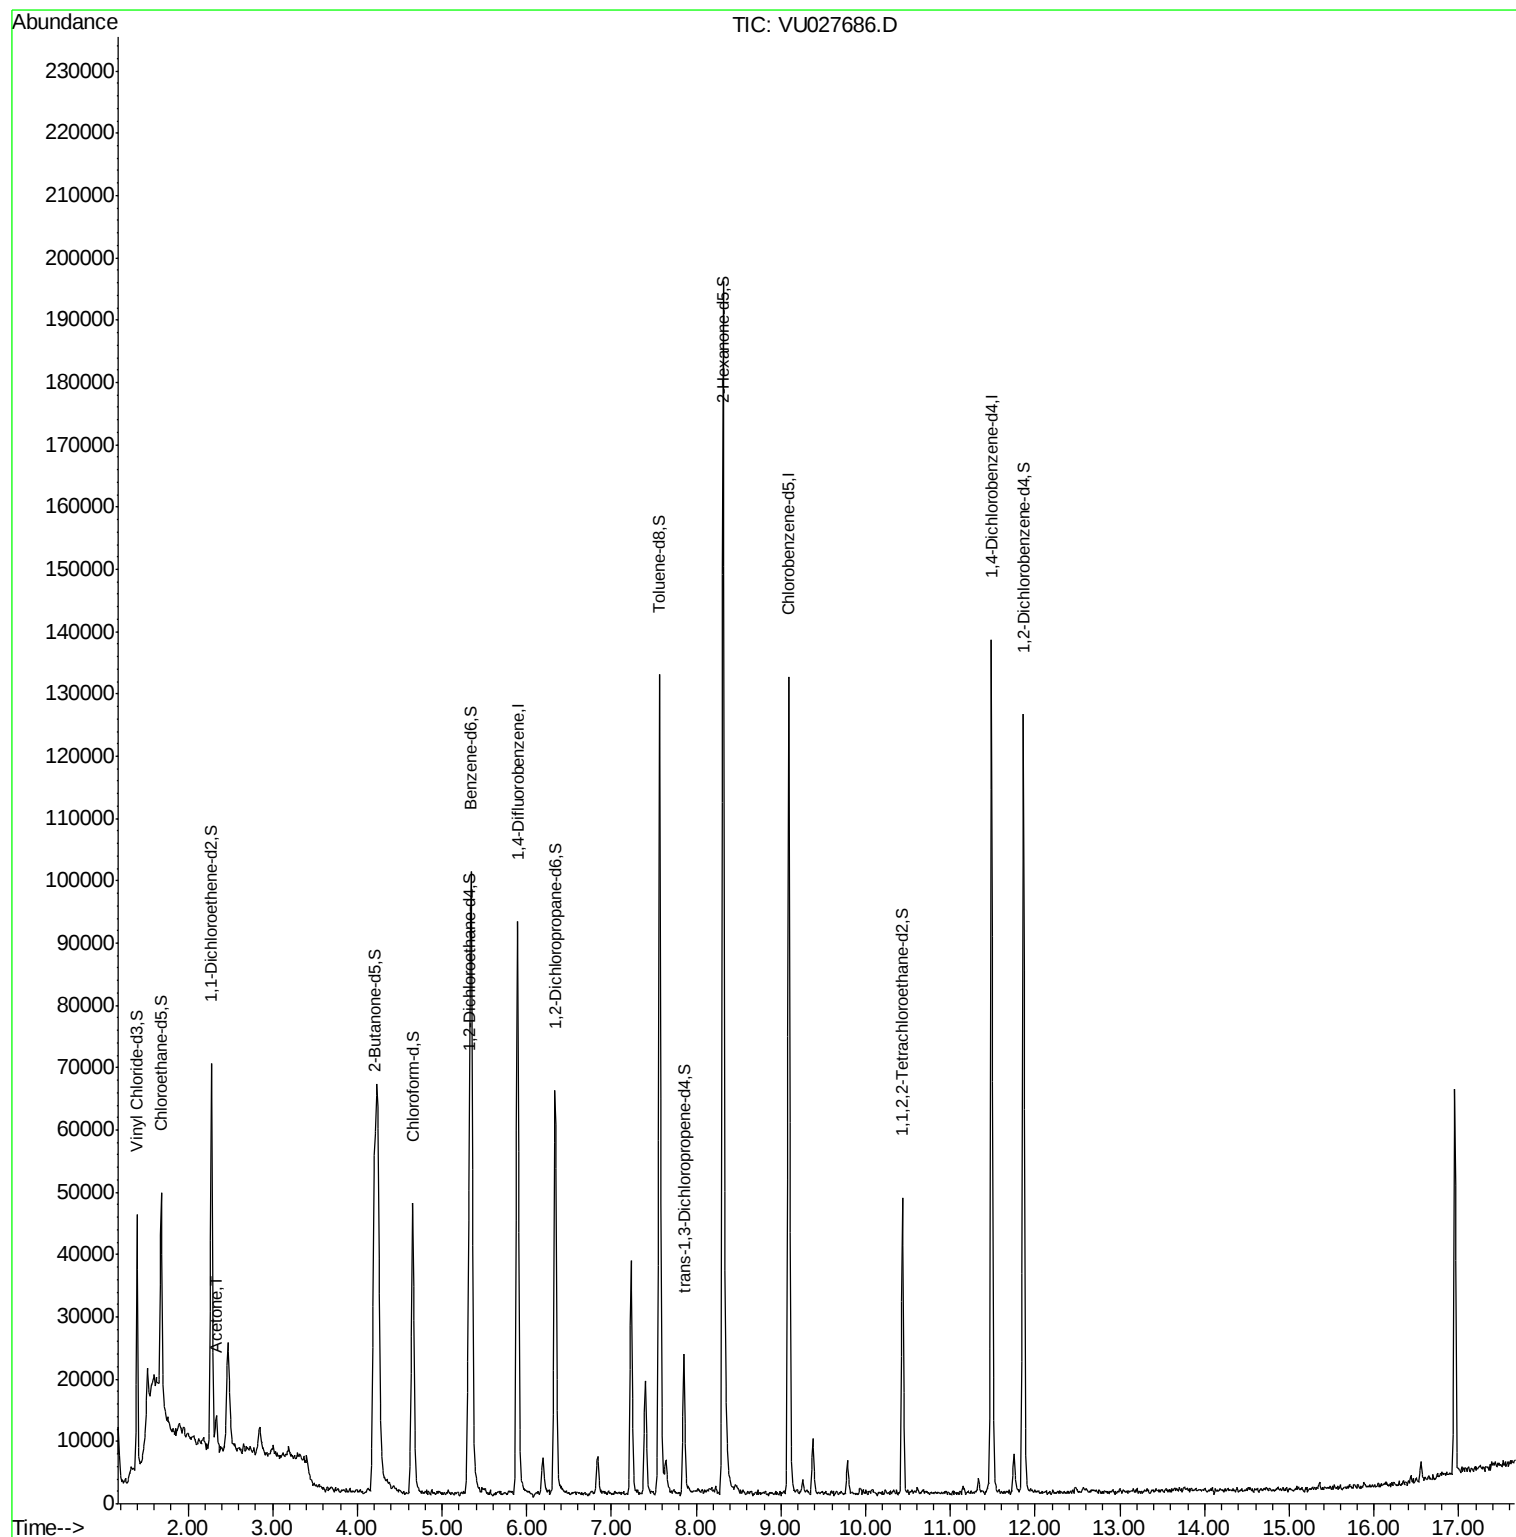

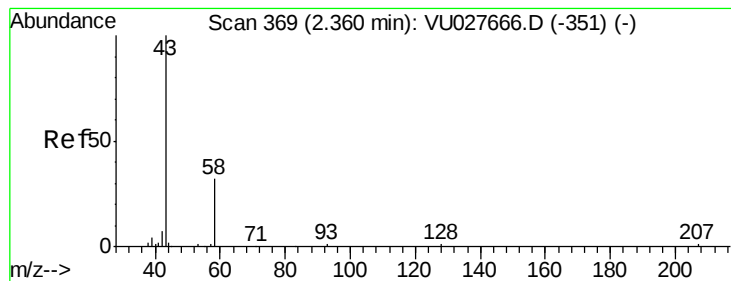

#13
 Acetone
 Concen: 3.921 ug/L
 RT: 2.33 min Scan# 361
 Delta R.T. -0.03 min
 Lab File: VU027686.D
 Acq: 17 Oct 2018 18:56

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JC0

Tot Ion: 43 Resp: 4474
 Ion Ratio Lower Upper
 43 100
 58 34.6 0.0 63.0

