


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101718\
 Data File : VU027663.D
 Acq On : 17 Oct 2018 07:34
 Operator : MD/SY
 Sample : BFB44
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB44

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Oct 19 08:11:17 2018

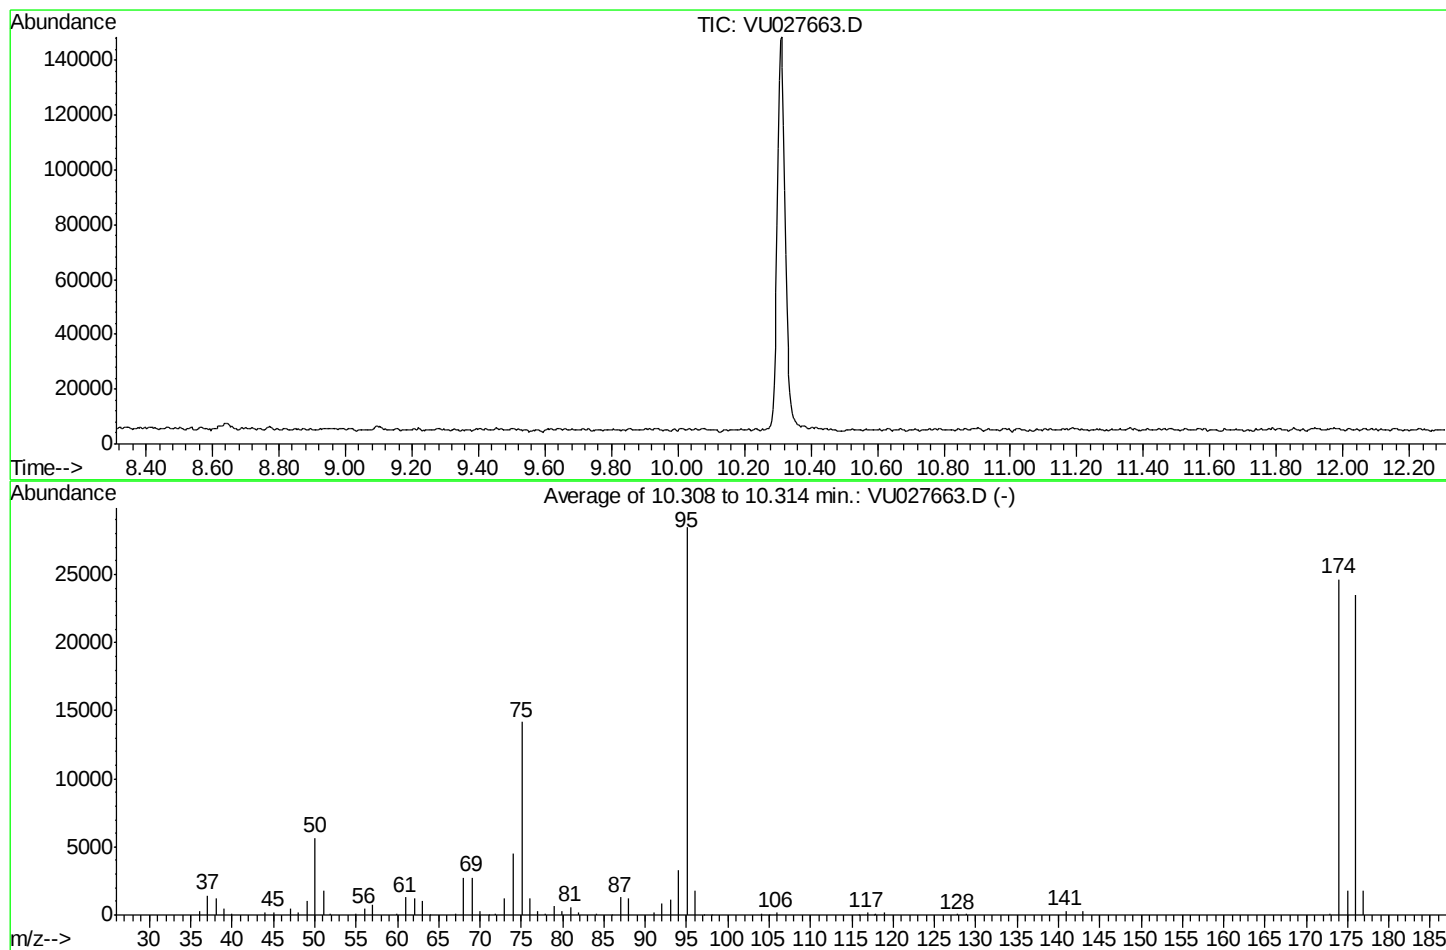

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	5643	PASS
75	95	30	80	49.7	14150	PASS
95	95	100	100	100.0	28464	PASS
96	95	5	9	6.4	1818	PASS
173	174	0.00	2	0.3	64	PASS
174	95	50	120	86.6	24661	PASS
175	174	5	9	7.2	1783	PASS
176	174	95	101	95.3	23509	PASS
177	176	5	9	7.5	1760	PASS

m/z	Abundance
39.00	228.0
41.00	450.0
42.10	247.0
43.00	633.0
44.00	838.0
45.00	218.0
53.00	122.0
54.00	112.0
55.10	412.0
56.00	212.0
57.10	195.0
59.90	253.0
67.00	119.0
68.00	102.0
69.10	198.0
70.00	155.0
71.10	101.0
73.00	149.0
81.00	137.0
83.10	115.0
84.90	170.0
97.10	121.0
98.10	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	246.0
37.00	1315.0
38.10	1144.0
39.00	705.0
40.00	123.0
41.00	426.0
42.00	246.0
43.00	604.0
44.00	970.0
45.00	423.0
47.00	394.0
47.90	139.0
49.00	1016.0
50.10	5292.0
51.10	1612.0
51.90	105.0
53.00	104.0
53.90	110.0
55.00	566.0
56.00	586.0
57.00	936.0
60.00	405.0
61.00	1220.0
62.00	1113.0
63.00	996.0
67.00	195.0
68.00	2617.0
69.10	2673.0
70.00	352.0
71.10	127.0
71.90	160.0
73.00	1281.0
74.00	4264.0
75.00	13349.0
76.00	1082.0
77.00	291.0
77.90	102.0
78.90	654.0
79.90	218.0
81.00	685.0
81.90	207.0
83.10	126.0
84.10	118.0
85.10	132.0
87.00	1214.0
88.00	1094.0
91.10	178.0
92.00	733.0
93.00	1104.0
94.00	3098.0
95.00	27176.0
96.00	1690.0
97.00	165.0
98.00	151.0
104.00	124.0
105.00	102.0
105.90	150.0
116.90	203.0
117.90	112.0
118.90	135.0
128.90	126.0
140.90	298.0
142.90	267.0
174.00	23704.0
175.00	1768.0
176.00	22472.0
176.90	1640.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	281.0
37.00	1461.0
38.10	1281.0
39.00	729.0
40.00	143.0
41.00	444.0
42.00	212.0
43.10	604.0
44.00	1030.0
45.00	438.0
47.00	478.0
47.90	160.0
49.00	1119.0
50.00	5781.0
51.00	1831.0
51.90	115.0
53.00	132.0
55.00	527.0
56.00	674.0
57.00	1007.0
60.00	398.0
61.00	1340.0
62.00	1215.0
63.00	1123.0
67.00	195.0
68.00	2892.0
69.00	3019.0
70.00	407.0
71.10	131.0
71.90	136.0
73.00	1377.0
74.00	4657.0
75.00	14655.0
76.00	1270.0
77.00	309.0
77.80	119.0
78.90	683.0
79.90	244.0
80.90	740.0
81.90	236.0
83.10	110.0
84.10	121.0
85.00	139.0
87.00	1329.0
87.90	1241.0
91.10	164.0
92.00	834.0
93.00	1222.0
94.00	3341.0
95.00	29248.0
96.00	1858.0
97.00	157.0
98.00	137.0
104.00	129.0
105.90	161.0
116.90	188.0
117.90	110.0
118.90	162.0
127.80	118.0
128.90	112.0
140.90	297.0
142.90	306.0
174.00	25480.0
175.00	1815.0
176.00	24288.0
177.00	1831.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	280.0
37.00	1470.0
38.00	1327.0
39.00	720.0
40.00	162.0
41.00	441.0
42.00	192.0
43.10	609.0
44.00	1086.0
45.00	454.0
47.00	490.0
48.00	189.0
49.00	1095.0
50.00	5856.0
51.00	1872.0
51.90	109.0
53.00	119.0
55.00	490.0
56.00	662.0
57.00	1028.0
59.90	371.0
61.00	1332.0
62.10	1265.0
63.00	1117.0
64.00	101.0
67.00	193.0
68.00	2923.0
69.00	3183.0
70.00	421.0
71.10	131.0
71.90	131.0
73.10	1331.0
74.00	4604.0
75.10	14446.0
76.00	1328.0
77.00	288.0
77.90	128.0
79.00	717.0
79.90	277.0
80.90	737.0
81.90	245.0
84.00	120.0
85.00	144.0
86.00	105.0
87.00	1302.0
87.90	1320.0
91.10	160.0
92.00	857.0
93.00	1160.0
94.00	3333.0
95.10	28968.0
96.00	1907.0
97.10	166.0
98.00	127.0
104.00	121.0
105.90	161.0
115.80	104.0
116.80	157.0
117.70	103.0
118.90	159.0
127.80	135.0
140.90	300.0
142.90	297.0
172.80	192.0
174.00	24800.0
175.00	1766.0
176.00	23768.0
177.00	1810.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44