


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101719\
Data File : VU035200.D
Acq On : 17 Oct 2019 08:44
Operator : JC/SP
Sample : BFB21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB21

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Oct 22 06:40:31 2019

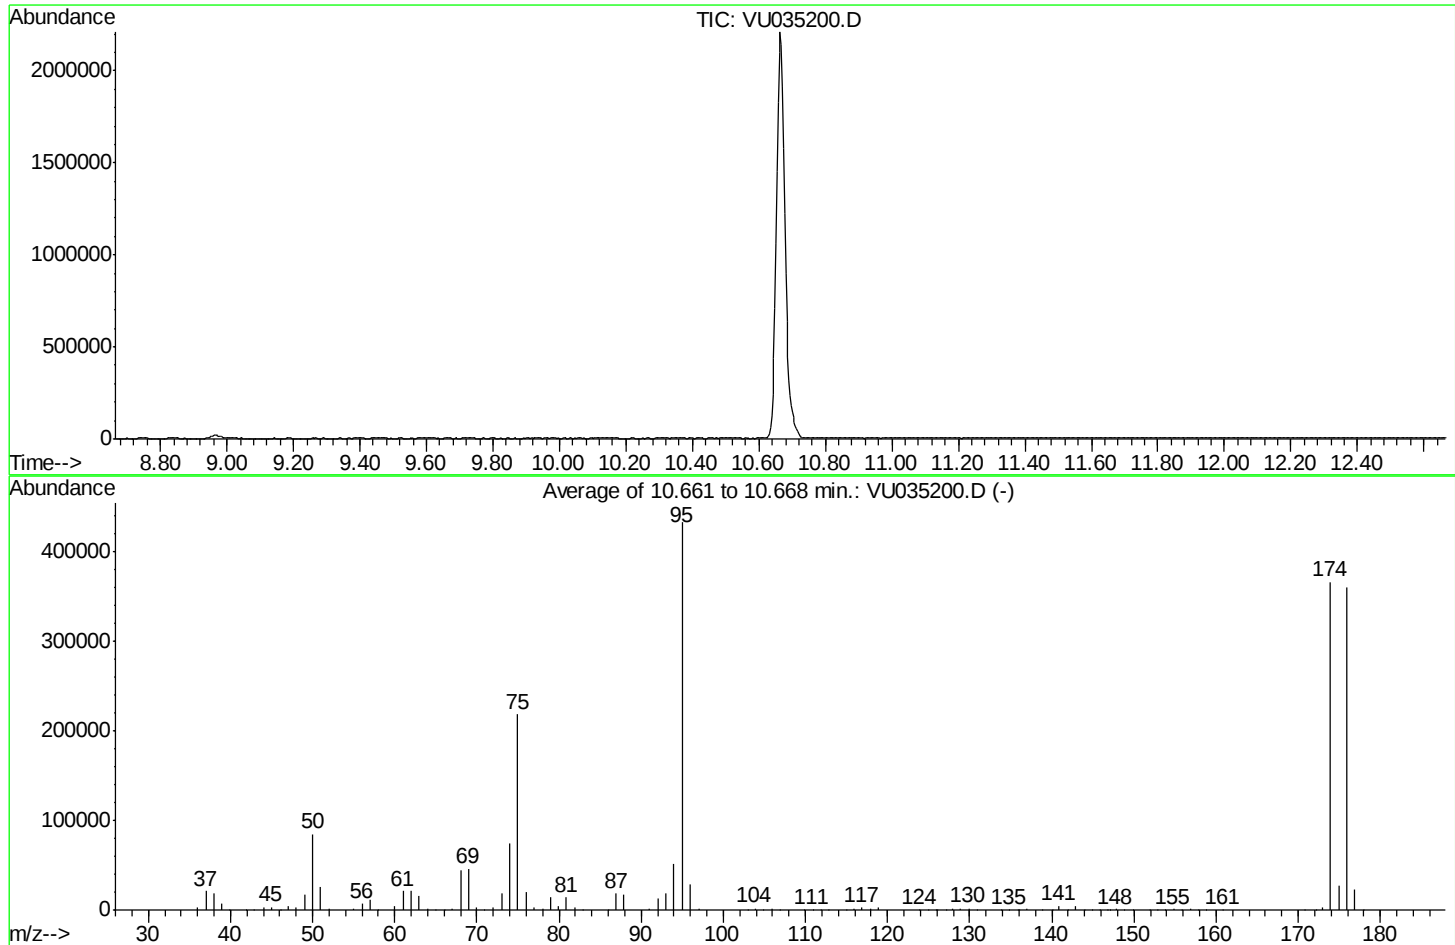

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	84245	PASS
75	95	30	80	50.5	218240	PASS
95	95	100	100	100.0	432106	PASS
96	95	5	9	6.6	28346	PASS
173	174	0.00	2	0.8	3043	PASS
174	95	50	120	84.6	365589	PASS
175	174	5	9	7.3	26728	PASS
176	174	95	101	98.5	360213	PASS
177	176	5	9	6.4	23090	PASS

m/z	Abundance
36.00	3543.0
37.00	20680.0
38.00	18264.0
39.00	7595.0
39.90	411.0
41.10	281.0
42.00	150.0
42.90	356.0
44.00	4621.0
45.00	3672.0
46.10	250.0
47.10	4770.0
48.00	2673.0
49.00	17824.0
50.00	83424.0
51.00	26296.0
52.00	1031.0
55.00	1352.0
56.00	6760.0
57.00	11398.0
58.00	605.0
60.00	3841.0
61.00	21744.0
62.00	20952.0
63.00	15181.0
64.00	1445.0
64.90	308.0
66.00	112.0
66.90	1084.0
68.00	43912.0
69.00	45816.0
70.00	3368.0
70.90	155.0
72.00	2533.0
73.00	19440.0
74.00	72472.0
75.00	215616.0
76.00	19136.0
77.00	2208.0
78.00	1818.0
78.90	13762.0
79.90	3814.0
80.90	13671.0
81.90	3179.0
82.90	306.0
86.10	511.0
87.00	18168.0
87.90	17184.0
91.00	1582.0
92.00	11820.0
93.00	17752.0
94.00	50384.0
95.00	423616.0
96.00	27864.0
97.00	825.0
103.00	152.0
103.90	1899.0
104.90	774.0
105.90	1790.0
106.90	474.0
109.90	277.0
110.80	329.0
111.80	278.0
112.90	349.0
115.00	498.0
115.90	1484.0
116.90	2856.0
117.90	1671.0
118.90	2281.0
123.90	332.0
124.90	138.0
125.80	217.0
127.90	1387.0
128.80	781.0
129.90	1566.0
130.80	539.0
133.80	116.0
134.80	643.0
135.80	121.0
136.90	843.0
138.90	181.0
140.00	319.0
140.90	4166.0
141.80	498.0
142.90	4320.0
144.00	281.0
144.90	453.0
145.70	483.0
146.80	266.0
147.00	258.0
147.80	1032.0
148.80	357.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

149.90	356.0
151.90	213.0
152.90	229.0
153.80	268.0
154.90	1048.0
155.80	140.0
156.90	855.0
157.80	120.0
158.80	533.0
160.90	353.0
170.80	209.0
173.00	2983.0
173.90	350272.0
174.90	26048.0
175.90	344704.0
176.90	22408.0
177.90	637.0
206.90	255.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	3721.0
37.00	21616.0
38.00	19096.0
39.00	7818.0
39.90	438.0
41.00	256.0
41.90	108.0
42.90	382.0
44.00	4842.0
45.00	3772.0
46.10	277.0
47.00	5111.0
48.00	2824.0
49.00	18344.0
50.00	86840.0
51.00	27192.0
52.00	1070.0
55.00	1194.0
56.00	7014.0
57.00	12046.0
58.00	702.0
60.00	4009.0
61.00	22000.0
62.00	21392.0
63.00	15729.0
64.00	1535.0
64.90	265.0
66.90	1050.0
68.00	45592.0
69.00	47728.0
70.00	3566.0
71.00	154.0
72.00	2719.0
73.00	19912.0
74.00	75888.0
75.00	223872.0
76.00	20016.0
77.00	2425.0
78.00	1985.0
78.90	14418.0
79.90	4007.0
80.90	14172.0
81.90	3380.0
82.90	322.0
86.00	603.0
87.00	18632.0
87.90	18176.0
91.00	1609.0
92.00	12601.0
93.00	18816.0
94.00	52944.0
95.00	444608.0
96.00	29168.0
97.00	807.0
102.90	165.0
103.90	1914.0
104.90	721.0
105.90	1964.0
106.90	451.0
109.90	272.0
110.90	387.0
111.90	328.0
112.90	367.0
115.00	522.0
115.90	1672.0
116.90	2877.0
117.90	1708.0
118.90	2374.0
123.90	357.0
124.90	106.0
126.00	215.0
127.90	1465.0
128.80	810.0
129.90	1600.0
130.80	589.0
133.80	136.0
134.80	738.0
136.00	128.0
137.00	871.0
138.80	179.0
140.00	421.0
140.90	4667.0
141.80	558.0
142.90	4629.0
143.90	281.0
144.90	445.0
145.70	477.0
146.70	223.0
147.10	249.0
147.80	1162.0
148.80	332.0
149.80	371.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

151.90	240.0
152.90	252.0
153.80	281.0
154.90	1027.0
155.80	156.0
156.90	900.0
157.80	109.0
158.80	480.0
160.90	422.0
170.80	228.0
172.10	715.0
173.00	3162.0
173.90	375424.0
174.90	27264.0
175.90	369856.0
176.90	23712.0
177.90	681.0
206.90	282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	3575.0
37.00	21072.0
38.00	18336.0
39.00	7348.0
39.90	519.0
40.90	256.0
42.90	366.0
44.00	4768.0
45.00	3539.0
46.10	296.0
47.00	5004.0
48.00	2587.0
49.00	17416.0
50.00	82472.0
51.00	25832.0
52.00	999.0
55.00	1072.0
56.00	6823.0
57.00	11626.0
58.00	688.0
60.00	4023.0
61.00	20440.0
62.00	20016.0
63.00	15030.0
64.00	1431.0
64.90	217.0
67.00	995.0
68.00	43616.0
69.00	45576.0
70.00	3334.0
71.00	148.0
72.00	2564.0
73.00	18824.0
74.00	73120.0
75.00	215232.0
76.00	19168.0
77.00	2409.0
78.00	1838.0
78.90	13792.0
79.90	3768.0
80.90	13543.0
81.90	3149.0
82.90	314.0
86.00	540.0
86.90	17632.0
87.90	17832.0
91.00	1573.0
92.00	12444.0
93.00	17856.0
94.00	50776.0
95.00	428096.0
96.00	28008.0
97.00	795.0
102.80	202.0
103.90	1872.0
104.80	620.0
105.90	1853.0
106.90	409.0
109.90	275.0
110.90	387.0
111.90	354.0
112.80	361.0
114.90	507.0
115.90	1661.0
116.90	2771.0
117.90	1502.0
118.90	2230.0
123.90	324.0
126.00	250.0
127.10	100.0
127.90	1419.0
128.90	765.0
129.90	1539.0
130.80	567.0
133.80	132.0
134.80	689.0
136.10	128.0
136.90	766.0
138.80	173.0
140.00	411.0
140.90	4723.0
141.90	564.0
142.90	4417.0
143.90	289.0
144.90	371.0
145.80	469.0
146.80	197.0
147.80	1067.0
148.80	299.0
149.80	366.0
151.90	239.0
152.80	253.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

153.80	283.0
154.80	961.0
155.80	157.0
156.90	851.0
158.70	456.0
160.80	485.0
170.80	184.0
172.10	682.0
173.00	2985.0
173.90	371072.0
174.90	26872.0
175.90	366080.0
176.90	23152.0
177.90	660.0
206.90	307.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

Scan 2881 (10.603 min): VU035200.D
BFB21

m/z	Abundance
38.90	202.0
39.90	253.0
40.90	289.0
41.70	134.0
43.00	257.0
44.00	2186.0
44.80	117.0
54.90	175.0
69.00	208.0
73.10	140.0
77.00	102.0
207.00	339.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21