
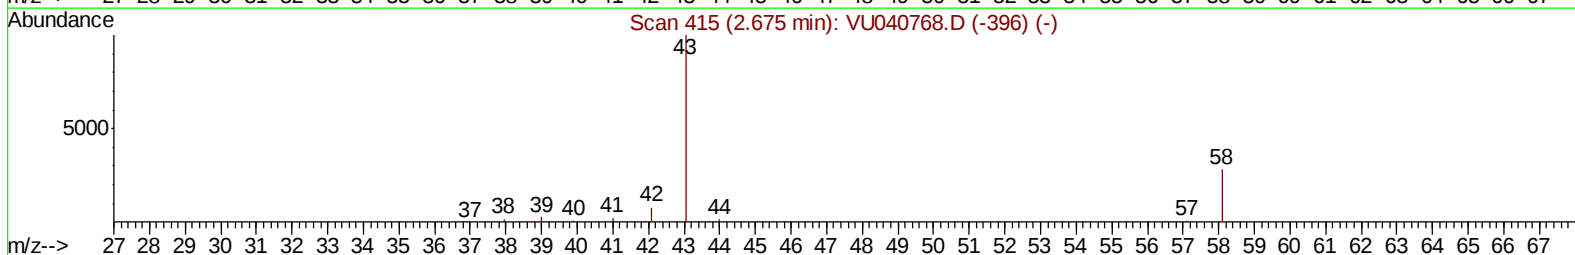
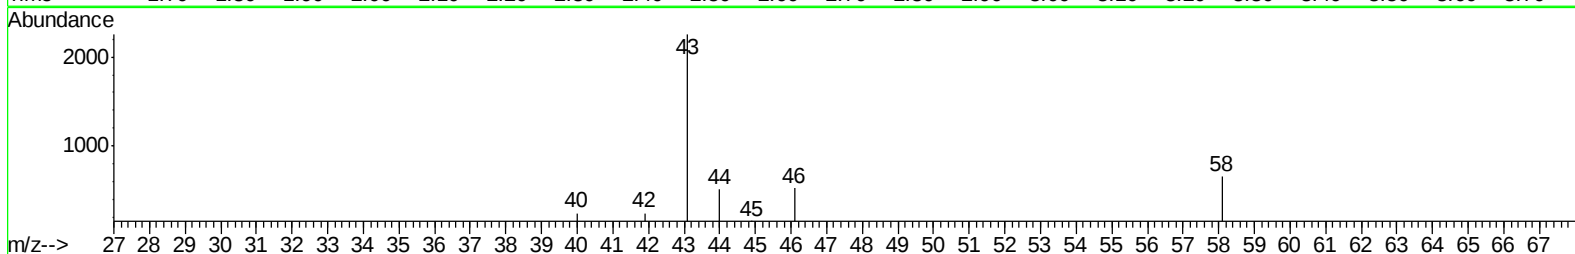


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101720\
Data File : VU040777.D
Acq On : 17 Oct 2020 21:37
Operator : SY/MD
Sample : L4423-05
Misc : 25.4mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Oct 19 03:10:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 19 03:08:11 2020
Response via : Initial Calibration

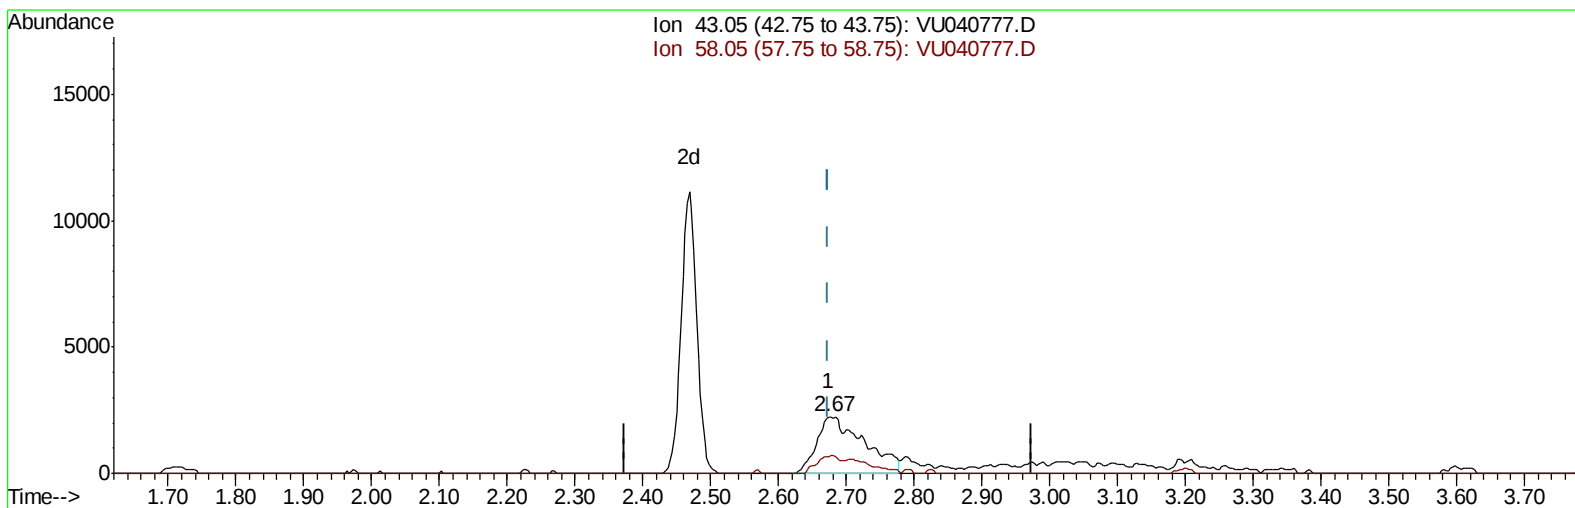

TIC: VU040777.D

(13) Acetone (T)

2.674min (-0.000) 4.59ug/L m

response 10913

Ion	Exp%	Act%
43.05	100	100
58.05	30.30	16.05
0.00	0.00	0.00
0.00	0.00	0.00