


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101720\
Data File : VU040777.D
Acq On : 17 Oct 2020 21:37
Operator : SY/MD
Sample : L4423-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFSG4

Manual Integrations
APPROVED

apatel
10/22/2020 9:09:48 AM

Quant Time: Oct 19 04:32:15 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 19 03:08:11 2020
Response via : Initial Calibration

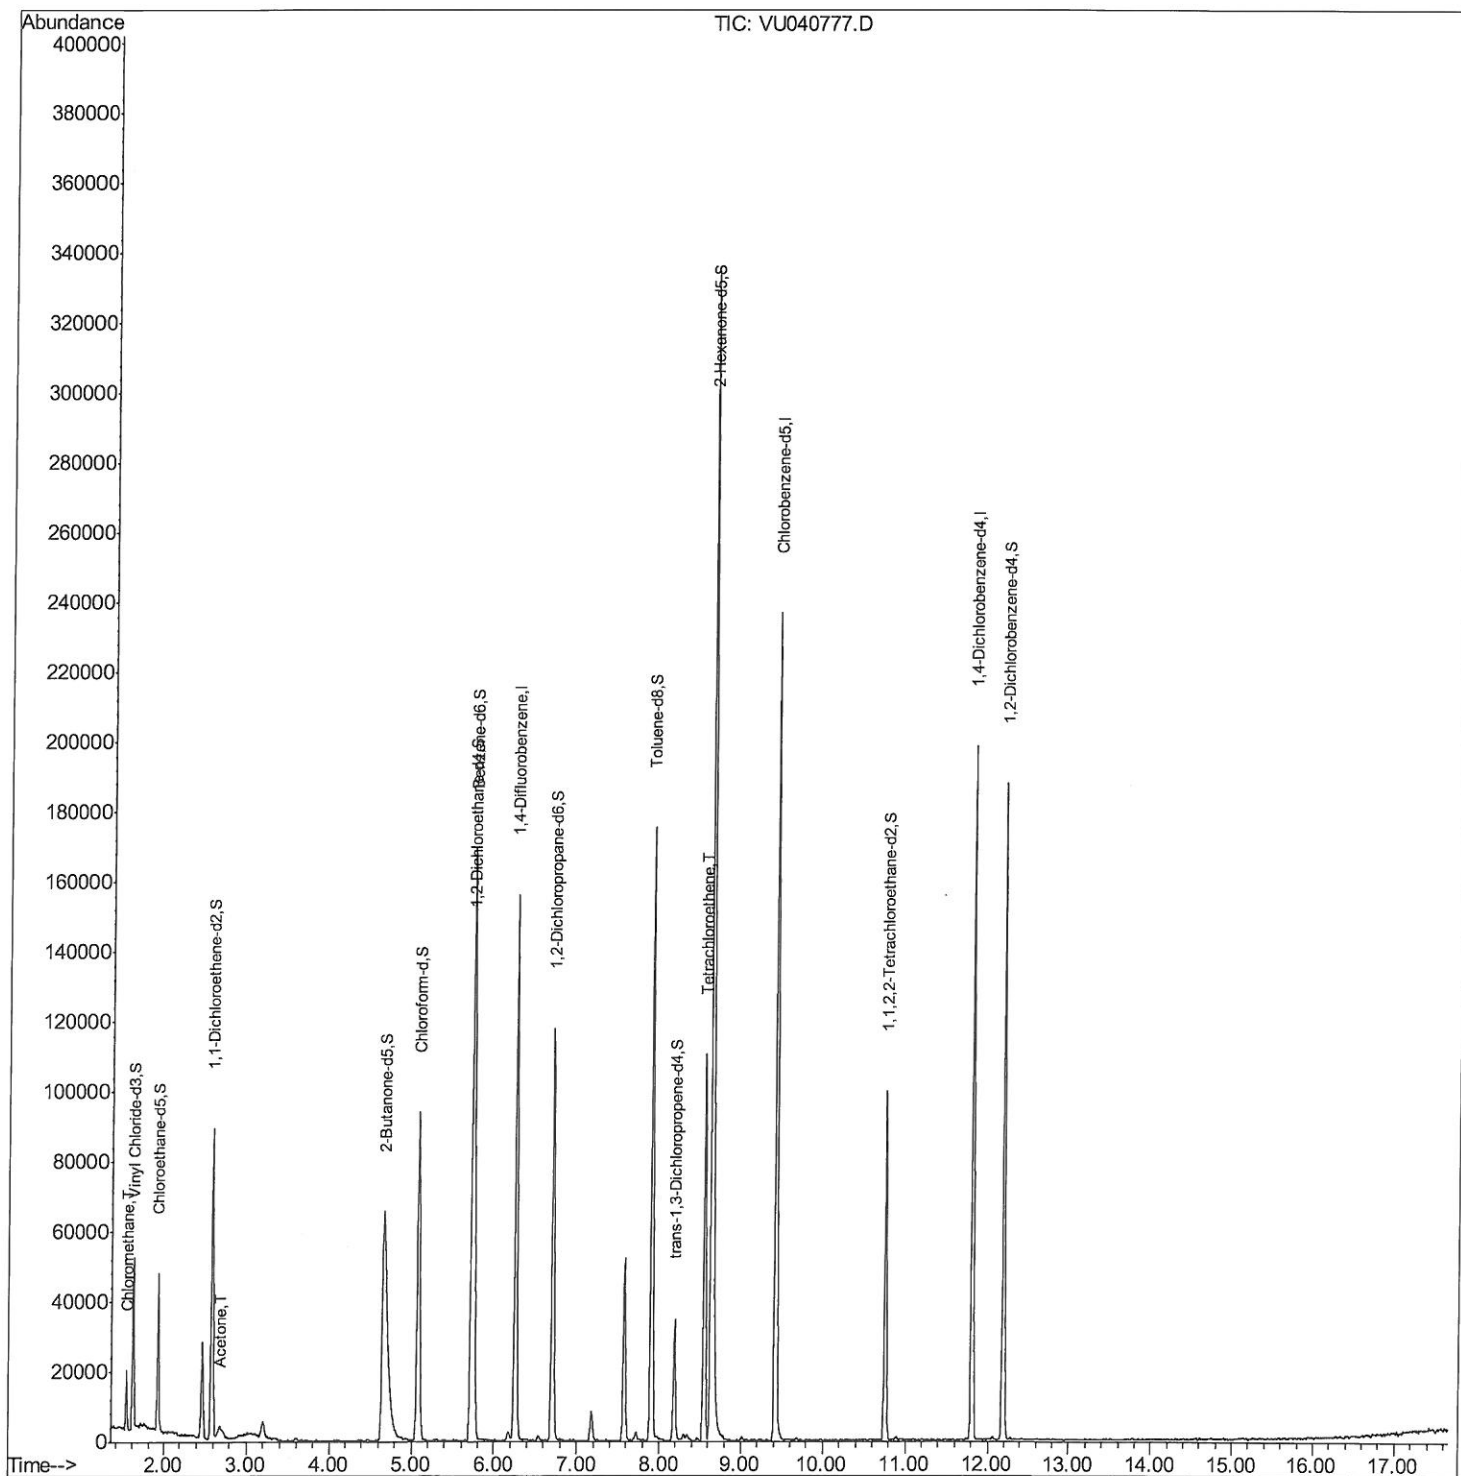

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101720\
Data File : VU040777.D
Acq On : 17 Oct 2020 21:37
Operator : SY/MD
Sample : L4423-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFSG4

Manual Integrations
APPROVED

apatel
10/22/2020 9:09:48 AM

Quant Time: Oct 19 03:10:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Oct 19 03:08:11 2020
Response via : Initial Calibration

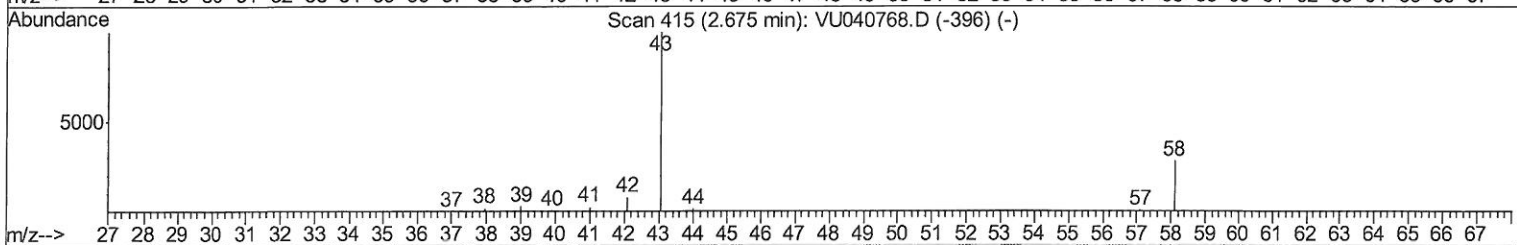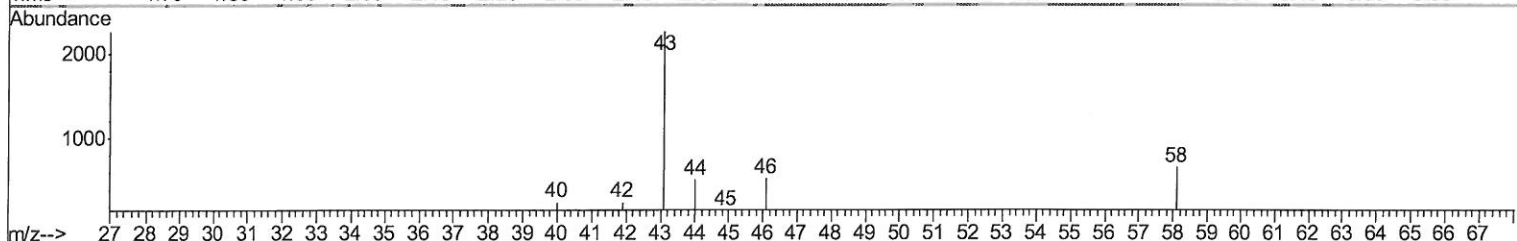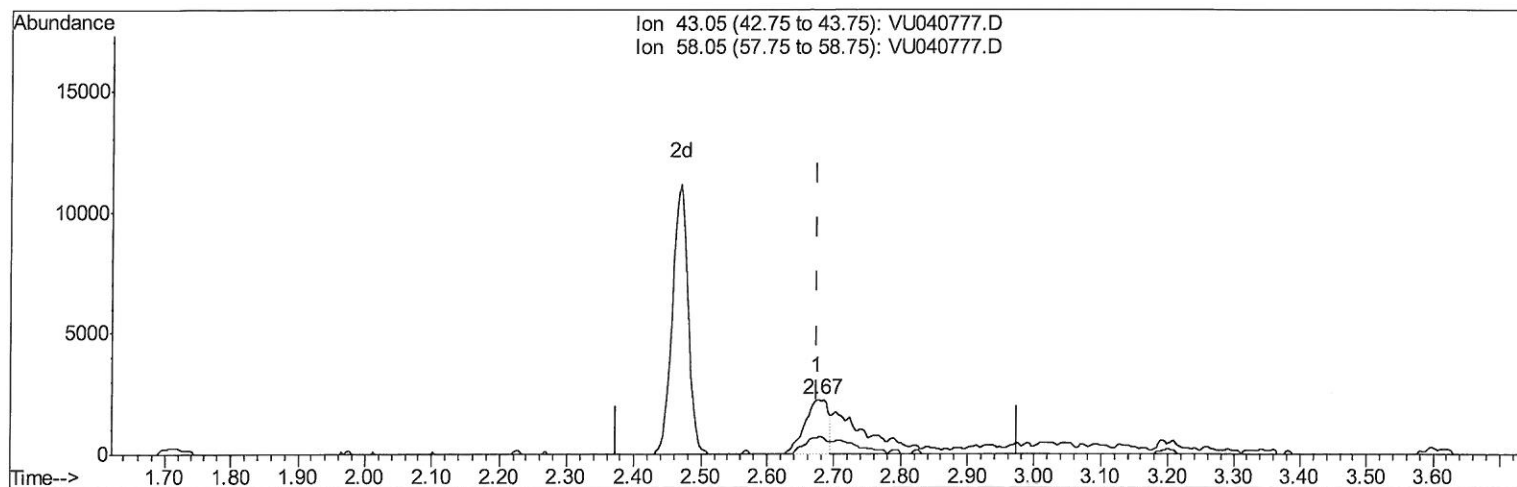

TIC: VU040777.D

(13) Acetone (T)

2.674min (-0.000) 2.29ug/L

response 5447

Ion	Exp%	Act%
43.05	100	100
58.05	30.30	32.15
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101720\
 Data File : VU040777.D
 Acq On : 17 Oct 2020 21:37
 Operator : SY/MD
 Sample : L4423-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFGS4

Manual Integrations
 APPROVED

apatel
 10/22/2020 9:09:48 AM

Quant Time: Oct 19 03:10:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 19 03:08:11 2020
 Response via : Initial Calibration

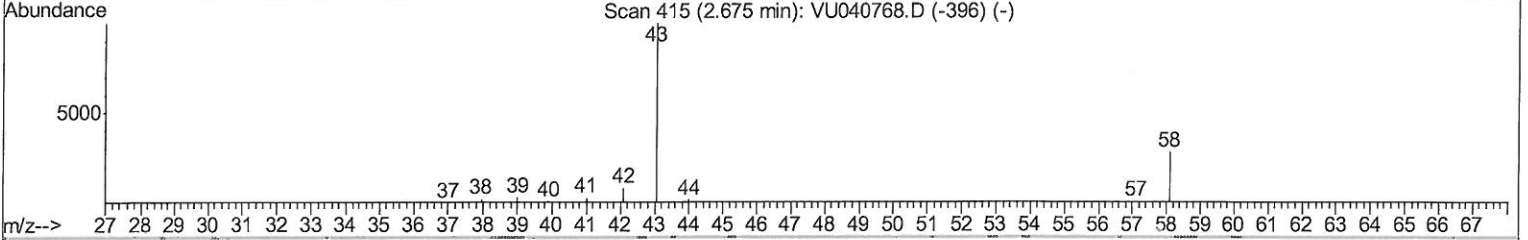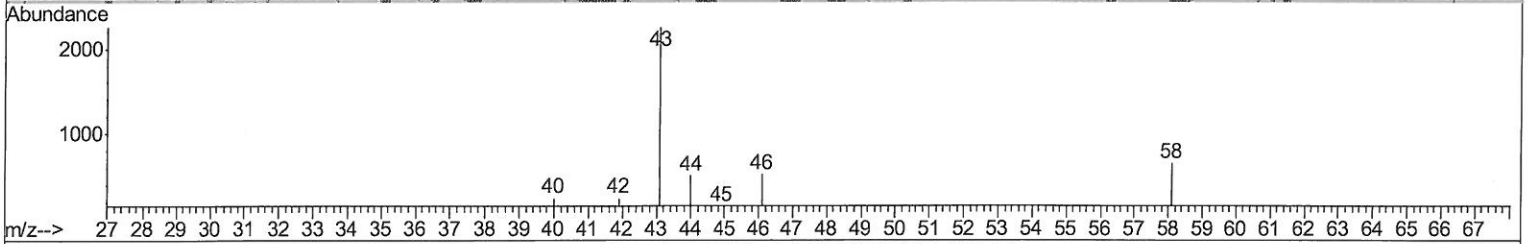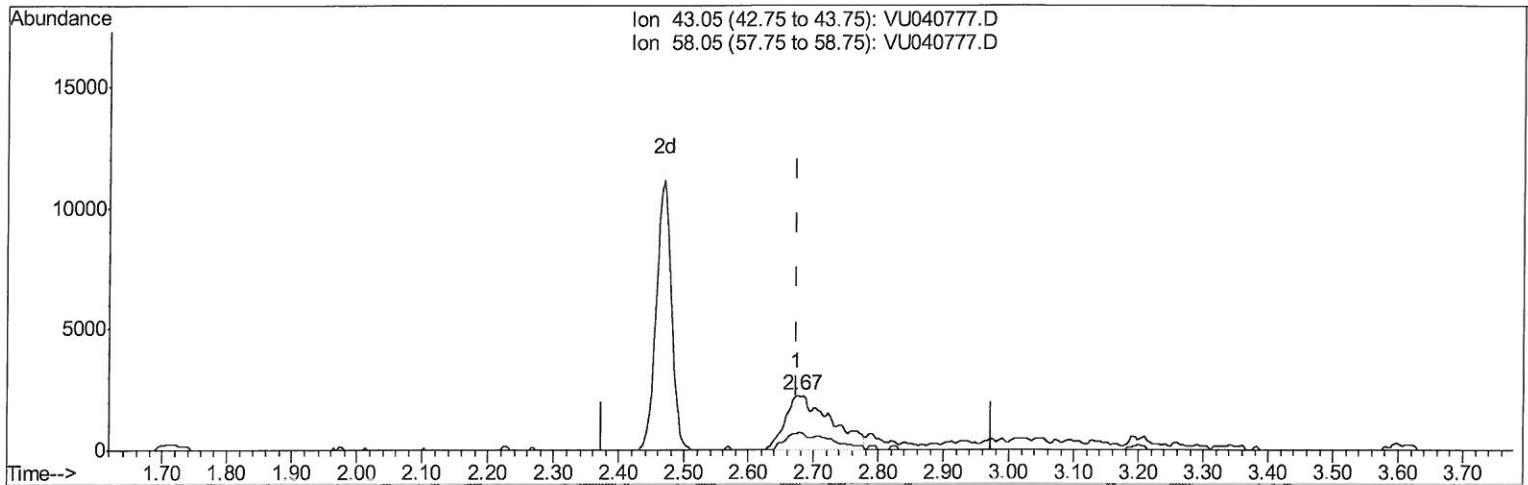

TIC: VU040777.D

(13) Acetone (T)

2.674min (-0.000) 4.59ug/L m

response 10913

Ion	Exp%	Act%
43.05	100	100
58.05	30.30	16.05
0.00	0.00	0.00
0.00	0.00	0.00

MD
10/22/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101720\
 Data File : VU040777.D
 Acq On : 17 Oct 2020 21:37
 Operator : SY/MD
 Sample : L4423-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFGS4

Manual Integrations
 APPROVED

apatel
 10/22/2020 9:09:48 AM

Quant Time: Oct 19 04:32:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Oct 19 03:08:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	115757	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	123829	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	49775	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	31721	3.31	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.20%
7) Chloroethane-d5	1.93	69	31970	4.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.40%
11) 1,1-Dichloroethene-d2	2.58	63	55422	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	4.66	46	172413	56.17	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.34%
24) Chloroform-d	5.08	84	83204	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.72	65	51927	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.20%
32) Benzene-d6	5.75	84	143292	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.80%
36) 1,2-Dichloropropane-d6	6.70	67	50955	4.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.00%
41) Toluene-d8	7.91	98	108357	3.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.40%
43) trans-1,3-Dichloropropene-	8.19	79	19514	4.15	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.00%
46) 2-Hexanone-d5	8.64	63	117672	48.62	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.24%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	48340	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	46650	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%

Target Compounds

Target Compounds					Ovalue
3) Chloromethane	1.53	50	12042	1.228	ug/L 100
13) Acetone	2.67	43	10913m	4.587	ug/L
47) Tetrachloroethene	8.56	164	24038	3.267	ug/L 95

MD
 10/22/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed