
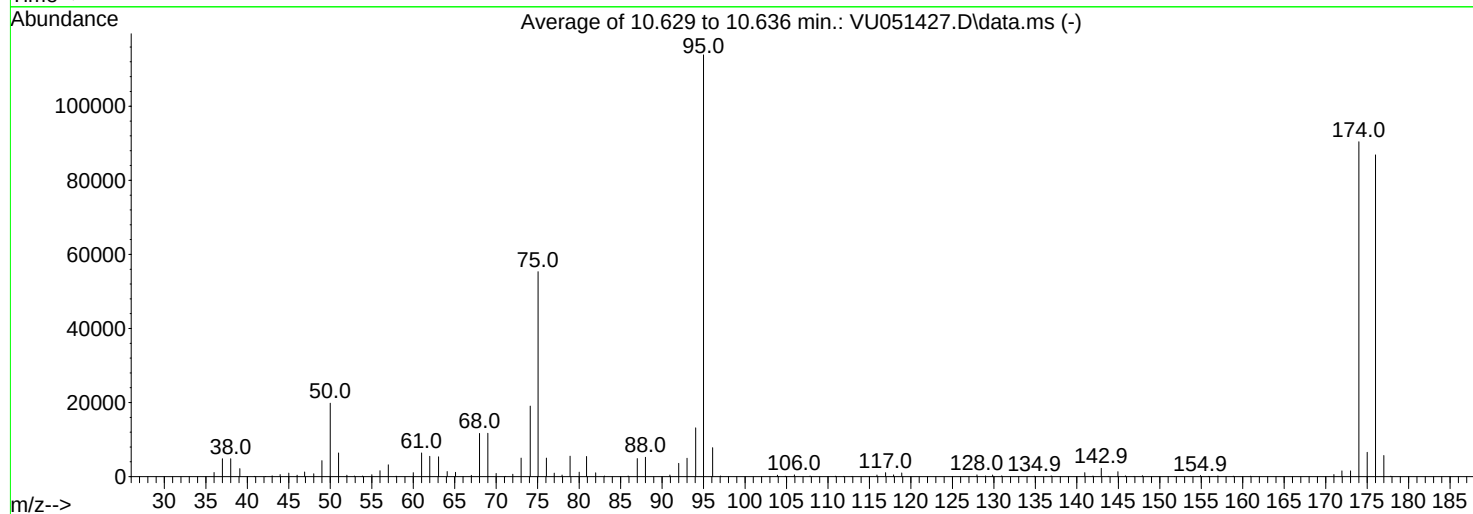


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101722\
 Data File : VU051427.D
 Acq On : 17 Oct 2022 14:03
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Tue Oct 18 04:53:19 2022

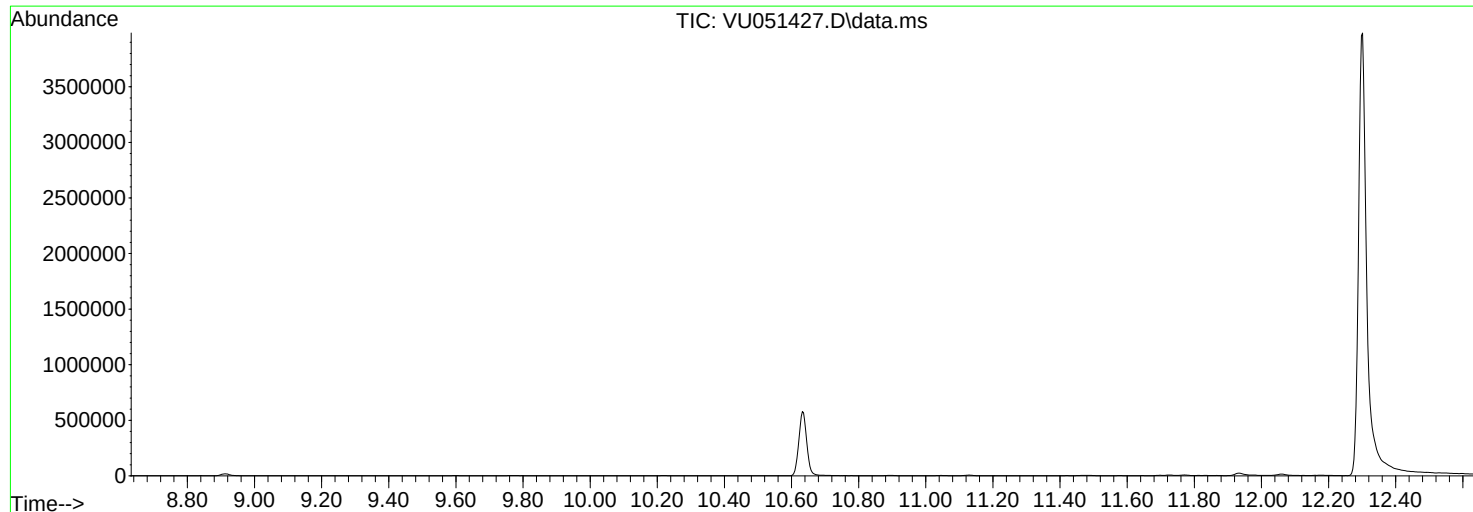

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	19819	PASS
75	95	30	60	48.6	55341	PASS
95	95	100	100	100.0	113880	PASS
96	95	5	9	6.9	7822	PASS
173	174	0.00	2	1.7	1579	PASS
174	95	50	100	79.4	90408	PASS
175	174	5	9	7.3	6576	PASS
176	174	95	101	96.1	86877	PASS
177	176	5	9	6.6	5698	PASS