

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101723\
 Data File : VU055788.D
 Acq On : 17 Oct 2023 12:58
 Operator : MD/SY
 Sample : 04874-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	116	rVB	249835	286119	12.63%	1.697%
2	1.911	185	193	217	rVB	213582	282460	12.47%	1.675%
3	2.566	384	397	415	rBV	415229	692135	30.56%	4.105%
4	2.972	521	523	525	rVB	536	165	0.01%	0.001%
5	3.036	536	543	545	rBV4	3278	3193	0.14%	0.019%
6	3.116	566	568	572	rBV2	170	119	0.01%	0.001%
7	3.142	572	576	578	rBV3	400	285	0.01%	0.002%
8	3.280	617	619	623	rVB	273	159	0.01%	0.001%
9	3.303	623	626	629	rBV2	420	295	0.01%	0.002%
10	3.335	634	636	639	rBV2	129	68	0.00%	0.000%
11	3.354	639	642	645	rBV2	422	288	0.01%	0.002%
12	3.399	655	656	659	rBV	309	165	0.01%	0.001%
13	3.441	666	669	670	rBV2	203	130	0.01%	0.001%
14	3.454	670	673	677	rVV3	302	225	0.01%	0.001%
15	3.595	715	717	718	rBV	183	67	0.00%	0.000%
16	3.631	725	728	729	rBV2	247	136	0.01%	0.001%
17	3.705	749	751	752	rBV	194	76	0.00%	0.000%
18	3.718	752	755	756	rVV	248	132	0.01%	0.001%
19	3.743	759	763	768	rVB	454	436	0.02%	0.003%
20	3.769	768	771	776	rBV2	277	250	0.01%	0.001%
21	3.862	795	800	802	rBV2	347	296	0.01%	0.002%
22	3.907	813	814	816	rBV2	257	113	0.00%	0.001%
23	3.965	827	832	835	rBV2	212	221	0.01%	0.001%
24	4.116	874	879	881	rBV	240	220	0.01%	0.001%
25	4.148	884	889	892	rBV2	278	294	0.01%	0.002%
26	4.248	917	920	921	rBV2	159	76	0.00%	0.000%
27	4.299	933	936	940	rBV	295	256	0.01%	0.002%
28	4.364	955	956	957	rBV	138	28	0.00%	0.000%
29	4.399	964	967	969	rVB2	302	152	0.01%	0.001%
30	4.412	969	971	974	rBV	268	125	0.01%	0.001%
31	4.444	975	981	986	rBV2	257	396	0.02%	0.002%
32	4.521	1002	1005	1009	rBV	346	273	0.01%	0.002%
33	4.563	1015	1018	1021	rBV	164	95	0.00%	0.001%
34	4.615	1022	1034	1062	rBV	200937	525496	23.20%	3.116%
35	5.058	1156	1172	1199	rBV	416900	930560	41.08%	5.519%
36	5.348	1258	1262	1266	rVB3	862	613	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101723\
 Data File : VU055788.D
 Acq On : 17 Oct 2023 12:58
 Operator : MD/SY
 Sample : 04874-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	5.406	1278	1280	1283	rVB2	574	297	0.01%	0.002%
38	5.515	1310	1314	1315	rBV2	248	127	0.01%	0.001%
39	5.531	1317	1319	1321	rBV2	396	179	0.01%	0.001%
40	5.550	1323	1325	1330	rBV2	244	200	0.01%	0.001%
41	5.624	1346	1348	1349	rBV	149	51	0.00%	0.000%
42	5.721	1357	1378	1404	rBV2	819573	2265012	100.00%	13.432%
43	6.171	1514	1518	1519	rBV	300	175	0.01%	0.001%
44	6.245	1528	1541	1574	rBV	614279	1214064	53.60%	7.200%
45	6.528	1620	1629	1649	rVB2	31327	62648	2.77%	0.372%
46	6.614	1654	1656	1658	rBV2	363	186	0.01%	0.001%
47	6.688	1664	1679	1700	rBV	513875	1032096	45.57%	6.121%
48	6.930	1751	1754	1757	rVB2	692	301	0.01%	0.002%
49	6.959	1761	1763	1765	rBV2	268	86	0.00%	0.001%
50	7.013	1777	1780	1785	rVB2	507	376	0.02%	0.002%
51	7.042	1785	1789	1795	rBV2	267	274	0.01%	0.002%
52	7.097	1804	1806	1808	rBV	122	64	0.00%	0.000%
53	7.110	1808	1810	1811	rBV	346	135	0.01%	0.001%
54	7.164	1824	1827	1828	rBV2	601	345	0.02%	0.002%
55	7.193	1828	1836	1837	rBV3	2855	3022	0.13%	0.018%
56	7.277	1858	1862	1863	rBV2	207	121	0.01%	0.001%
57	7.312	1870	1873	1876	rVB2	354	208	0.01%	0.001%
58	7.332	1876	1879	1884	rVB2	394	280	0.01%	0.002%
59	7.354	1884	1886	1891	rVB2	238	183	0.01%	0.001%
60	7.380	1891	1894	1897	rBV2	136	111	0.00%	0.001%
61	7.415	1902	1905	1909	rVB3	384	295	0.01%	0.002%
62	7.441	1909	1913	1916	rBV2	241	196	0.01%	0.001%
63	7.476	1916	1924	1928	rBV2	387	486	0.02%	0.003%
64	7.563	1938	1951	1980	rBV	269571	500197	22.08%	2.966%
65	7.804	2023	2026	2029	rVB	453	261	0.01%	0.002%
66	7.830	2031	2034	2036	rBV	321	186	0.01%	0.001%
67	7.897	2041	2055	2084	rBV	976349	1739982	76.82%	10.319%
68	8.177	2130	2142	2162	rBV	189969	336711	14.87%	1.997%
69	8.393	2206	2209	2211	rVB2	817	443	0.02%	0.003%
70	8.412	2211	2215	2218	rBV	345	289	0.01%	0.002%
71	8.457	2227	2229	2233	rBV	245	145	0.01%	0.001%
72	8.534	2251	2253	2257	rBV2	193	124	0.01%	0.001%
73	8.557	2257	2260	2266	rVB5	621	687	0.03%	0.004%
74	8.582	2266	2268	2269	rBV	224	110	0.00%	0.001%
75	8.630	2270	2283	2326	rBV5	462159	1224067	54.04%	7.259%
76	8.981	2390	2392	2394	rBV	488	265	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101723\
 Data File : VU055788.D
 Acq On : 17 Oct 2023 12:58
 Operator : MD/SY
 Sample : 04874-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	9.093	2423	2427	2429	rBV	588	423	0.02%	0.003%
78	9.148	2442	2444	2446	rBV	222	102	0.00%	0.001%
79	9.164	2446	2449	2450	rBV3	602	342	0.02%	0.002%
80	9.264	2477	2480	2481	rBV	297	117	0.01%	0.001%
81	9.415	2514	2527	2553	rBV	920068	1544459	68.19%	9.159%
82	9.698	2612	2615	2617	rBV2	869	517	0.02%	0.003%
83	9.762	2633	2635	2637	rBV	449	256	0.01%	0.002%
84	9.894	2674	2676	2679	rBV	359	227	0.01%	0.001%
85	9.939	2688	2690	2692	rBV	335	131	0.01%	0.001%
86	10.013	2711	2713	2715	rBV2	427	190	0.01%	0.001%
87	10.174	2760	2763	2767	rBV2	442	309	0.01%	0.002%
88	10.399	2830	2833	2836	rBV	473	305	0.01%	0.002%
89	10.431	2841	2843	2844	rBV2	185	57	0.00%	0.000%
90	10.753	2930	2943	2964	rBV	717904	1191425	52.60%	7.066%
91	11.039	3029	3032	3037	rBV	552	439	0.02%	0.003%
92	11.216	3084	3087	3091	rBV2	506	433	0.02%	0.003%
93	11.701	3237	3238	3240	rVB	611	128	0.01%	0.001%
94	11.810	3259	3272	3296	rBV	864162	1422645	62.81%	8.437%
95	12.190	3377	3390	3411	rBV	953475	1588687	70.14%	9.422%




Sum of corrected areas: 16862294

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101723\
Data File : VU055788.D
Acq On : 17 Oct 2023 12:58
Operator : MD/SY
Sample : 04874-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

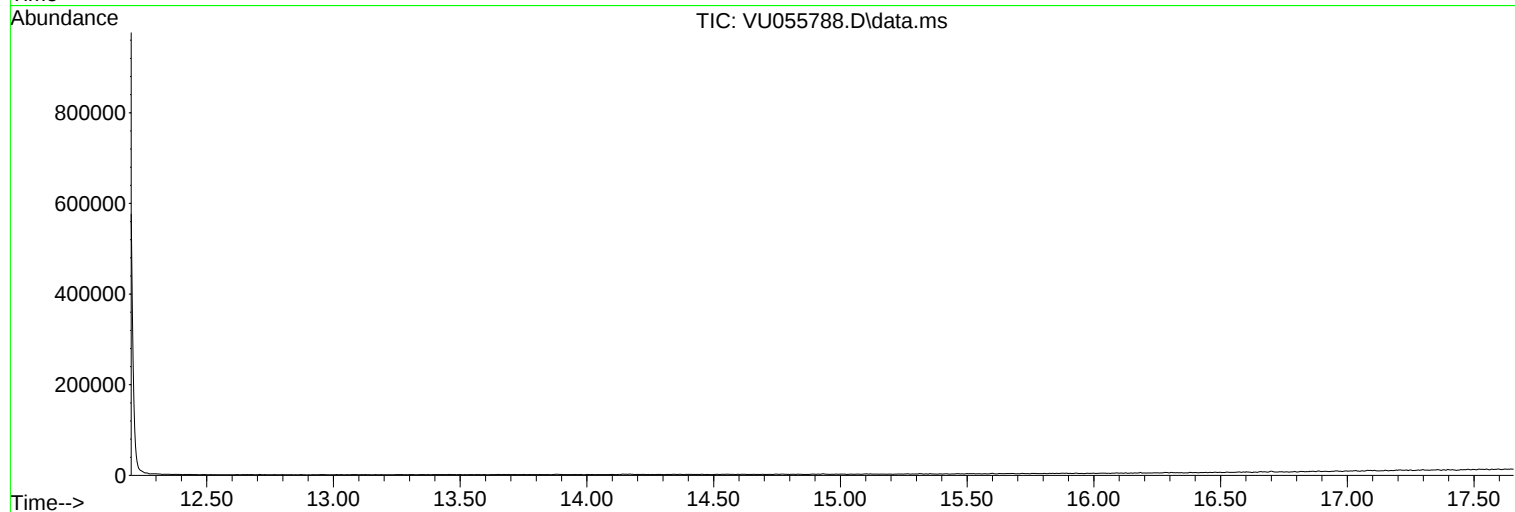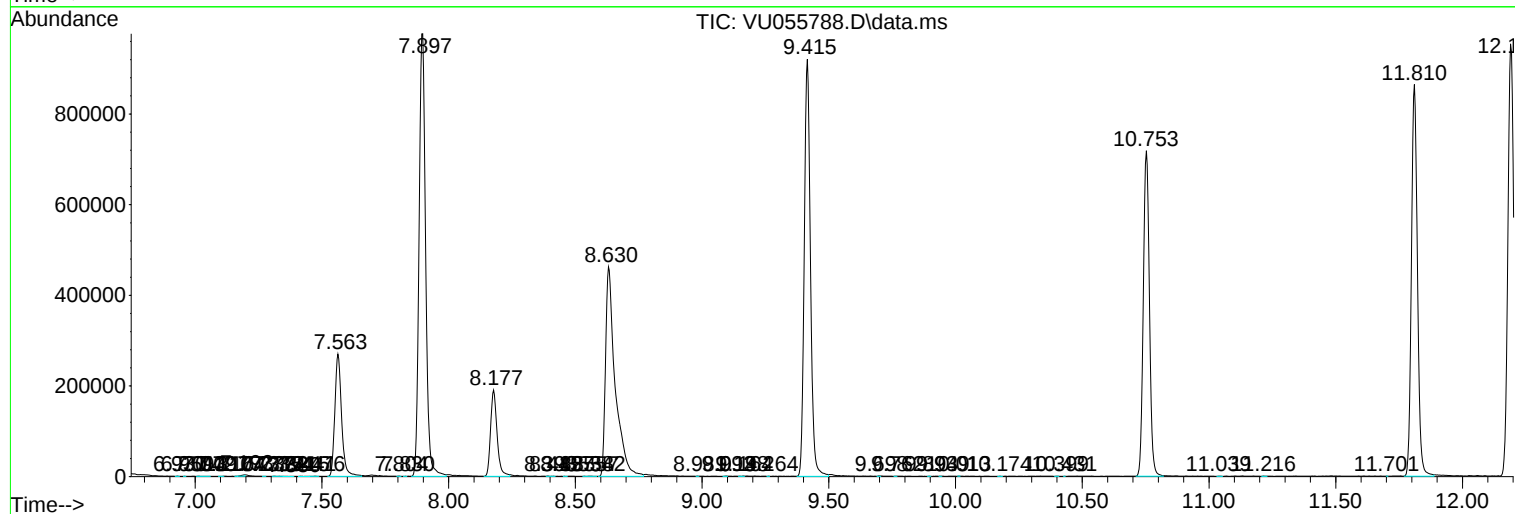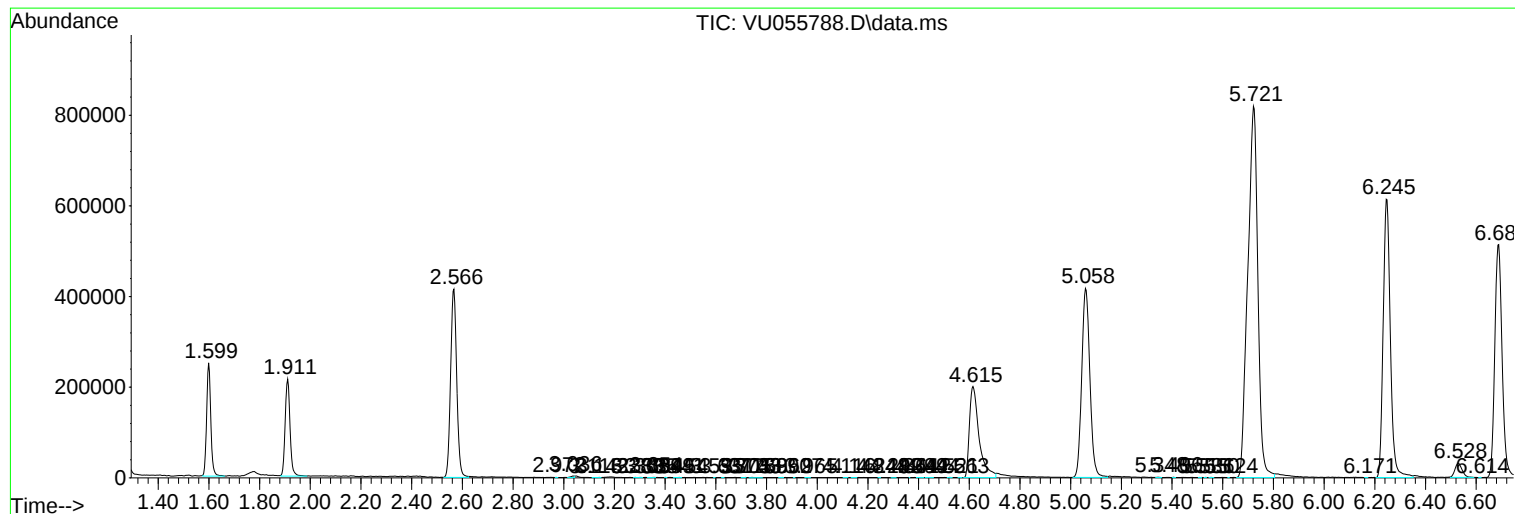

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101723\
Data File : VU055788.D
Acq On : 17 Oct 2023 12:58
Operator : MD/SY
Sample : 04874-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101723\
Data File : VU055788.D
Acq On : 17 Oct 2023 12:58
Operator : MD/SY
Sample : 04874-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------