

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101724\
 Data File : VU061147.D
 Acq On : 17 Oct 2024 17:05
 Operator : MD/SY
 Sample : VU1017WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1017WBL01

Quant Time: Oct 18 04:09:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Oct 18 02:52:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.110	96	27850	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	12896	0.871	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	13109	0.899	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101724\
Data File : VU061147.D
Acq On : 17 Oct 2024 17:05
Operator : MD/SY
Sample : VU1017WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1017WBL01

Quant Time: Oct 18 04:09:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Oct 18 02:52:28 2024
Response via : Initial Calibration




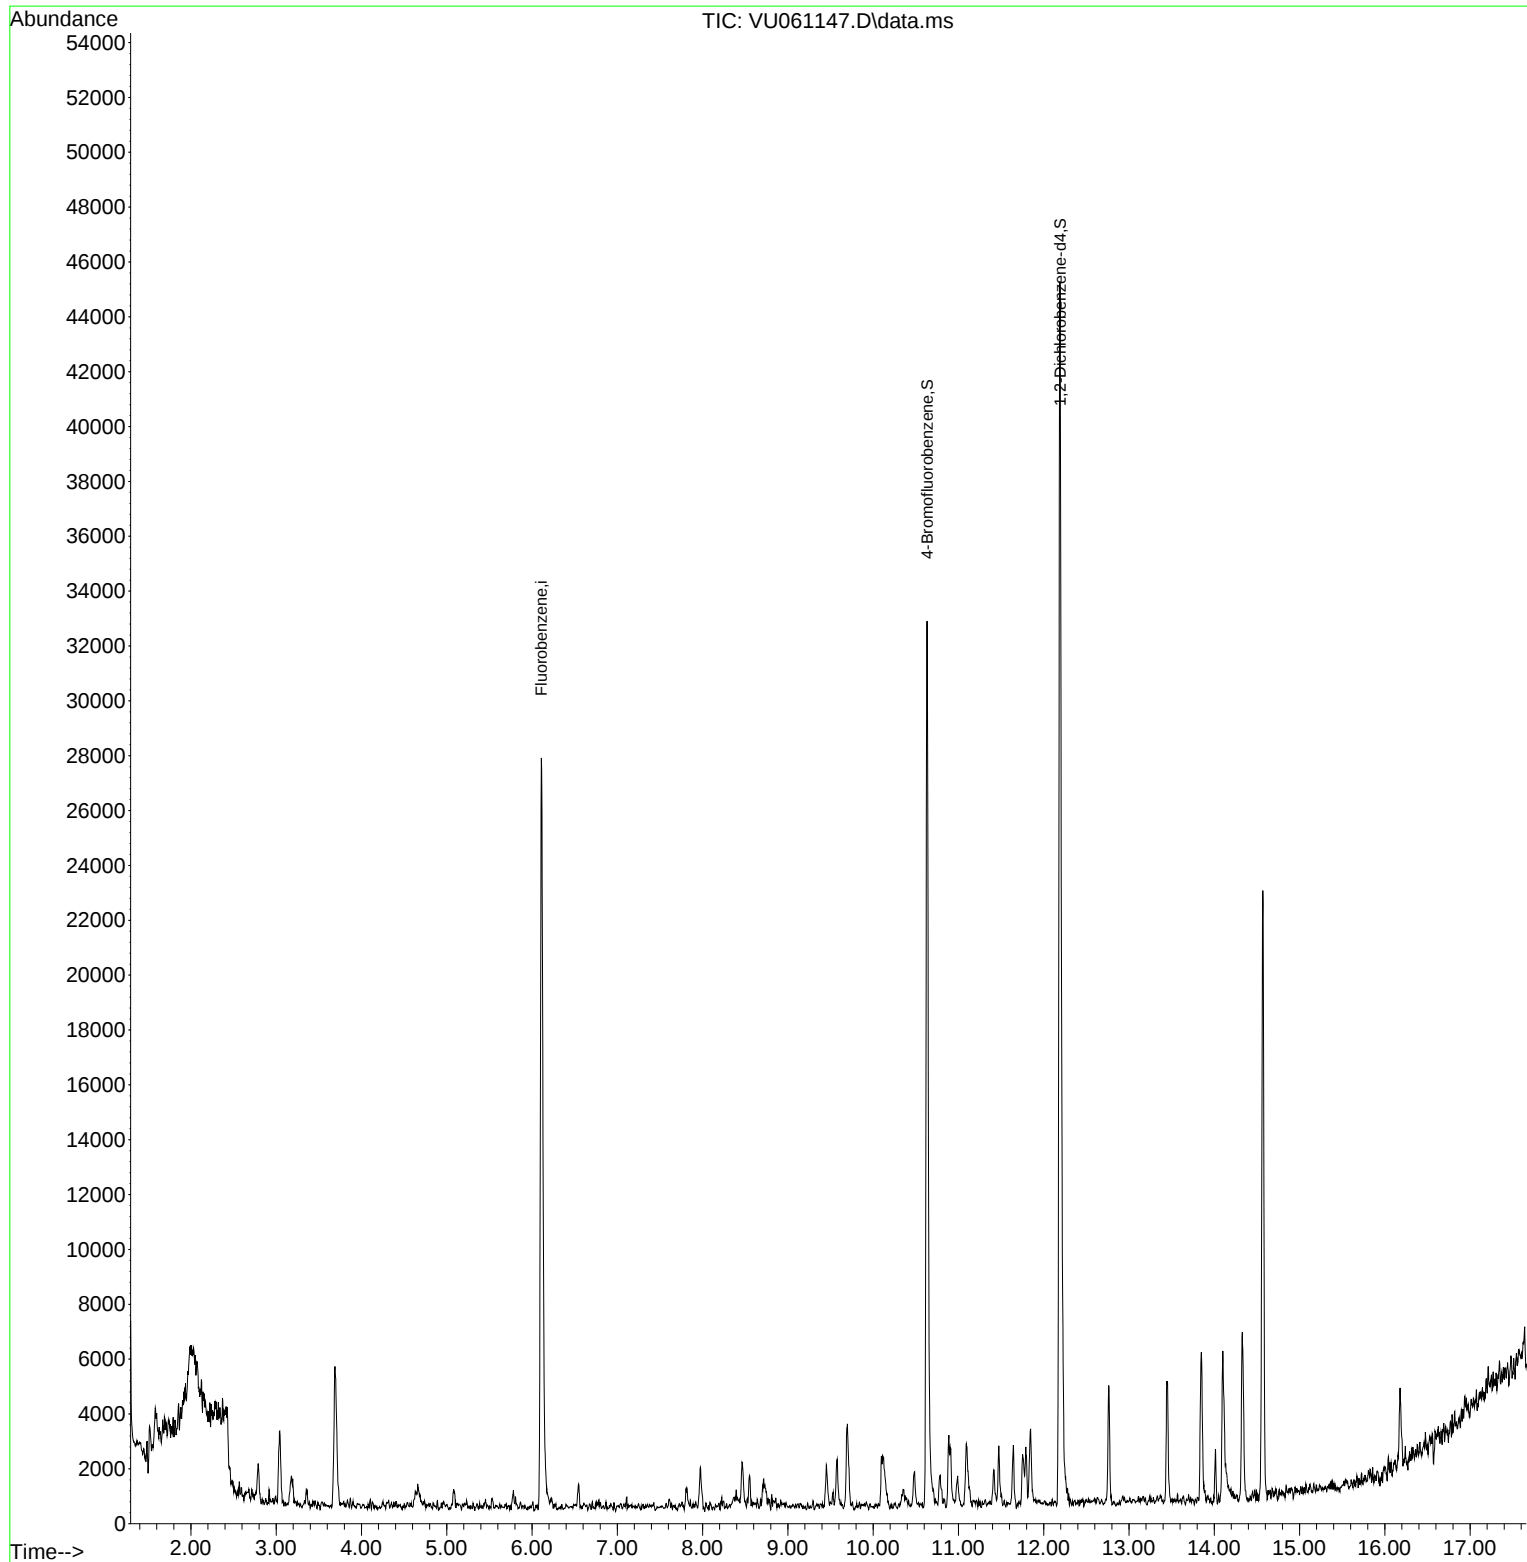


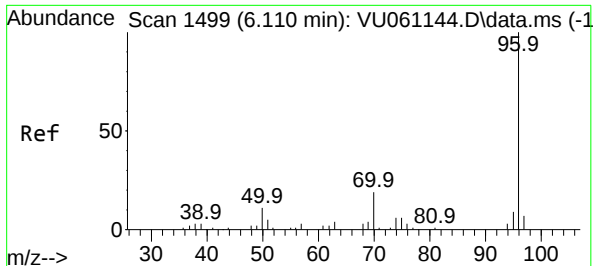

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.110 min Scan# 1499
Delta R.T. -0.000 min
Lab File: VU061147.D
Acq: 17 Oct 2024 17:05




Instrument :
MSVOA_U
ClientSampleId :
VU1017WBL01


Tgt Ion:	96	Resp:	27850
Ion	Ratio	Lower	Upper
96	100		
70	19.4	16.1	24.1
95	9.5	0.0	0.0#
97	6.9	0.0	0.0#

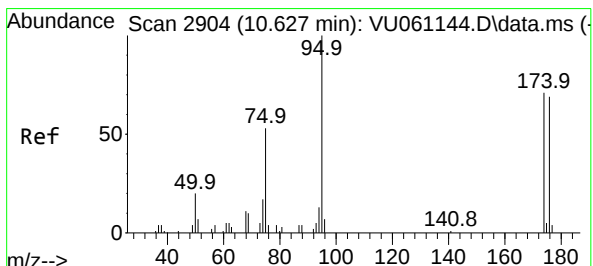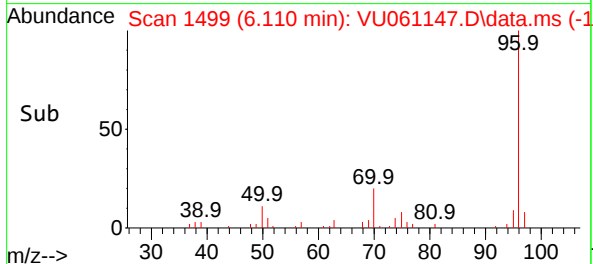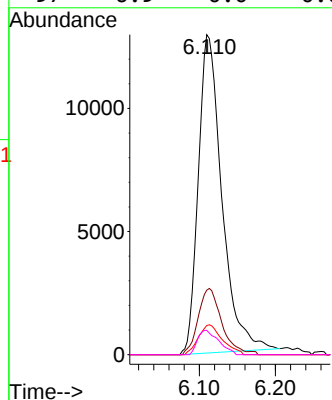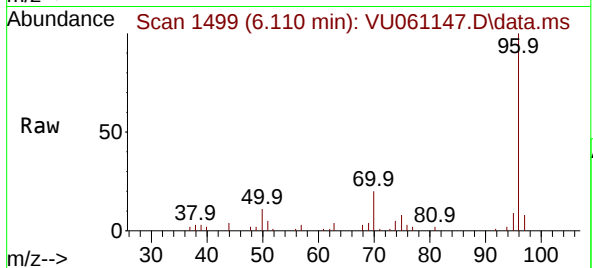

#57
4-Bromofluorobenzene
Concen: 0.871 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.006 min
Lab File: VU061147.D
Acq: 17 Oct 2024 17:05


Tgt Ion:	95	Resp:	12896
Ion	Ratio	Lower	Upper
95	100		
174	74.2	55.4	83.0
176	74.5	54.4	81.6

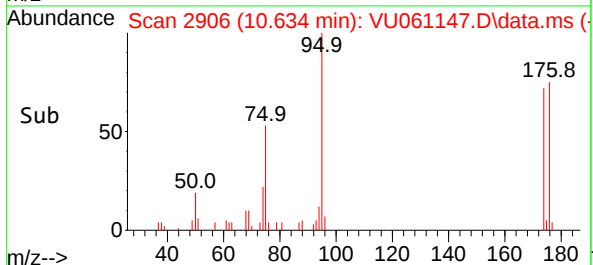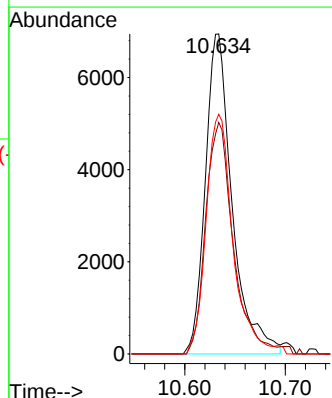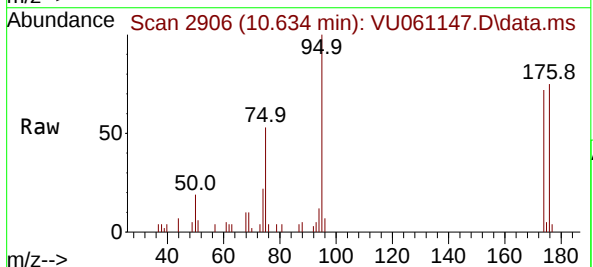

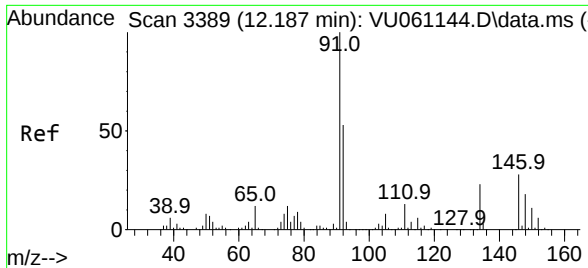

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.899 ug/l
 RT: 12.193 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VU061147.D
 Acq: 17 Oct 2024 17:05

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1017WBL01

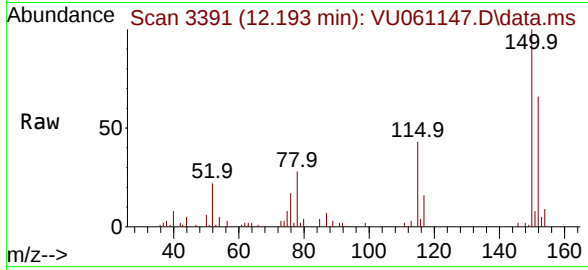

Tgt Ion:	152	Resp:	13109
Ion Ratio	Lower	Upper	
152	100		
115	67.4	0.0	275.0
150	154.5	0.0	668.8

