


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101724\
Data File : VU061139.D
Acq On : 17 Oct 2024 10:06
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Oct 18 02:52:28 2024

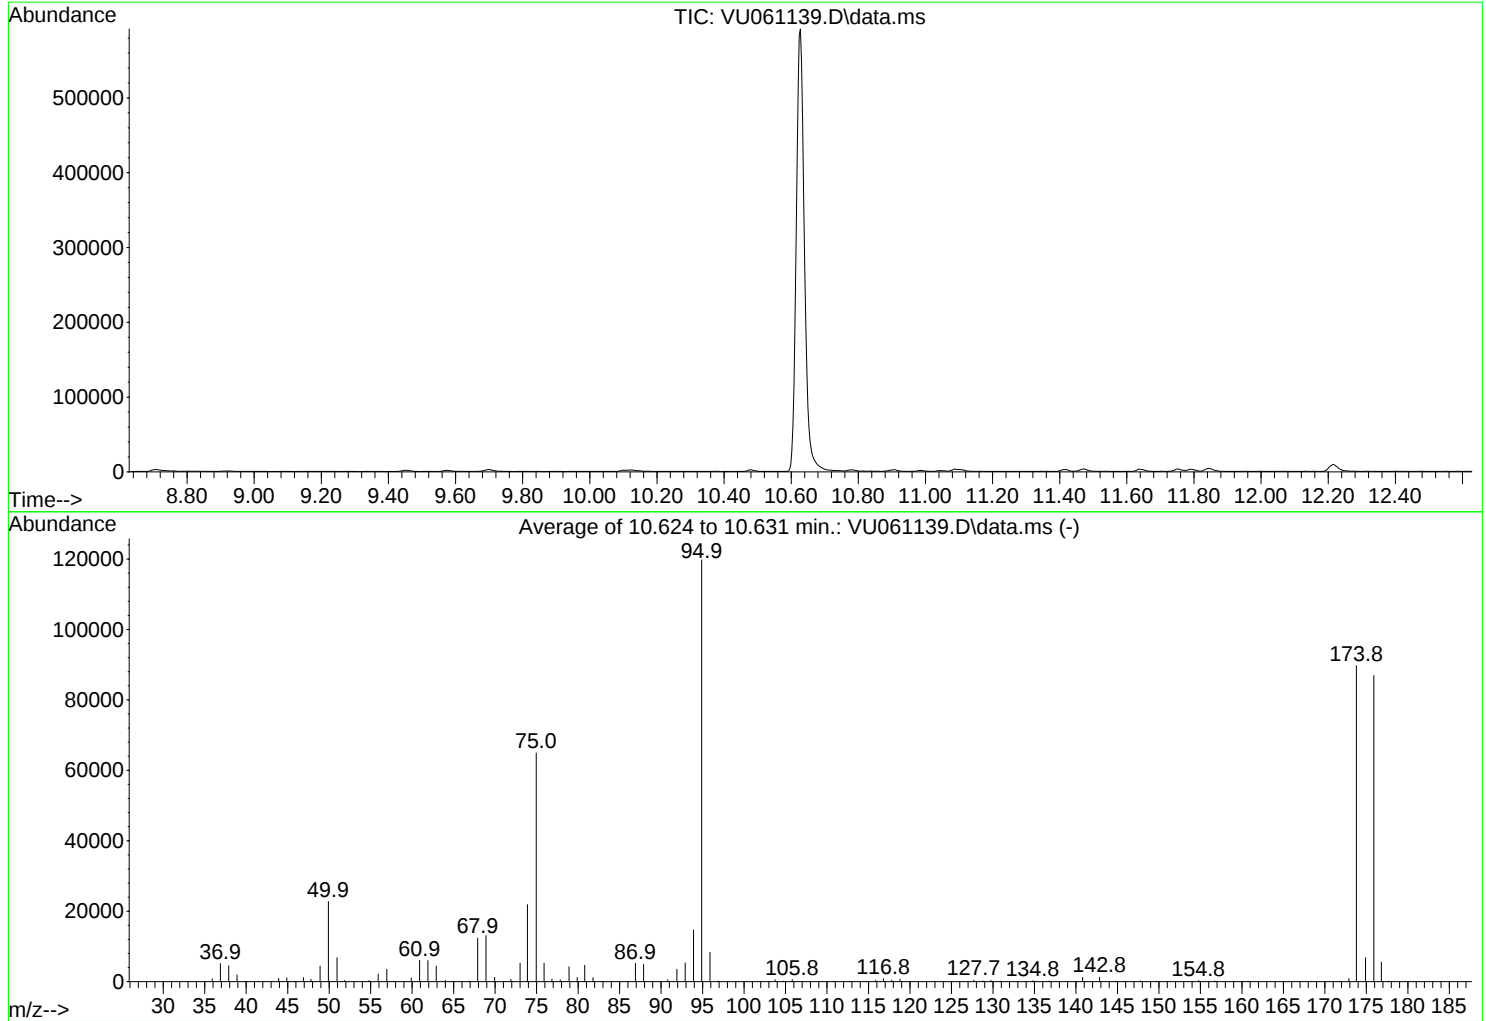

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	22733	PASS
75	95	30	60	54.2	64907	PASS
95	95	100	100	100.0	119760	PASS
96	95	5	9	6.9	8313	PASS
173	174	0.00	2	1.0	873	PASS
174	95	50	100	74.9	89688	PASS
175	174	5	9	7.6	6837	PASS
176	174	95	101	97.0	86957	PASS
177	176	5	9	6.4	5564	PASS