


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101818\
Data File : VU027689.D
Acq On : 18 Oct 2018 09:08
Operator : MD/SY
Sample : BFB45
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB45

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Oct 19 08:11:17 2018

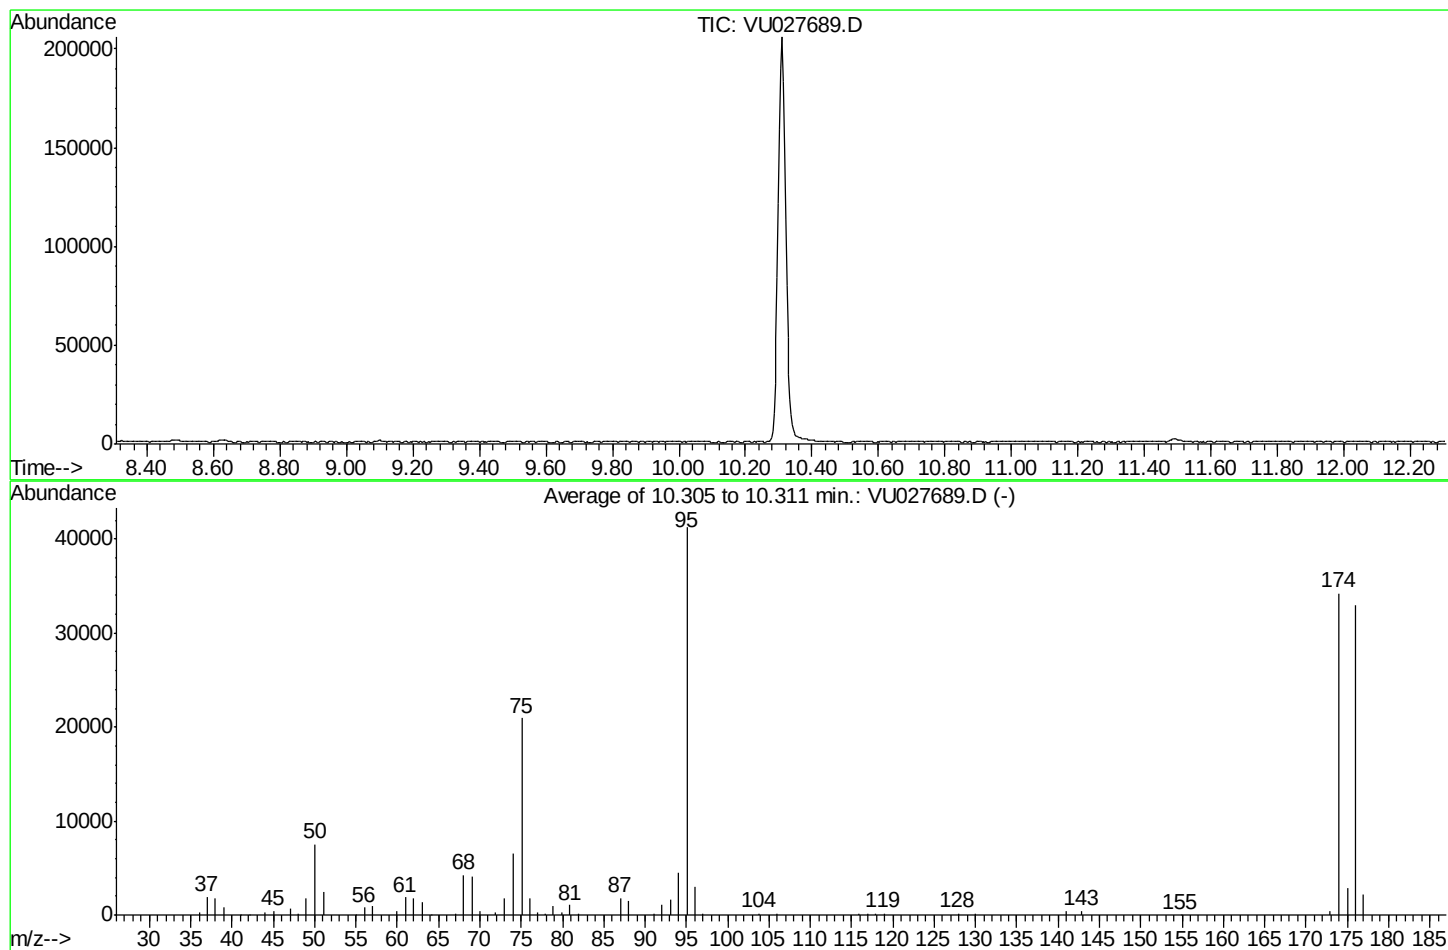

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	7537	PASS
75	95	30	80	50.7	20912	PASS
95	95	100	100	100.0	41250	PASS
96	95	5	9	7.3	3011	PASS
173	174	0.00	2	1.3	439	PASS
174	95	50	120	83.0	34245	PASS
175	174	5	9	8.2	2806	PASS
176	174	95	101	96.3	32962	PASS
177	176	5	9	6.6	2173	PASS

Scan 2828 (10.266 min): VU027689.D
BFB45

m/z	Abundance
39.90	130.0
41.10	159.0
43.00	227.0
44.00	408.0
55.00	158.0
57.00	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	306.0
37.00	1987.0
38.00	1654.0
39.00	778.0
41.00	154.0
42.10	101.0
43.10	174.0
44.00	634.0
45.00	432.0
47.00	618.0
48.00	195.0
49.00	1817.0
50.10	7231.0
51.10	2387.0
55.00	219.0
56.00	797.0
57.10	1062.0
59.90	373.0
61.00	1789.0
62.00	1744.0
63.00	1319.0
64.00	112.0
67.00	102.0
68.00	4013.0
69.00	3940.0
70.00	333.0
71.90	259.0
73.00	1780.0
74.00	6515.0
75.10	20104.0
76.10	1694.0
77.00	306.0
77.90	166.0
78.90	901.0
79.90	296.0
80.90	995.0
81.90	171.0
87.00	1710.0
88.00	1636.0
91.00	169.0
92.00	1112.0
93.10	1701.0
94.00	4313.0
95.10	39184.0
96.10	2964.0
97.00	102.0
103.80	188.0
105.90	163.0
115.90	132.0
117.00	173.0
117.90	125.0
118.90	178.0
127.90	150.0
129.90	160.0
141.00	294.0
142.90	414.0
173.00	453.0
174.00	31824.0
175.00	2681.0
176.00	30688.0
177.00	1999.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	307.0
37.00	2046.0
38.00	1783.0
39.00	836.0
39.90	104.0
41.00	180.0
42.10	111.0
43.10	171.0
44.00	652.0
45.00	475.0
47.00	646.0
48.00	197.0
49.00	1885.0
50.10	7671.0
51.10	2559.0
55.00	206.0
56.00	835.0
57.10	1118.0
60.00	395.0
61.00	1918.0
62.00	1787.0
63.00	1424.0
64.10	107.0
67.00	138.0
68.00	4394.0
69.00	4163.0
70.00	359.0
71.90	277.0
73.00	1851.0
74.00	6683.0
75.10	21656.0
76.10	1714.0
76.90	345.0
77.90	199.0
78.90	1031.0
79.90	312.0
80.90	1086.0
81.90	192.0
87.00	1891.0
88.00	1558.0
91.00	194.0
92.00	1142.0
93.00	1763.0
94.00	4674.0
95.10	42600.0
96.10	3131.0
96.90	108.0
103.80	212.0
105.90	181.0
115.90	137.0
117.00	204.0
117.90	136.0
118.90	208.0
127.90	168.0
129.90	155.0
140.90	380.0
142.80	455.0
173.00	453.0
174.00	35376.0
175.00	2901.0
176.00	33944.0
177.00	2289.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	297.0
37.00	1883.0
38.00	1775.0
39.00	760.0
39.90	118.0
41.00	185.0
43.10	186.0
44.00	646.0
45.00	484.0
47.00	637.0
48.00	203.0
49.00	1821.0
50.00	7710.0
51.10	2366.0
55.00	191.0
56.00	774.0
57.00	1135.0
60.00	402.0
61.00	1952.0
62.00	1707.0
63.00	1391.0
67.00	140.0
68.00	4345.0
69.10	4157.0
70.00	361.0
71.90	233.0
73.00	1857.0
74.00	6346.0
75.10	20976.0
76.00	1746.0
77.00	333.0
77.80	186.0
78.90	1067.0
79.90	276.0
80.90	1105.0
81.90	224.0
87.00	1851.0
88.00	1465.0
91.00	184.0
92.00	1129.0
93.00	1649.0
94.00	4563.0
95.10	41968.0
96.10	2939.0
96.90	119.0
103.80	201.0
105.90	184.0
115.90	129.0
117.00	223.0
117.90	148.0
118.90	217.0
127.90	154.0
129.90	147.0
140.90	461.0
142.80	427.0
154.90	122.0
172.90	413.0
174.00	35536.0
175.00	2837.0
176.00	34256.0
177.00	2231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45