

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101819\
 Data File : VU035265.D
 Acq On : 18 Oct 2019 14:30
 Operator : JC/SP
 Sample : K5318-12DL 4X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CH1DL

Quant Time: Oct 19 04:06:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 19 03:38:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	347336	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	336973	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	136544	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	95597	4.51	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.20%
7) Chloroethane-d5	1.93	69	90752	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.59	63	134509	3.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.80%
20) 2-Butanone-d5	4.72	46	289007	47.49	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.98%
24) Chloroform-d	5.11	84	184830	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	5.75	65	106002	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.77	84	374948	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
36) 1,2-Dichloropropane-d6	6.74	67	122843	5.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.40%
41) Toluene-d8	7.93	98	348874	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	8.22	79	53530	4.51	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.20%
46) 2-Hexanone-d5	8.69	63	234117	44.71	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.42%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	102362	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.80%
64) 1,2-Dichlorobenzene-d4	12.22	152	120666	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%


Target Compounds					Ovalue
47) Tetrachloroethene	8.58	164	133036	5.991 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101819\
Data File : VU035265.D
Acq On : 18 Oct 2019 14:30
Operator : JC/SP
Sample : K5318-12DL 4X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CH1DL

Quant Time: Oct 19 04:06:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 19 03:38:09 2019
Response via : Initial Calibration

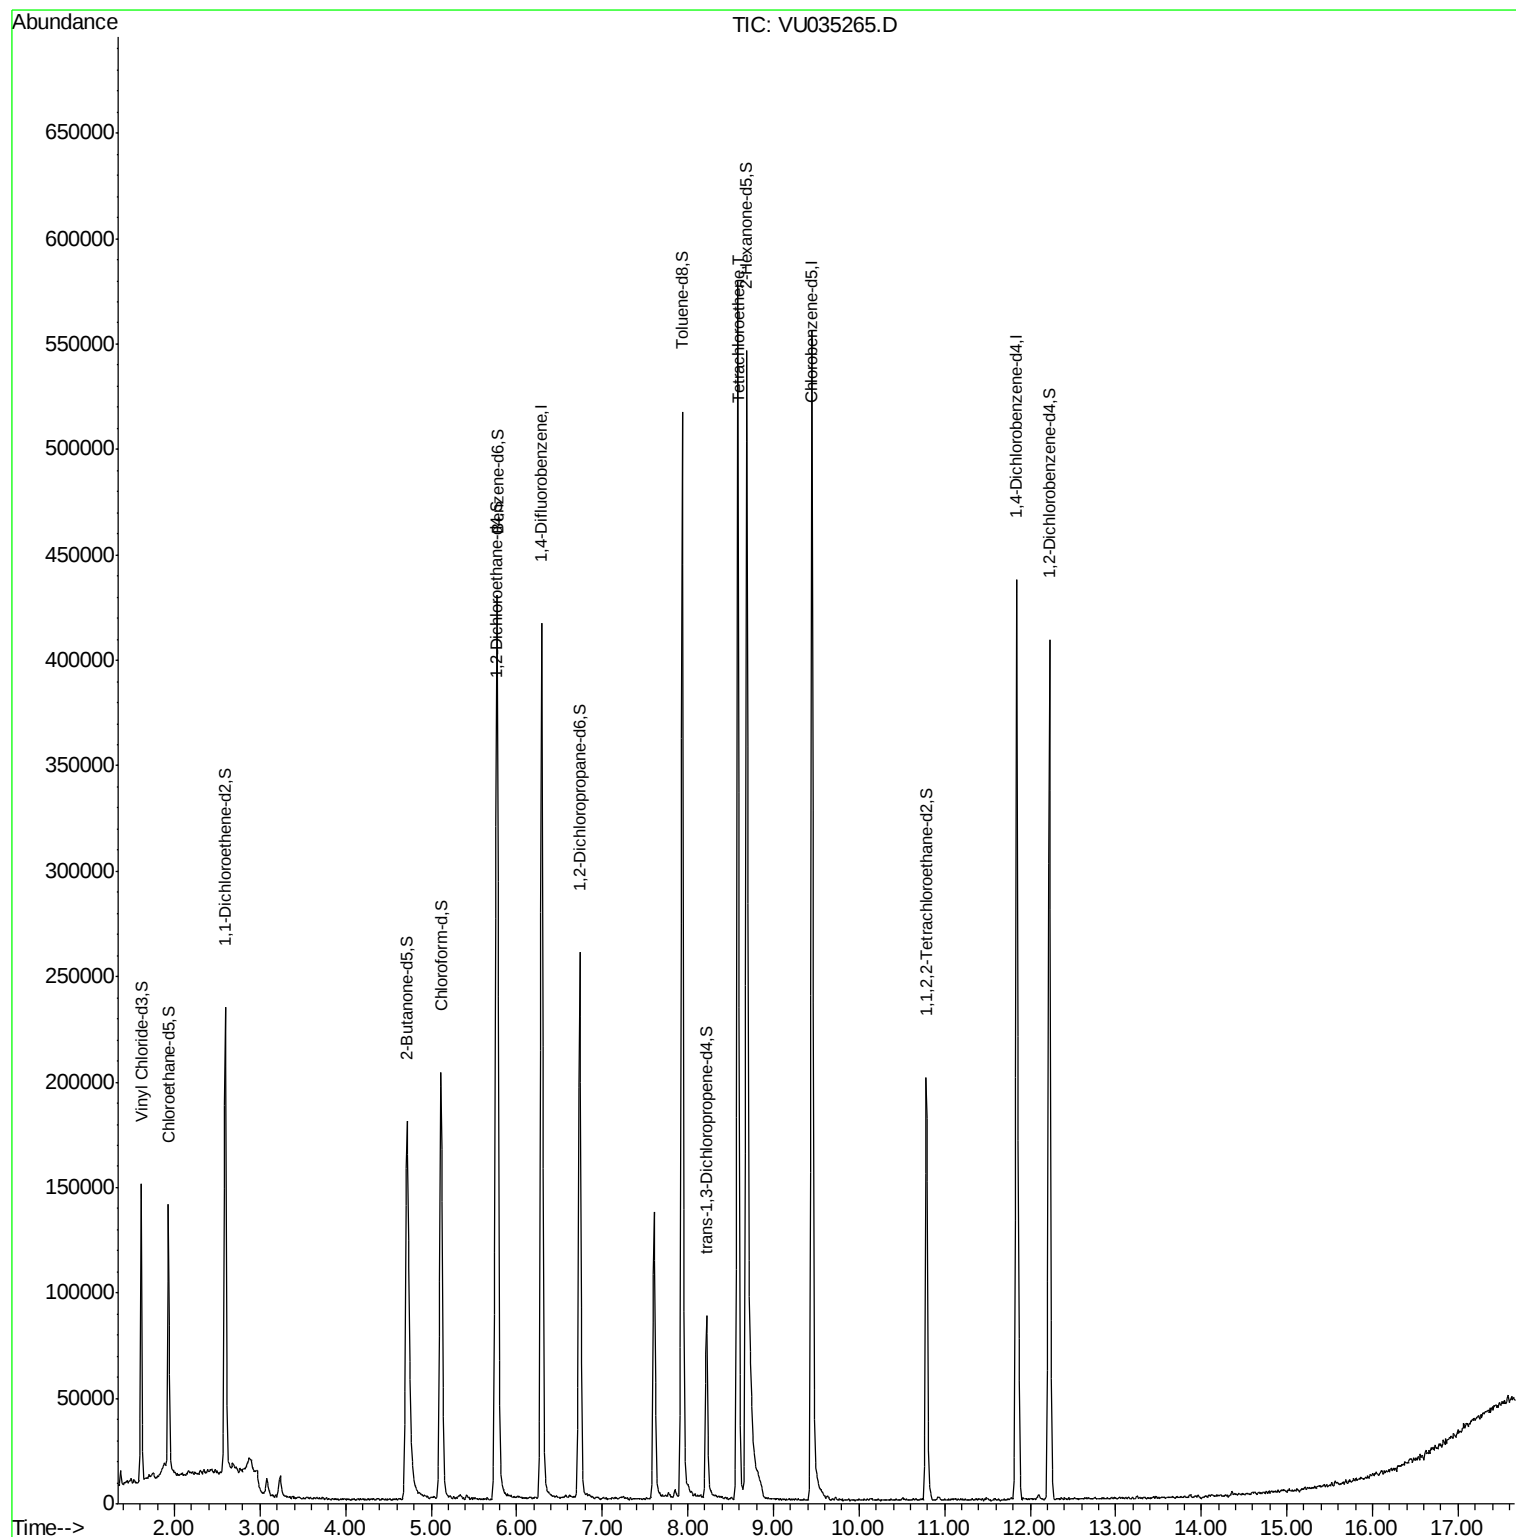

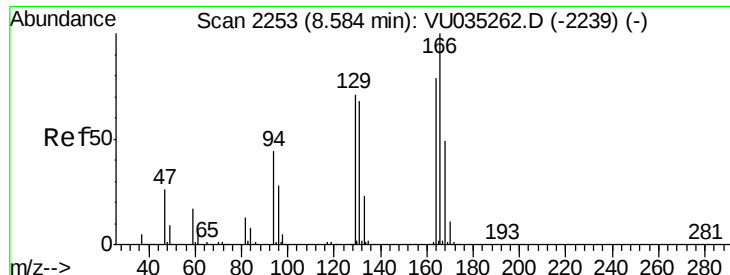

#47

Tetrachloroethene

Concen: 5.991 ug/L

RT: 8.58 min Scan# 2253

Delta R.T. -0.00 min

Lab File: VU035265.D


Acq: 18 Oct 2019 14:30

Instrument :

MSVOA_U

ClientSampleId :

C0CH1DL

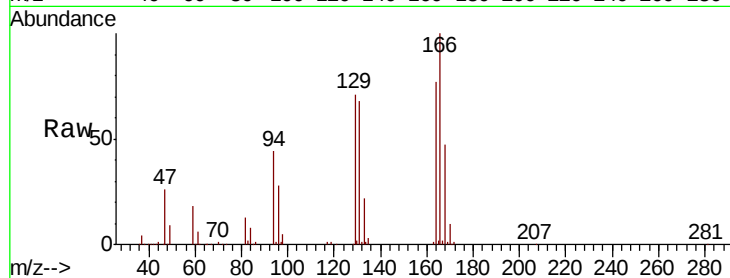

Tot Ion:164 Resp: 133036

Ion Ratio Lower Upper

164 100

129 91.7 65.2 121.0

131 88.7 62.9 116.9

166 129.5 91.5 169.9

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

