

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101823\
 Data File : VU055799.D
 Acq On : 18 Oct 2023 15:24
 Operator : MD/SY
 Sample : VU1018WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK12

Quant Time: Oct 19 03:41:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101823DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Oct 19 03:10:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	87833	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	29817	0.861	ug/l	0.00
Spiked Amount 1.000			Recovery	=	86.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	26003	0.810	ug/l	0.00
Spiked Amount 1.000			Recovery	=	81.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101823\
Data File : VU055799.D
Acq On : 18 Oct 2023 15:24
Operator : MD/SY
Sample : VU1018WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK12

Quant Time: Oct 19 03:41:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101823DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Oct 19 03:10:04 2023
Response via : Initial Calibration




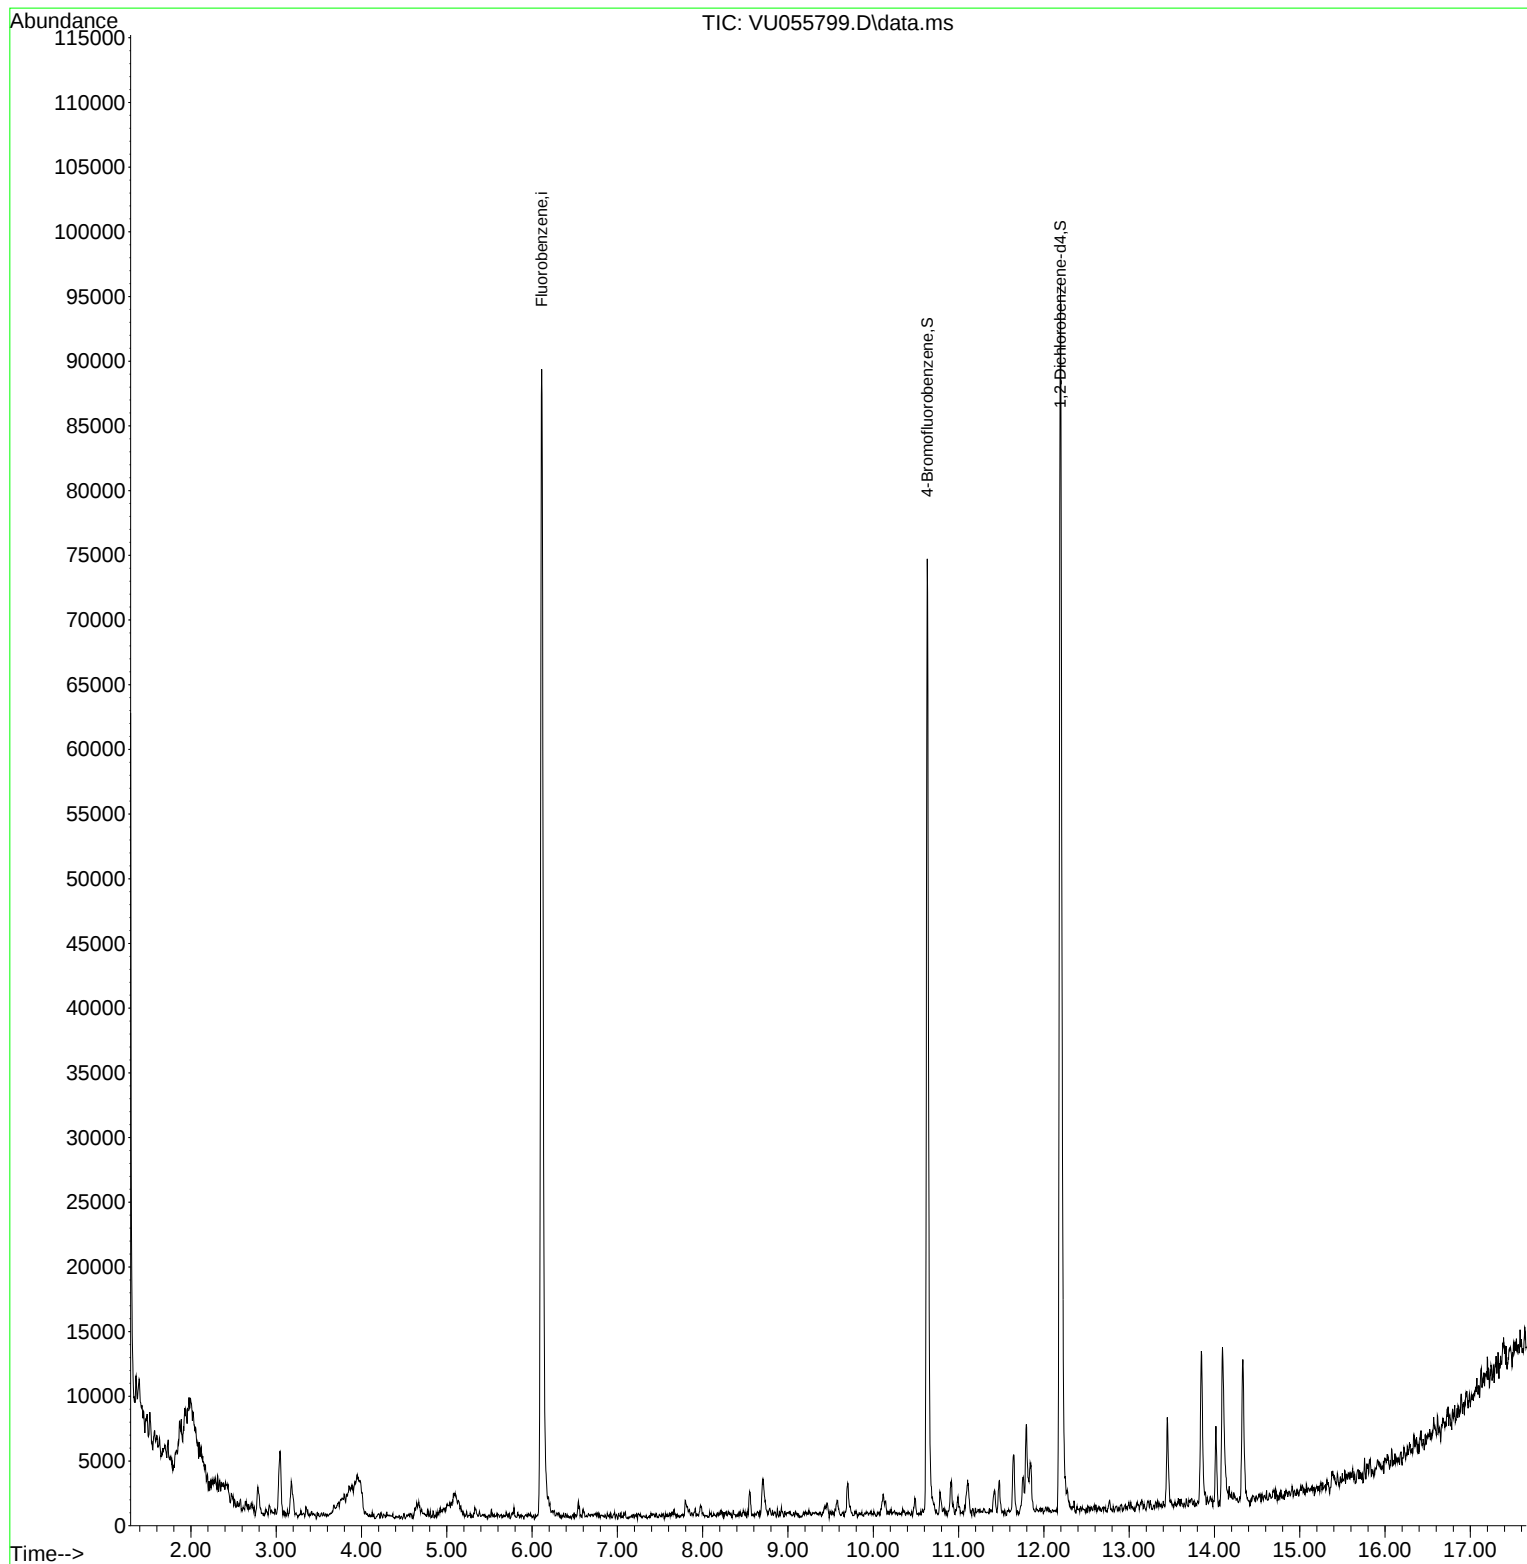


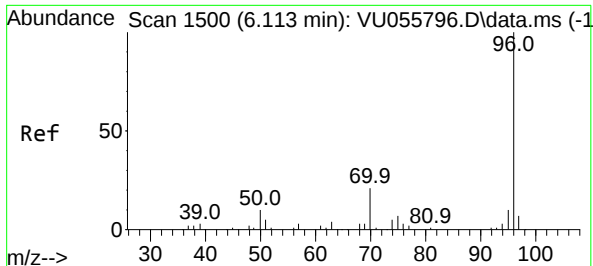

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 1
Delta R.T. -0.000 min
Lab File: VU055799.D
Acq: 18 Oct 2023 15:24




Instrument :
MSVOA_U
ClientSampleId :
VBLK12


Tgt Ion: 96	Resp: 87833
Ion Ratio	Lower Upper
96 100	
70 19.9	16.5 24.7
95 9.4	7.4 11.0
97 5.7	0.0 0.0

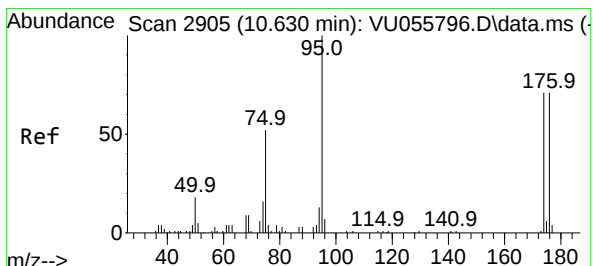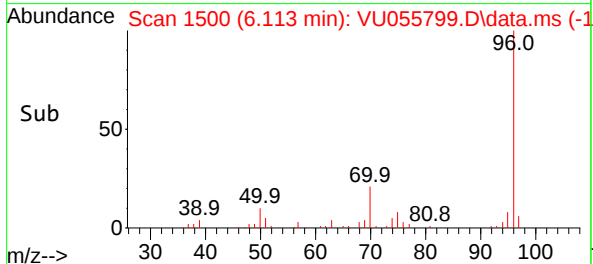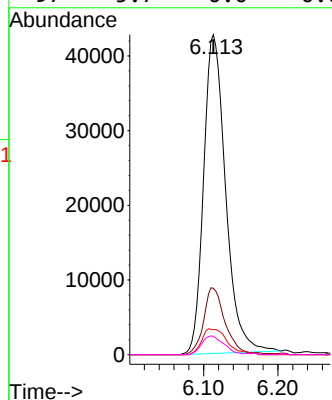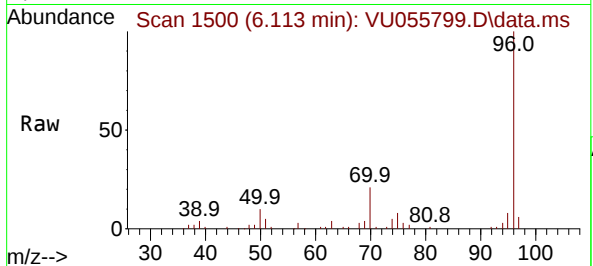

#57
4-Bromofluorobenzene
Concen: 0.861 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.004 min
Lab File: VU055799.D
Acq: 18 Oct 2023 15:24


Tgt Ion: 95	Resp: 29817
Ion Ratio	Lower Upper
95 100	
174 70.5	63.3 94.9
176 67.8	59.3 88.9

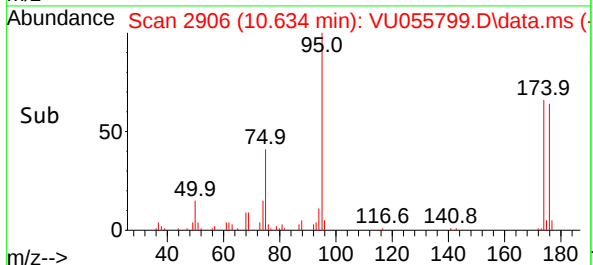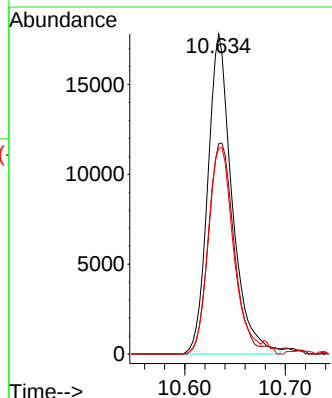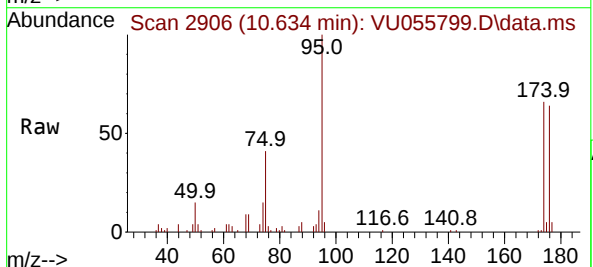

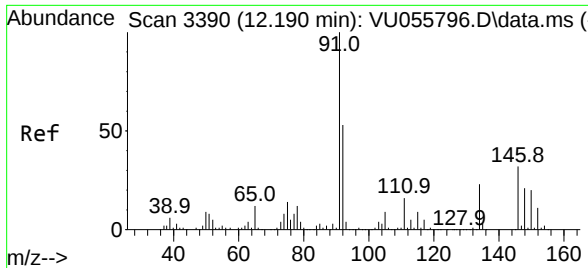

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.810 ug/l
 RT: 12.193 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU055799.D
 Acq: 18 Oct 2023 15:24

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK12

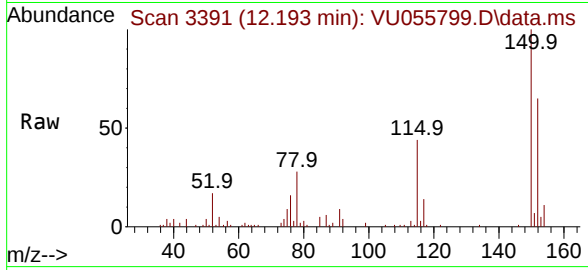

Tgt Ion:	152	Resp:	26003
Ion Ratio	Lower	Upper	
152	100		
115	70.8	0.0	308.8
150	157.6	0.0	635.0

