


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101823\
Data File : VU055791.D
Acq On : 18 Oct 2023 09:08
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101823DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Oct 19 03:10:04 2023

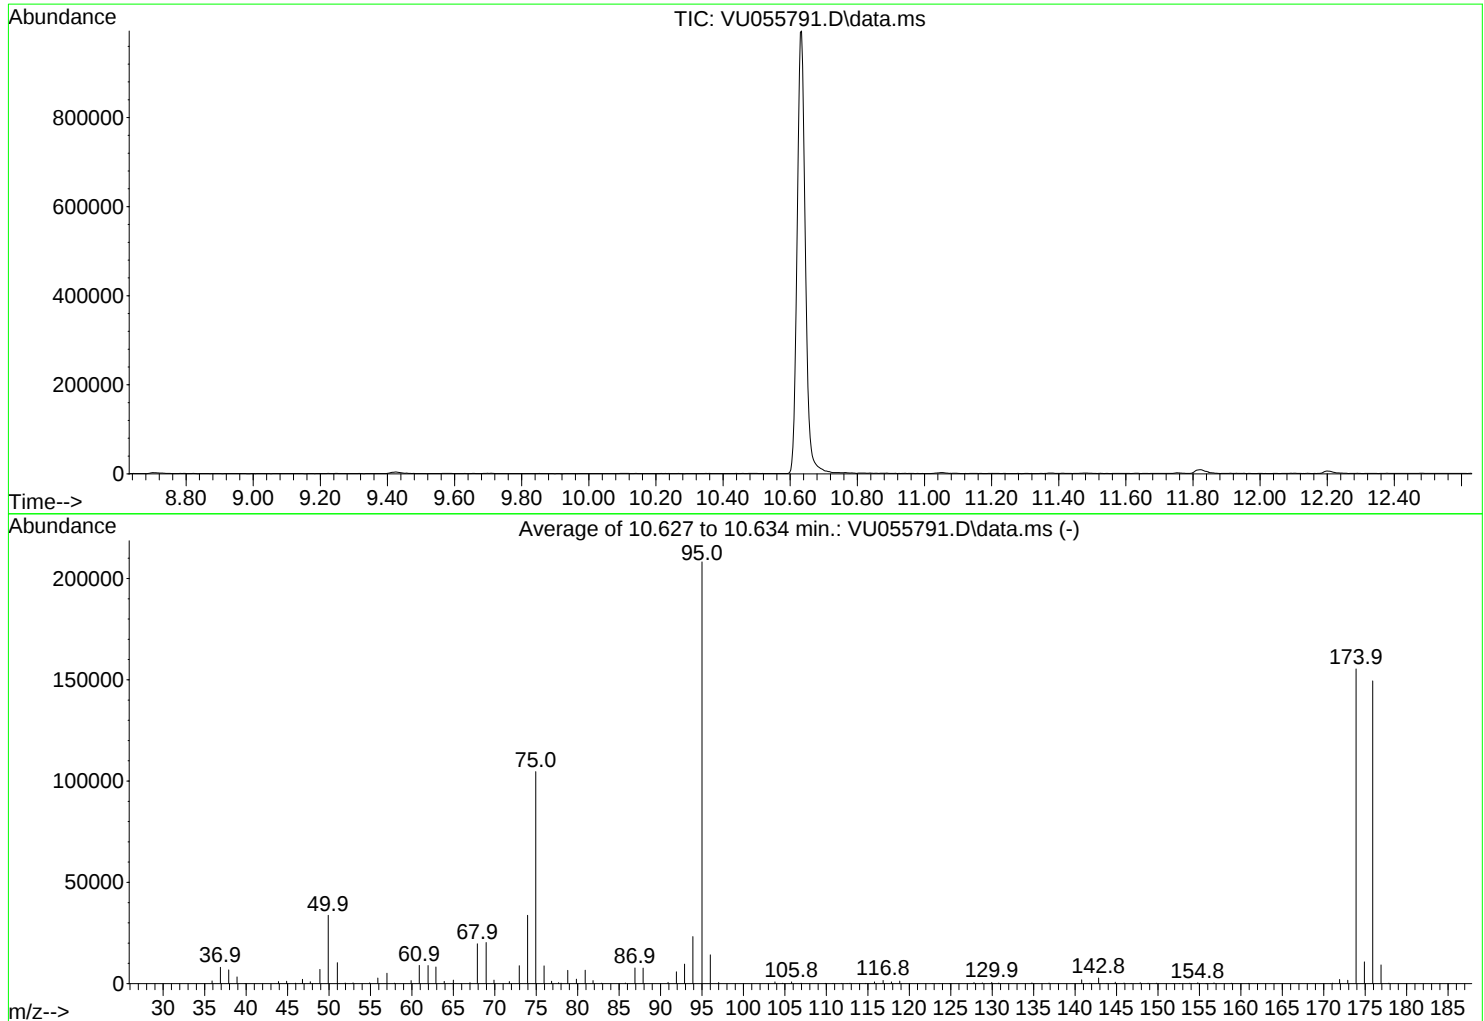

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	33723	PASS
75	95	30	60	50.3	104661	PASS
95	95	100	100	100.0	208235	PASS
96	95	5	9	6.8	14194	PASS
173	174	0.00	2	1.1	1644	PASS
174	95	50	100	74.6	155349	PASS
175	174	5	9	6.9	10772	PASS
176	174	95	101	96.2	149461	PASS
177	176	5	9	6.2	9284	PASS