

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101919\
 Data File : VU035304.D
 Acq On : 19 Oct 2019 08:45
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.617	78	86	99	rBV	417708	458085	16.42%	2.180%
2	1.935	176	185	202	rBV	326738	429990	15.41%	2.046%
3	2.597	379	391	408	rBV	598716	1004549	36.01%	4.781%
4	2.829	454	463	478	rVB	18034	31245	1.12%	0.149%
5	2.999	512	516	524	rVB6	1858	1911	0.07%	0.009%
6	3.089	532	544	557	rVB7	4199	9384	0.34%	0.045%
7	3.157	560	565	569	rBV5	775	826	0.03%	0.004%
8	3.237	577	590	606	rVB	26866	62805	2.25%	0.299%
9	3.327	615	618	621	rBV3	710	396	0.01%	0.002%
10	3.398	629	640	653	rBV2	8409	16814	0.60%	0.080%
11	3.472	658	663	666	rBV3	522	510	0.02%	0.002%
12	3.665	720	723	730	rVB3	557	469	0.02%	0.002%
13	3.694	730	732	740	rBV4	460	396	0.01%	0.002%
14	3.764	751	754	758	rVB3	499	394	0.01%	0.002%
15	3.787	758	761	764	rBV3	625	523	0.02%	0.002%
16	3.867	780	786	789	rVB4	550	583	0.02%	0.003%
17	3.925	793	804	810	rBV5	1340	2702	0.10%	0.013%
18	3.980	818	821	825	rBV3	539	349	0.01%	0.002%
19	4.054	838	844	846	rBV3	497	457	0.02%	0.002%
20	4.086	852	854	858	rVB3	549	366	0.01%	0.002%
21	4.112	859	862	865	rVB3	924	538	0.02%	0.003%
22	4.131	865	868	871	rBV3	434	370	0.01%	0.002%
23	4.343	931	934	936	rBV	533	384	0.01%	0.002%
24	4.382	942	946	949	rBV3	419	486	0.02%	0.002%
25	4.449	964	967	974	rBV4	553	549	0.02%	0.003%
26	4.642	1025	1027	1029	rBV2	536	340	0.01%	0.002%
27	4.700	1029	1045	1065	rBV	256112	635812	22.79%	3.026%
28	5.118	1157	1175	1204	rBV	487596	1090289	39.08%	5.189%
29	5.433	1262	1273	1289	rVB7	5262	12343	0.44%	0.059%
30	5.774	1357	1379	1418	rBV2	1049470	2789806	100.00%	13.278%
31	6.192	1507	1509	1511	rBV3	687	441	0.02%	0.002%
32	6.295	1525	1541	1572	rBV	806776	1552227	55.64%	7.388%
33	6.581	1623	1630	1641	rVB5	8646	16832	0.60%	0.080%
34	6.735	1662	1678	1697	rBV	636004	1261279	45.21%	6.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101919\
 Data File : VU035304.D
 Acq On : 19 Oct 2019 08:45
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
 Title : VOC Analysis

35	7.067	1777	1781	1784	rBV3	455	402	0.01%	0.002%
36	7.144	1799	1805	1814	rBV5	1911	3269	0.12%	0.016%
37	7.295	1849	1852	1856	rVB2	661	423	0.02%	0.002%
38	7.314	1856	1858	1862	rBV3	478	367	0.01%	0.002%
39	7.349	1862	1869	1873	rBV6	480	647	0.02%	0.003%
40	7.404	1883	1886	1895	rBV6	580	559	0.02%	0.003%
41	7.607	1935	1949	1975	rBV	371645	685574	24.57%	3.263%
42	7.845	2014	2023	2037	rBV3	22799	41001	1.47%	0.195%
43	7.935	2037	2051	2067	rBV	1280706	2251444	80.70%	10.715%
44	8.218	2126	2139	2173	rBV	246875	473899	16.99%	2.255%
45	8.439	2200	2208	2215	rBV4	4165	5957	0.21%	0.028%
46	8.584	2243	2253	2265	rBV4	9142	16232	0.58%	0.077%
47	8.684	2269	2284	2327	rBV	449549	1340173	48.04%	6.378%
48	8.960	2362	2370	2373	rBV4	2879	3900	0.14%	0.019%
49	9.111	2415	2417	2423	rVB4	693	538	0.02%	0.003%
50	9.144	2423	2427	2429	rBV2	462	361	0.01%	0.002%
51	9.195	2441	2443	2449	rVV3	838	918	0.03%	0.004%
52	9.234	2452	2455	2462	rVB5	494	476	0.02%	0.002%
53	9.301	2473	2476	2480	rBV3	664	448	0.02%	0.002%
54	9.327	2480	2484	2488	rBV2	570	528	0.02%	0.003%
55	9.394	2500	2505	2508	rBV3	475	401	0.01%	0.002%
56	9.449	2508	2522	2560	rVV	1042315	1907537	68.38%	9.079%
57	9.603	2560	2570	2583	rBV2	14411	24197	0.87%	0.115%
58	9.726	2598	2608	2618	rBV2	14289	23718	0.85%	0.113%
59	9.851	2644	2647	2651	rVB4	642	453	0.02%	0.002%
60	9.951	2672	2678	2681	rBV4	503	540	0.02%	0.003%
61	10.092	2718	2722	2724	rBV2	597	444	0.02%	0.002%
62	10.140	2724	2737	2755	rBV5	21798	49880	1.79%	0.237%
63	10.266	2772	2776	2780	rBV4	375	406	0.01%	0.002%
64	10.324	2785	2794	2803	rBV7	3699	6498	0.23%	0.031%
65	10.513	2844	2853	2866	rVV	19011	30053	1.08%	0.143%
66	10.616	2880	2885	2888	rBV3	496	446	0.02%	0.002%
67	10.668	2898	2901	2904	rVB3	930	512	0.02%	0.002%
68	10.787	2925	2938	2955	rBV	781736	1360878	48.78%	6.477%
69	11.118	3030	3041	3054	rBV2	21202	36441	1.31%	0.173%
70	11.195	3062	3065	3069	rBV3	518	406	0.01%	0.002%
71	11.214	3069	3071	3076	rVB4	538	342	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101919\
 Data File : VU035304.D
 Acq On : 19 Oct 2019 08:45
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
 Title : VOC Analysis

72	11.285	3091	3093	3096	rBV3	548	354	0.01%	0.002%
73	11.324	3100	3105	3106	rBV	511	351	0.01%	0.002%
74	11.446	3139	3143	3148	rVB3	1346	1098	0.04%	0.005%
75	11.497	3148	3159	3173	rBV	24262	42753	1.53%	0.203%
76	11.578	3179	3184	3188	rBV4	365	423	0.02%	0.002%
77	11.626	3194	3199	3201	rBV	492	393	0.01%	0.002%
78	11.703	3218	3223	3224	rBV2	469	385	0.01%	0.002%
79	11.777	3236	3246	3255	rVV3	26338	47615	1.71%	0.227%
80	11.844	3255	3267	3289	rVB	726704	1316904	47.20%	6.268%
81	11.973	3303	3307	3311	rBV3	993	802	0.03%	0.004%
82	12.063	3332	3335	3339	rVB3	649	493	0.02%	0.002%
83	12.086	3339	3342	3345	rBV3	611	423	0.02%	0.002%
84	12.160	3363	3365	3368	rVB2	629	350	0.01%	0.002%
85	12.224	3368	3385	3404	rBV	911142	1566593	56.15%	7.456%
86	12.488	3461	3467	3470	rBV3	679	733	0.03%	0.003%
87	12.555	3484	3488	3493	rVB3	662	574	0.02%	0.003%
88	12.655	3516	3519	3522	rBV	644	348	0.01%	0.002%
89	12.774	3553	3556	3559	rBV3	647	443	0.02%	0.002%
90	12.825	3569	3572	3574	rBV	638	345	0.01%	0.002%
91	12.864	3581	3584	3587	rVB2	783	440	0.02%	0.002%
92	13.028	3622	3635	3643	rBV4	11552	19350	0.69%	0.092%
93	13.098	3655	3657	3662	rVB2	668	433	0.02%	0.002%
94	13.246	3692	3703	3716	rBV2	40887	65168	2.34%	0.310%
95	13.468	3769	3772	3776	rBV3	862	734	0.03%	0.003%
96	13.661	3828	3832	3835	rVB3	815	714	0.03%	0.003%
97	13.867	3886	3896	3906	rVB2	50121	76791	2.75%	0.365%
98	13.928	3913	3915	3919	rBV2	683	403	0.01%	0.002%
99	14.111	3962	3972	3987	rVB	68179	107516	3.85%	0.512%
100	14.356	4037	4048	4061	rVB	65279	103474	3.71%	0.492%


Sum of corrected areas: 21011121

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101919\
Data File : VU035304.D
Acq On : 19 Oct 2019 08:45
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

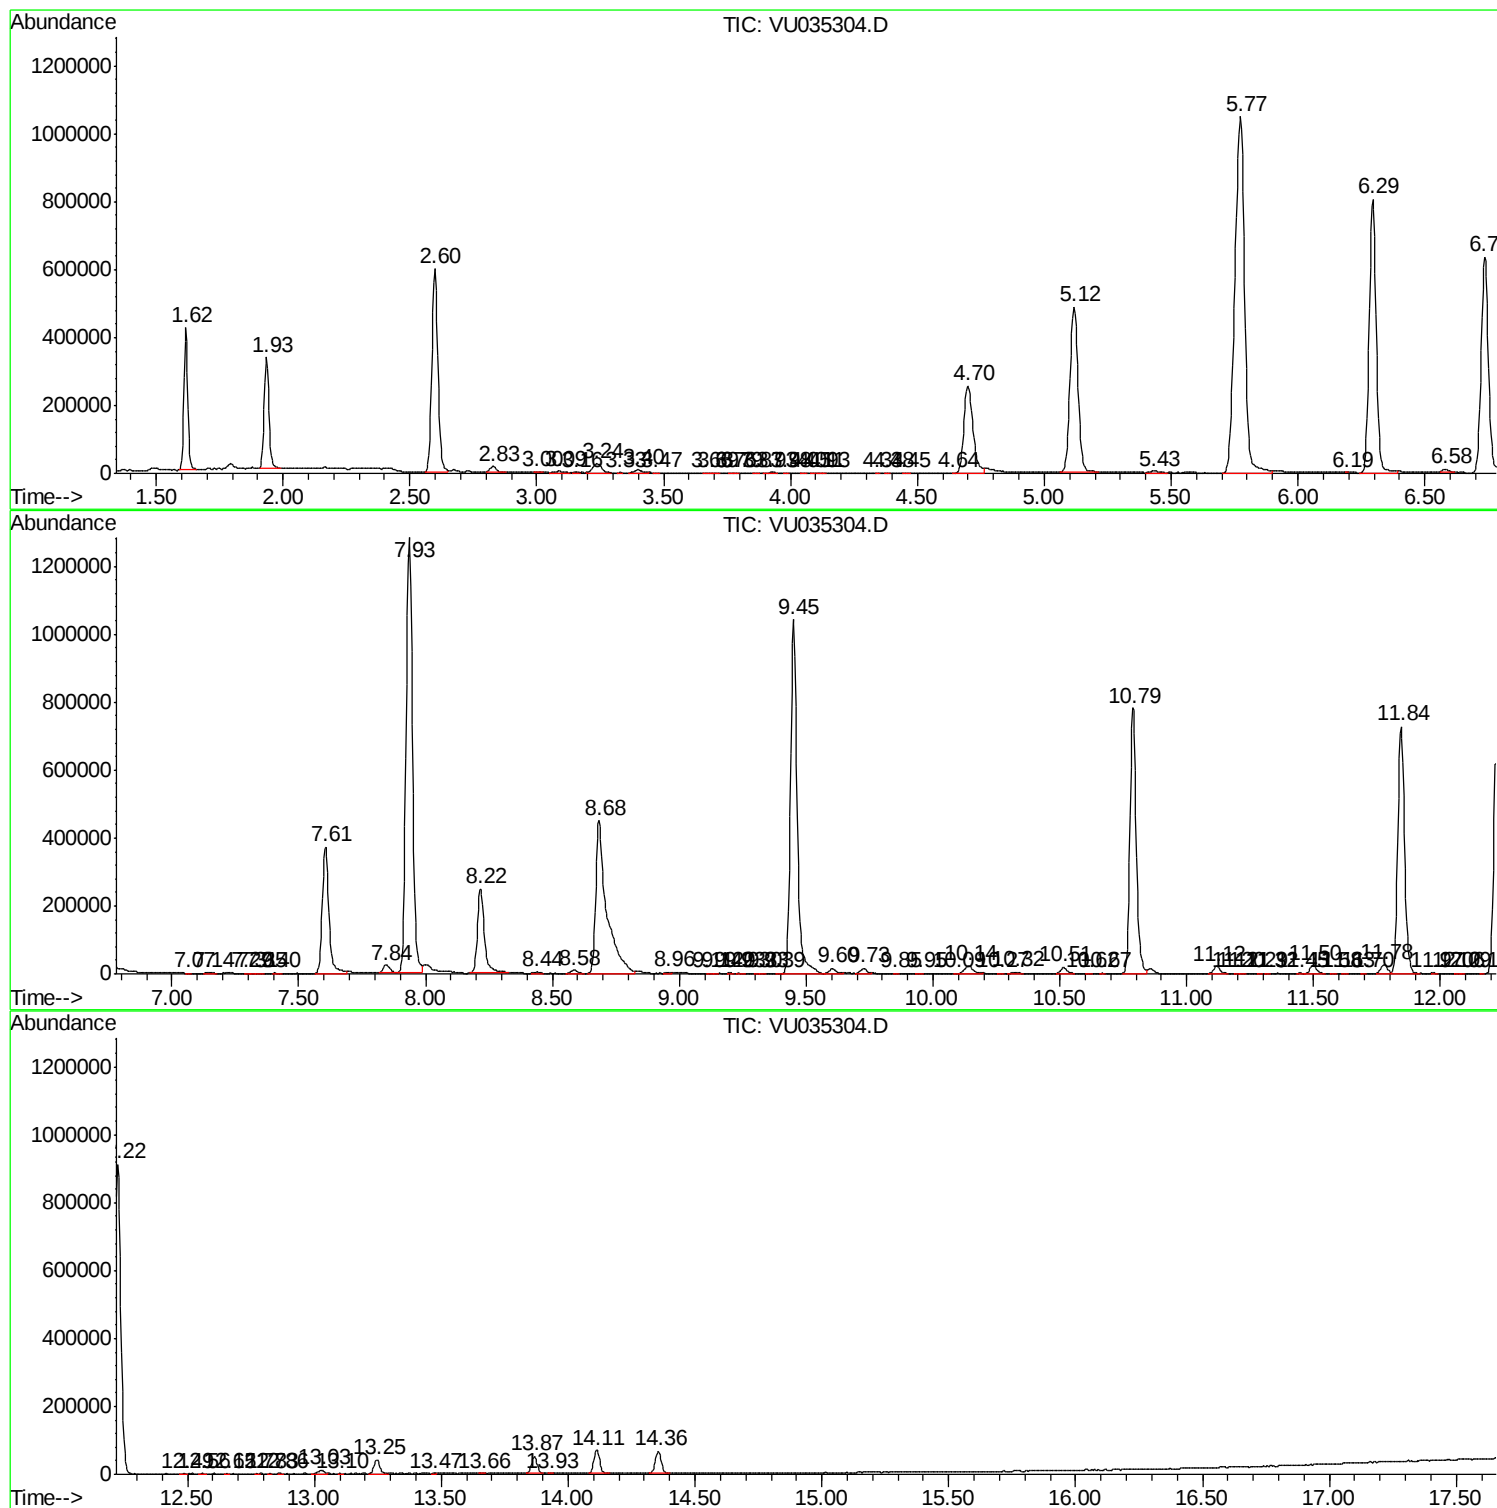

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101919\
Data File : VU035304.D
Acq On : 19 Oct 2019 08:45
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101919\
Data File : VU035304.D
Acq On : 19 Oct 2019 08:45
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc