

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101919\
 Data File : VU035316.D
 Acq On : 19 Oct 2019 14:14
 Operator : JC/SP
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.616	78	86	99	rBV	474335	512332	16.60%	2.126%
2	1.932	176	184	202	rVB	365996	483431	15.66%	2.006%
3	2.594	378	390	409	rBV	684976	1123411	36.39%	4.661%
4	2.960	501	504	507	rBV2	715	394	0.01%	0.002%
5	3.076	535	540	541	rBV3	2714	1860	0.06%	0.008%
6	3.237	576	590	607	rVB	26851	63526	2.06%	0.264%
7	3.298	607	609	613	rVB2	792	484	0.02%	0.002%
8	3.350	621	625	629	rVB3	389	320	0.01%	0.001%
9	3.459	656	659	664	rBV4	594	569	0.02%	0.002%
10	3.494	666	670	674	rVB4	738	725	0.02%	0.003%
11	3.697	731	733	737	rBV	513	332	0.01%	0.001%
12	3.829	769	774	779	rBV3	328	338	0.01%	0.001%
13	3.893	789	794	801	rBV3	696	833	0.03%	0.003%
14	3.970	816	818	823	rVB4	510	448	0.01%	0.002%
15	4.005	825	829	834	rBV4	455	407	0.01%	0.002%
16	4.070	842	849	854	rBV4	973	1268	0.04%	0.005%
17	4.095	854	857	862	rVB4	359	304	0.01%	0.001%
18	4.128	862	867	868	rBV	472	360	0.01%	0.001%
19	4.231	894	899	903	rBV3	730	625	0.02%	0.003%
20	4.314	923	925	929	rBV2	497	320	0.01%	0.001%
21	4.337	929	932	938	rVB3	531	572	0.02%	0.002%
22	4.584	1004	1009	1014	rVB3	716	560	0.02%	0.002%
23	4.697	1027	1044	1071	rBV	311340	757140	24.53%	3.141%
24	5.115	1157	1174	1196	rBV	550836	1205227	39.04%	5.001%
25	5.401	1259	1263	1266	rBV2	1000	1005	0.03%	0.004%
26	5.478	1285	1287	1291	rVB2	642	352	0.01%	0.001%
27	5.533	1299	1304	1308	rBV5	548	447	0.01%	0.002%
28	5.575	1313	1317	1318	rBV4	499	402	0.01%	0.002%
29	5.626	1331	1333	1336	rBV2	733	475	0.02%	0.002%
30	5.658	1338	1343	1348	rBV5	397	432	0.01%	0.002%
31	5.684	1348	1351	1355	rVB4	569	433	0.01%	0.002%
32	5.771	1355	1378	1406	rBV2	1175327	3087060	100.00%	12.809%
33	6.292	1526	1540	1577	rBV	1053209	2011969	65.17%	8.348%
34	6.735	1661	1678	1706	rBV	708617	1402854	45.44%	5.821%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101919\
 Data File : VU035316.D
 Acq On : 19 Oct 2019 14:14
 Operator : JC/SP
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
 Title : VOC Analysis

35	6.967	1748	1750	1754	rVB2	828	519	0.02%	0.002%
36	7.224	1828	1830	1833	rVV3	1037	597	0.02%	0.002%
37	7.282	1846	1848	1851	rBV3	641	376	0.01%	0.002%
38	7.414	1886	1889	1893	rBV4	554	498	0.02%	0.002%
39	7.536	1923	1927	1930	rVV3	809	762	0.02%	0.003%
40	7.603	1935	1948	1966	rBV	409372	740382	23.98%	3.072%
41	7.845	2013	2023	2037	rBV2	26162	46423	1.50%	0.193%
42	7.935	2038	2051	2067	rBV	1480460	2556443	82.81%	10.607%
43	8.218	2126	2139	2156	rBV	290463	513702	16.64%	2.131%
44	8.459	2209	2214	2217	rBV3	1505	1311	0.04%	0.005%
45	8.494	2222	2225	2228	rBV	936	569	0.02%	0.002%
46	8.536	2235	2238	2241	rVB3	811	488	0.02%	0.002%
47	8.565	2241	2247	2251	rBV	2468	2125	0.07%	0.009%
48	8.584	2251	2253	2261	rVB5	1409	1438	0.05%	0.006%
49	8.632	2265	2268	2270	rBV3	747	408	0.01%	0.002%
50	8.681	2270	2283	2329	rBV	687471	1577460	51.10%	6.545%
51	8.931	2359	2361	2363	rVB2	850	391	0.01%	0.002%
52	9.012	2384	2386	2390	rBV3	629	431	0.01%	0.002%
53	9.079	2404	2407	2409	rBV2	543	324	0.01%	0.001%
54	9.189	2438	2441	2446	rVB6	738	617	0.02%	0.003%
55	9.353	2488	2492	2494	rBV4	574	495	0.02%	0.002%
56	9.381	2498	2501	2505	rVB3	449	335	0.01%	0.001%
57	9.449	2508	2522	2560	rVV	1402564	2457864	79.62%	10.198%
58	9.603	2562	2570	2574	rBV4	2481	3043	0.10%	0.013%
59	9.725	2598	2608	2615	rBV2	5409	8909	0.29%	0.037%
60	9.771	2620	2622	2625	rVB2	1013	567	0.02%	0.002%
61	9.915	2664	2667	2669	rBV3	566	373	0.01%	0.002%
62	9.954	2676	2679	2684	rBV4	749	788	0.03%	0.003%
63	9.999	2689	2693	2701	rVB5	492	474	0.02%	0.002%
64	10.044	2704	2707	2714	rVB5	755	805	0.03%	0.003%
65	10.073	2714	2716	2722	rBV3	630	471	0.02%	0.002%
66	10.137	2725	2736	2744	rBV5	4093	7343	0.24%	0.030%
67	10.172	2744	2747	2750	rBV4	611	452	0.01%	0.002%
68	10.262	2769	2775	2776	rBV3	1091	939	0.03%	0.004%
69	10.275	2776	2779	2785	rVB5	1234	1358	0.04%	0.006%
70	10.388	2806	2814	2819	rBV9	1129	1867	0.06%	0.008%
71	10.600	2877	2880	2884	rBV5	797	682	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101919\
 Data File : VU035316.D
 Acq On : 19 Oct 2019 14:14
 Operator : JC/SP
 Sample : VIBLK41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
 Title : VOC Analysis

72	10.671	2900	2902	2905	rBV2	841	647	0.02%	0.003%
73	10.787	2923	2938	2962	rBV	899294	1531027	49.59%	6.352%
74	10.877	2962	2966	2970	rVB4	693	522	0.02%	0.002%
75	11.024	3005	3012	3016	rBV5	3244	4272	0.14%	0.018%
76	11.140	3036	3048	3063	rVB9	6259	13180	0.43%	0.055%
77	11.266	3083	3087	3089	rBV2	1079	1038	0.03%	0.004%
78	11.330	3096	3107	3110	rBV5	1996	2739	0.09%	0.011%
79	11.439	3138	3141	3147	rVB7	2719	2794	0.09%	0.012%
80	11.497	3150	3159	3168	rBV2	6919	11057	0.36%	0.046%
81	11.584	3183	3186	3187	rBV	721	423	0.01%	0.002%
82	11.616	3187	3196	3204	rVV5	3492	6302	0.20%	0.026%
83	11.680	3208	3216	3219	rBV8	1603	2306	0.07%	0.010%
84	11.841	3253	3266	3282	rBV	1120122	1943767	62.96%	8.065%
85	12.092	3337	3344	3350	rBV6	4564	7557	0.24%	0.031%
86	12.224	3371	3385	3402	rVB	1125575	1921121	62.23%	7.971%
87	12.349	3417	3424	3434	rVB6	6656	10363	0.34%	0.043%
88	12.481	3461	3465	3466	rBV2	1726	1047	0.03%	0.004%
89	12.549	3484	3486	3489	rVB3	883	379	0.01%	0.002%
90	12.684	3526	3528	3532	rVB3	712	443	0.01%	0.002%
91	12.819	3568	3570	3573	rBV3	656	492	0.02%	0.002%
92	12.838	3573	3576	3579	rBV4	1163	966	0.03%	0.004%
93	12.944	3603	3609	3610	rBV5	1094	1125	0.04%	0.005%
94	13.053	3637	3643	3647	rBV4	3013	3717	0.12%	0.015%
95	13.102	3656	3658	3661	rBV4	726	413	0.01%	0.002%
96	13.455	3760	3768	3771	rBV6	4017	6039	0.20%	0.025%
97	13.642	3823	3826	3827	rBV3	1317	770	0.02%	0.003%
98	13.741	3855	3857	3859	rBV2	841	444	0.01%	0.002%
99	13.767	3859	3865	3867	rBV5	2304	2680	0.09%	0.011%
100	14.114	3964	3973	3983	rVB	19557	30771	1.00%	0.128%


Sum of corrected areas: 24101645

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101919\
Data File : VU035316.D
Acq On : 19 Oct 2019 14:14
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

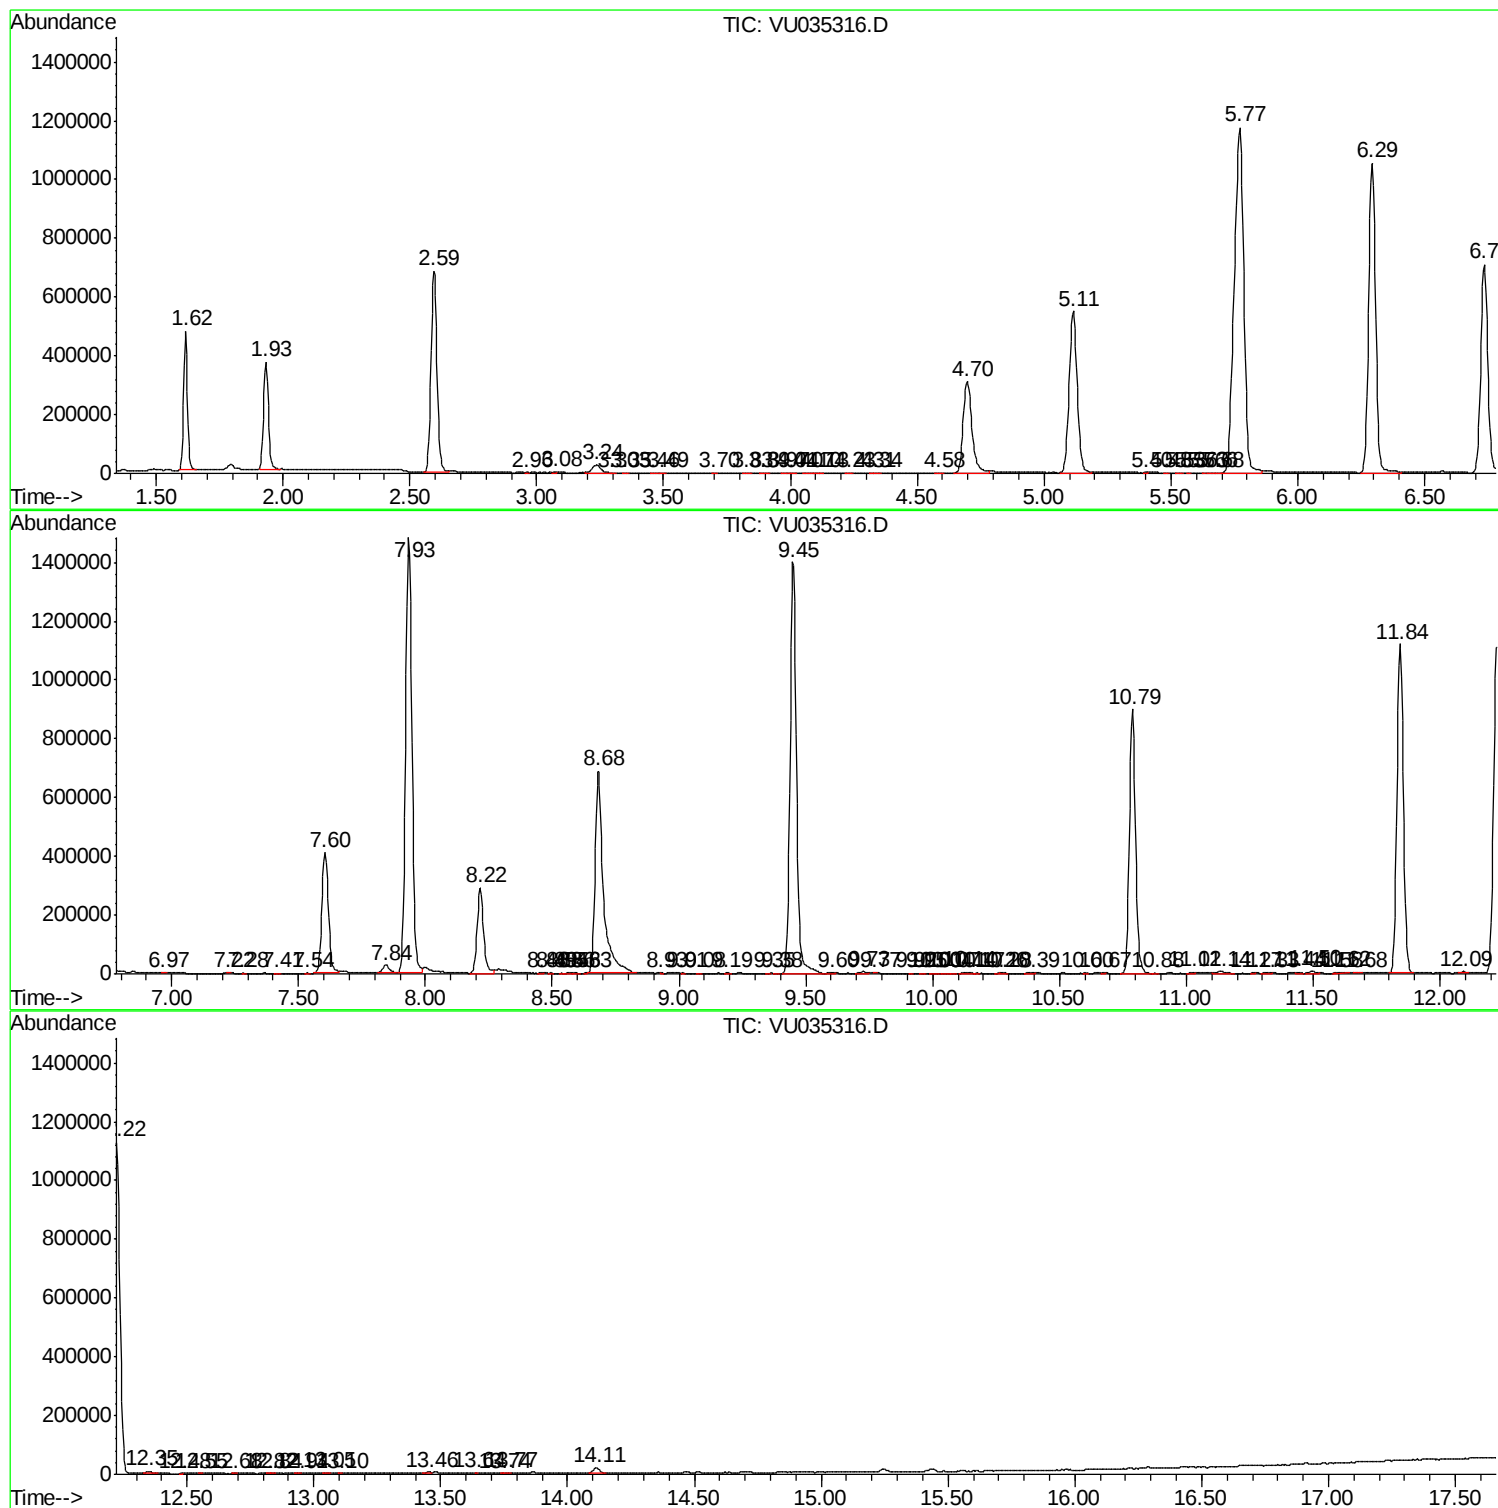

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101919\
Data File : VU035316.D
Acq On : 19 Oct 2019 14:14
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU101919\
Data File : VU035316.D
Acq On : 19 Oct 2019 14:14
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc