


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101919\
Data File : VU035298.D
Acq On : 19 Oct 2019 06:24
Operator : JC/SP
Sample : BFB44
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
Title : VOC Analysis
Last Update : Mon Oct 21 05:38:49 2019

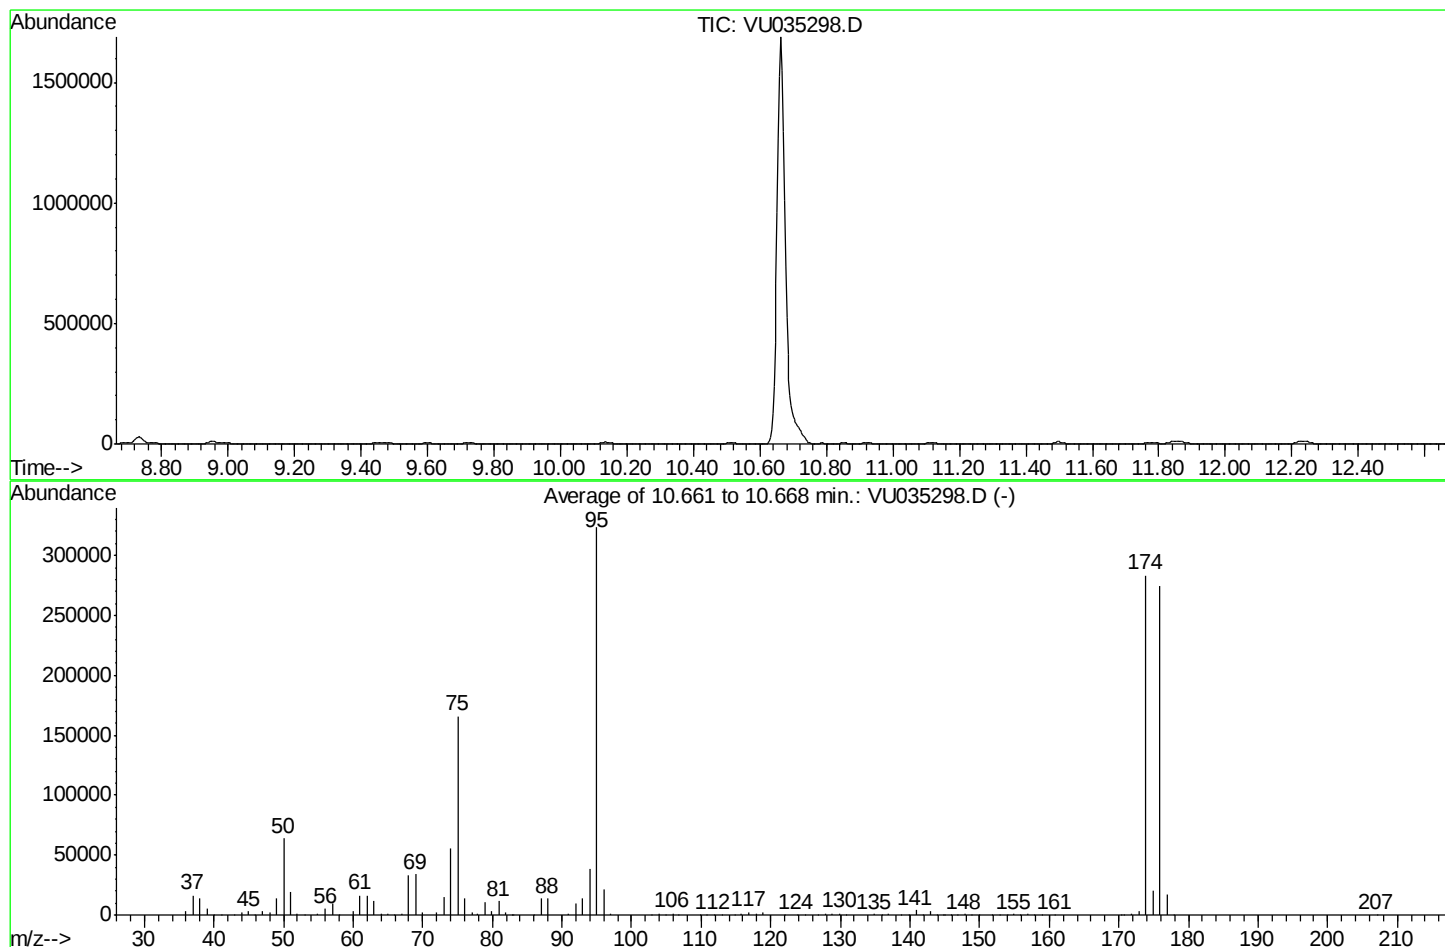

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	63824	PASS
75	95	30	80	51.2	165781	PASS
95	95	100	100	100.0	323541	PASS
96	95	5	9	6.5	21114	PASS
173	174	0.00	2	1.0	2815	PASS
174	95	50	120	87.6	283370	PASS
175	174	5	9	7.2	20528	PASS
176	174	95	101	96.8	274368	PASS
177	176	5	9	6.1	16771	PASS

m/z	Abundance
36.00	2828.0
37.00	16992.0
38.00	14803.0
39.00	5882.0
40.00	417.0
43.00	189.0
44.00	2972.0
45.00	3440.0
45.90	304.0
47.00	4035.0
48.00	2166.0
49.00	14357.0
50.00	66144.0
51.00	20488.0
52.00	963.0
53.00	182.0
54.90	901.0
56.00	5542.0
57.00	9887.0
58.00	424.0
60.00	3315.0
61.00	17392.0
62.00	16648.0
63.00	13217.0
64.00	1247.0
65.00	881.0
67.00	823.0
68.00	35136.0
69.00	35456.0
70.00	2767.0
71.90	1846.0
73.00	15447.0
74.00	57872.0
75.00	172608.0
76.00	14794.0
77.10	2249.0
77.90	1256.0
78.90	11381.0
79.90	3129.0
80.90	11953.0
81.90	2783.0
82.80	212.0
85.80	473.0
87.00	13981.0
87.90	14356.0
91.00	1216.0
92.00	10418.0
93.00	14277.0
94.00	39376.0
95.00	331520.0
96.00	22272.0
97.00	746.0
102.90	165.0
103.90	1544.0
104.80	517.0
105.90	1554.0
106.80	295.0
109.80	192.0
110.80	262.0
111.80	316.0
112.90	297.0
114.80	395.0
115.80	1385.0
116.90	2220.0
117.80	1388.0
118.90	1749.0
123.80	130.0
124.80	107.0
127.80	1245.0
128.90	655.0
129.90	1383.0
130.80	516.0
134.90	715.0
136.80	535.0
139.80	265.0
140.90	3962.0
141.90	533.0
143.00	3543.0
144.00	167.0
144.80	391.0
145.80	497.0
146.80	251.0
147.80	838.0
148.80	213.0
150.00	346.0
151.80	128.0
152.80	204.0
154.00	223.0
154.90	856.0
155.80	136.0
156.90	735.0
157.90	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

158.80	285.0
160.90	471.0
170.40	162.0
170.80	184.0
171.90	1428.0
173.00	2805.0
173.90	283712.0
174.90	21008.0
175.90	276096.0
176.90	17144.0
177.90	611.0
207.00	188.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	2857.0
37.00	16824.0
38.00	14642.0
39.00	5918.0
40.00	461.0
41.00	109.0
43.00	247.0
44.00	2999.0
45.00	3169.0
45.90	337.0
47.00	3947.0
48.00	2164.0
49.00	14107.0
50.00	65536.0
51.00	20280.0
52.00	972.0
53.00	143.0
54.90	924.0
56.00	5423.0
57.00	9910.0
58.00	463.0
60.00	3199.0
61.00	16720.0
62.00	16504.0
63.00	12434.0
64.00	1265.0
65.00	821.0
65.90	107.0
67.00	823.0
68.00	34320.0
69.00	34888.0
70.00	2705.0
71.90	1896.0
73.00	15203.0
74.00	57384.0
75.00	170432.0
76.00	13990.0
77.00	2247.0
77.90	1176.0
78.90	11170.0
80.00	3005.0
80.90	11734.0
81.90	2772.0
83.00	233.0
85.90	425.0
87.00	14098.0
87.90	14278.0
90.90	1269.0
92.00	10278.0
93.00	14225.0
94.00	39688.0
95.00	333376.0
96.00	21760.0
97.00	663.0
102.90	152.0
103.90	1584.0
104.80	564.0
105.90	1596.0
106.80	289.0
109.80	243.0
110.80	244.0
111.80	291.0
112.90	343.0
114.90	426.0
115.80	1356.0
116.90	2357.0
117.80	1310.0
118.80	1800.0
123.80	111.0
124.90	127.0
127.80	1242.0
128.80	665.0
129.90	1370.0
130.80	472.0
134.90	645.0
136.80	562.0
139.70	290.0
140.90	3980.0
141.90	485.0
142.90	3584.0
143.90	166.0
144.80	373.0
145.80	462.0
146.80	221.0
147.90	900.0
148.80	221.0
150.00	358.0
151.80	156.0
152.80	221.0
153.90	233.0
154.90	868.0
155.90	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

156.90	769.0
157.90	198.0
158.90	377.0
160.80	429.0
170.70	199.0
171.90	1327.0
173.00	2877.0
173.90	292544.0
175.00	21144.0
175.90	283520.0
176.90	17200.0
177.90	575.0
207.10	174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	2806.0
37.00	15137.0
38.00	13369.0
39.00	5230.0
40.00	452.0
41.00	122.0
43.00	241.0
44.00	2860.0
45.00	2655.0
45.90	298.0
47.00	3337.0
48.00	1957.0
49.00	12612.0
50.00	59792.0
51.00	18496.0
52.00	822.0
53.00	115.0
55.00	857.0
56.00	4725.0
57.00	8736.0
58.00	375.0
60.00	2873.0
61.00	15077.0
62.00	15071.0
63.00	10619.0
64.00	1219.0
65.00	792.0
67.00	789.0
68.00	30816.0
69.00	31480.0
70.00	2355.0
71.90	1736.0
73.00	13563.0
74.00	52368.0
75.00	154304.0
76.00	12176.0
77.00	2065.0
77.90	1086.0
78.90	9909.0
80.00	2577.0
80.90	10803.0
81.90	2538.0
83.00	236.0
85.90	332.0
87.00	13037.0
87.90	12859.0
90.80	1311.0
92.00	8954.0
93.00	13204.0
94.00	36376.0
95.00	305728.0
96.00	19312.0
97.00	553.0
102.90	160.0
103.90	1428.0
104.90	492.0
105.90	1456.0
106.80	277.0
109.80	236.0
110.80	222.0
111.90	253.0
112.90	346.0
114.90	442.0
115.80	1184.0
116.90	2321.0
117.90	1145.0
118.80	1682.0
121.90	102.0
123.80	104.0
124.90	100.0
126.70	111.0
127.80	1069.0
128.80	618.0
129.90	1192.0
130.80	383.0
134.90	510.0
135.90	109.0
136.90	649.0
138.80	122.0
139.80	269.0
140.90	3527.0
141.90	393.0
142.90	3289.0
143.90	163.0
145.00	335.0
145.80	373.0
146.80	183.0
147.80	902.0
148.80	201.0
149.90	301.0
151.80	168.0
152.80	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

153.90	208.0
154.90	866.0
155.90	157.0
156.90	643.0
157.90	188.0
158.90	407.0
160.80	364.0
170.70	178.0
171.90	1142.0
173.00	2765.0
173.90	273856.0
174.90	19432.0
175.90	263488.0
176.90	15969.0
177.90	495.0
207.10	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

Scan 2885 (10.616 min): VU035298.D
BFB44

m/z	Abundance
39.80	189.0
43.00	116.0
44.00	836.0
73.00	117.0
207.10	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44