
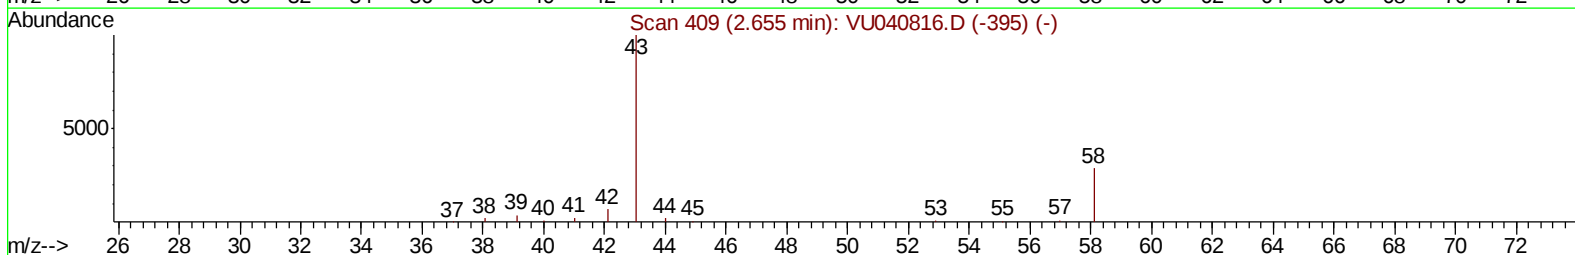
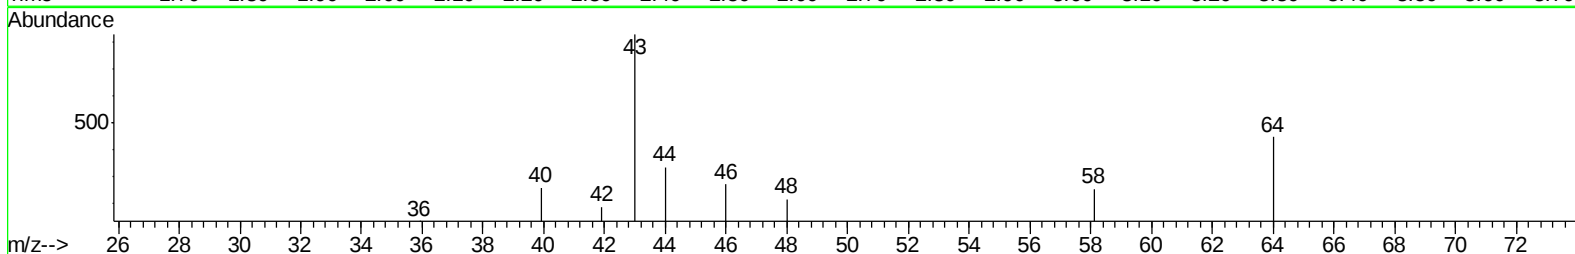


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101920\
Data File : VU040832.D
Acq On : 20 Oct 2020 02:33
Operator : SY/MD
Sample : L4428-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Oct 20 05:21:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 20 05:12:18 2020
Response via : Initial Calibration

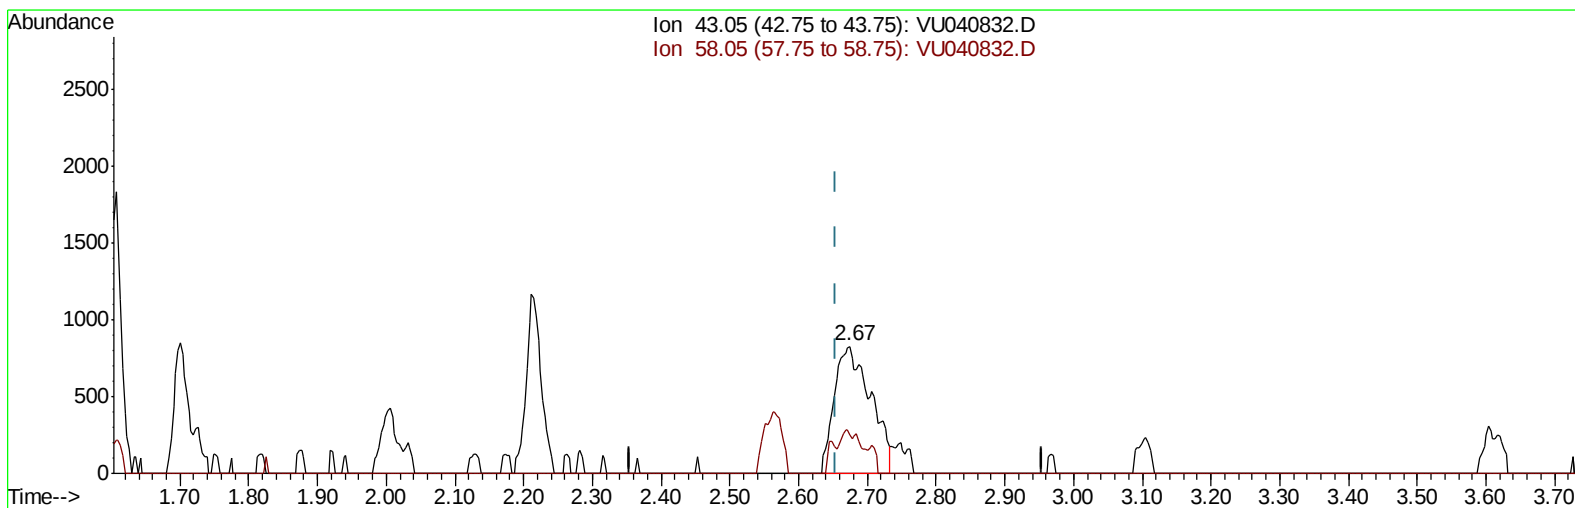

TIC: VU040832.D

(13) Acetone (T)

2.674min (+0.019) 1.36ug/L m

response 3037

Ion	Exp%	Act%
43.05	100	100
58.05	30.30	4.87
0.00	0.00	0.00
0.00	0.00	0.00