

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U101920\  
 Data File : VU040826.D  
 Acq On : 20 Oct 2020 00:14  
 Operator : SY/MD  
 Sample : L4420-11  
 Misc : 25.0mL/MSVOA U/WATER  
 ALS Vial : 39 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 C0AK4

Quant Time: Oct 20 05:20:42 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Tue Oct 20 05:12:18 2020  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Difluorobenzene     | 6.26  | 114  | 115012   | 5.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 9.42  | 117  | 121077   | 5.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 11.81 | 152  | 47649    | 5.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                                |        |       |          |          |      |         |
|--------------------------------|--------|-------|----------|----------|------|---------|
| 4) Vinyl Chloride-d3           | 1.60   | 65    | 27276    | 2.86     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 40 - 130 | Recovery | =    | 57.20%  |
| 7) Chloroethane-d5             | 1.92   | 69    | 28100    | 3.82     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 130 | Recovery | =    | 76.40%  |
| 11) 1,1-Dichloroethene-d2      | 2.59   | 63    | 89400    | 4.80     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 125 | Recovery | =    | 96.00%  |
| 20) 2-Butanone-d5              | 4.66   | 46    | 174446   | 57.20    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 40 - 130 | Recovery | =    | 114.40% |
| 24) Chloroform-d               | 5.08   | 84    | 79261    | 4.74     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 94.80%  |
| 26) 1,2-Dichloroethane-d4      | 5.72   | 65    | 50696    | 4.98     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 99.60%  |
| 32) Benzene-d6                 | 5.74   | 84    | 132527   | 4.06     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 81.20%  |
| 36) 1,2-Dichloropropane-d6     | 6.70   | 67    | 50466    | 4.66     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 140 | Recovery | =    | 93.20%  |
| 41) Toluene-d8                 | 7.91   | 98    | 97750    | 3.34     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 66.80%# |
| 43) trans-1,3-Dichloropropene- | 8.19   | 79    | 17949    | 3.91     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 55 - 130 | Recovery | =    | 78.20%  |
| 46) 2-Hexanone-d5              | 8.64   | 63    | 118958   | 50.26    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 45 - 130 | Recovery | =    | 100.52% |
| 57) 1,1,2,2-Tetrachloroethane- | 10.75  | 84    | 47989    | 4.93     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 120 | Recovery | =    | 98.60%  |
| 64) 1,2-Dichlorobenzene-d4     | 12.19  | 152   | 44946    | 5.09     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 80 - 120 | Recovery | =    | 101.80% |

## Target Compounds

|                                |      |     |        |              | Ovalue |
|--------------------------------|------|-----|--------|--------------|--------|
| 3) Chloromethane               | 1.53 | 50  | 1303   | 0.134 ug/L # | 73     |
| 5) Vinyl chloride              | 1.61 | 62  | 2912   | 0.284 ug/L # | 1      |
| 10) 1,1,2-Trichloro-1,2,2-trif | 2.59 | 101 | 519    | 0.054 ug/L # | 20     |
| 12) 1,1-Dichloroethene         | 2.59 | 96  | 76556  | 9.329 ug/L # | 85     |
| 14) Carbon disulfide           | 2.81 | 76  | 2810   | 0.122 ug/L # | 94     |
| 15) Methyl Acetate             | 2.96 | 43  | 710    | 0.132 ug/L # | 56     |
| 17) Methyl tert-butyl Ether    | 3.39 | 73  | 4163   | 0.179 ug/L   | 97     |
| 18) trans-1,2-Dichloroethene   | 3.37 | 96  | 5371   | 0.625 ug/L   | 99     |
| 19) 1,1-Dichloroethane         | 3.89 | 63  | 17762  | 1.000 ug/L   | 97     |
| 22) cis-1,2-Dichloroethene     | 4.69 | 96  | 129282 | 13.956 ug/L  | 95     |
| 25) Chloroform                 | 5.10 | 83  | 2572   | 0.142 ug/L   | 87     |
| 27) 1,2-Dichloroethane         | 5.82 | 62  | 877    | 0.068 ug/L # | 77     |
| 29) 1,1,1-Trichloroethane      | 5.33 | 97  | 5211   | 0.320 ug/L   | 98     |
| 34) Trichloroethene            | 6.56 | 95  | 153699 | 15.243 ug/L  | 98     |
| 35) Methylcyclohexane          | 6.70 | 83  | 11853  | 0.829 ug/L # | 14     |
| 37) 1,2-Dichloropropane        | 6.70 | 63  | 5737   | 0.529 ug/L # | 87     |
| 39) cis-1,3-Dichloropropene    | 7.57 | 75  | 1260   | 0.085 ug/L # | 36     |

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU101920\  
Data File : VU040826.D  
Acq On : 20 Oct 2020 00:14  
Operator : SY/MD  
Sample : L4420-11  
Misc : 25.0mL/MSVOA U/WATER  
ALS Vial : 39 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
C0AK4

Quant Time: Oct 20 05:20:42 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Tue Oct 20 05:12:18 2020  
Response via : Initial Calibration


| Internal Standards            | R.T.  | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|-------|------|----------|--------|--------|----------|
| 42) Toluene                   | 7.97  | 91   | 1872     | 0.047  | ug/L   | 95       |
| 44) trans-1,3-Dichloropropene | 8.19  | 75   | 846      | 0.062  | ug/L # | 4        |
| 45) 1,1,2-Trichloroethane     | 8.40  | 97   | 405      | 0.050  | ug/L # | 87       |
| 47) Tetrachloroethene         | 8.56  | 164  | 166299   | 23.117 | ug/L   | 97       |
| 48) 2-Hexanone                | 8.64  | 43   | 19433    | 3.021  | ug/L # | 71       |
| 49) Dibromochloromethane      | 8.56  | 129  | 159638   | 17.092 | ug/L # | 10       |
| 59) 1,2,3-Trichloropropane    | 11.81 | 75   | 6495     | 0.816  | ug/L   | 90       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101920\  
Data File : VU040826.D  
Acq On : 20 Oct 2020 00:14  
Operator : SY/MD  
Sample : L4420-11  
Misc : 25.0mL/MSVOA U/WATER  
ALS Vial : 39 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
C0AK4

Quant Time: Oct 20 05:20:42 2020  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Tue Oct 20 05:12:18 2020  
Response via : Initial Calibration

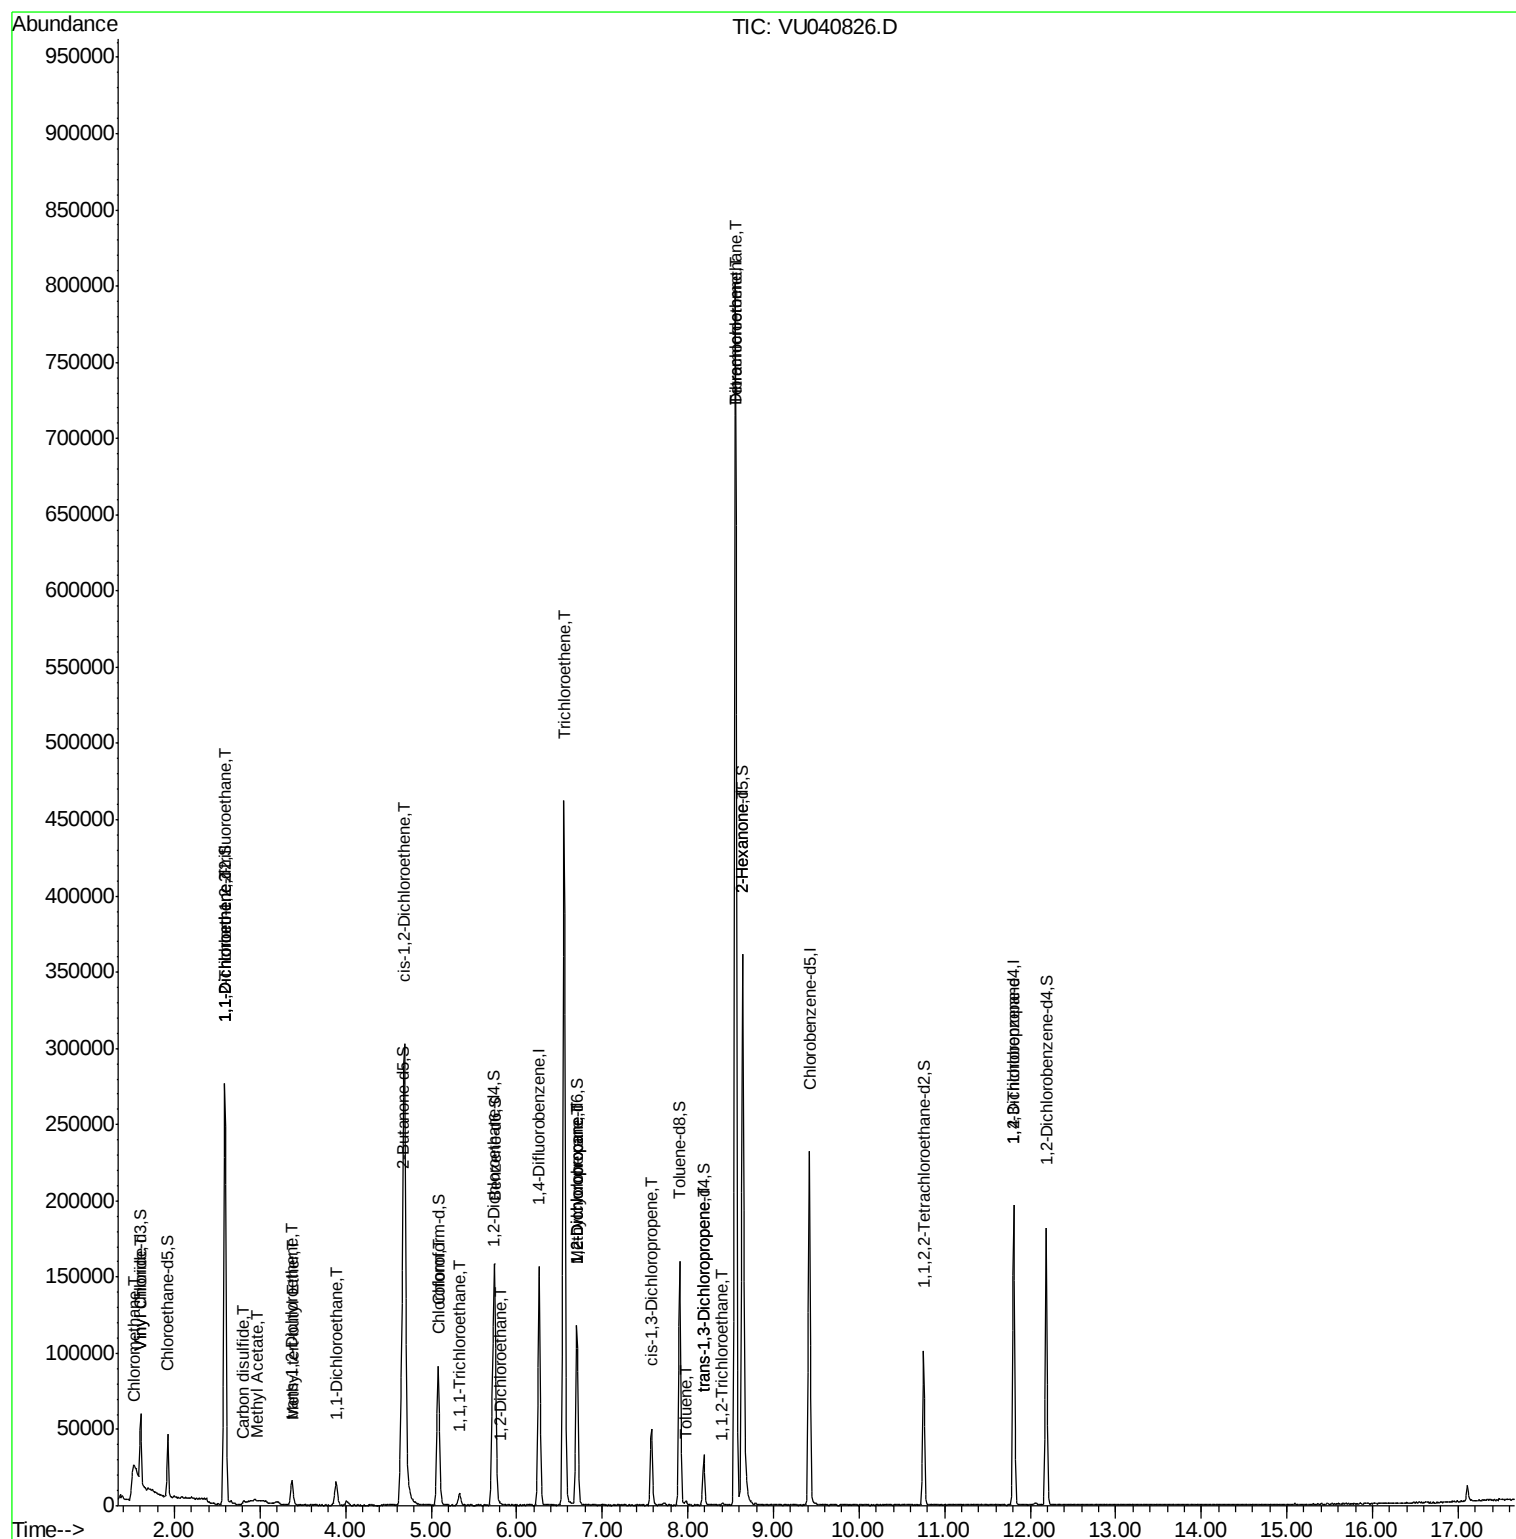

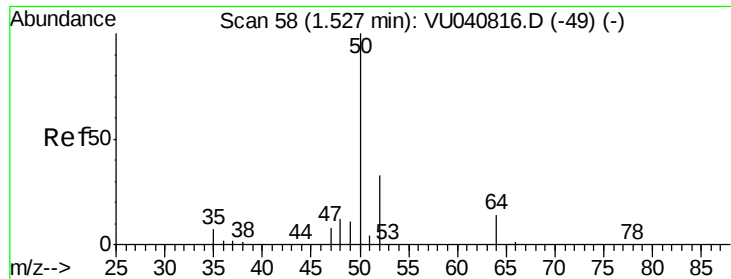

#3

Chloromethane

Concen: 0.134 ug/L

RT: 1.53 min Scan# 58

Delta R.T. -0.00 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Instrument :

MSVOA\_U

ClientSampleId :





C0AK4

Tot Ion: 50 Resp: 1303

Ion Ratio Lower Upper

50 100

52 16.6 21.9 40.7#

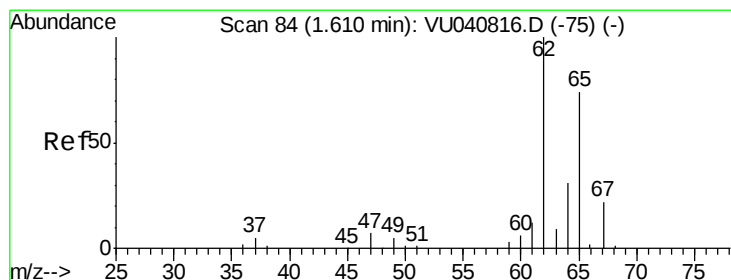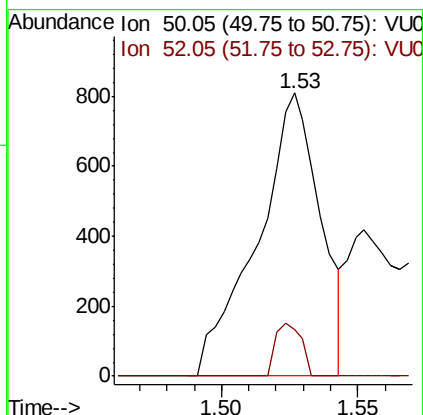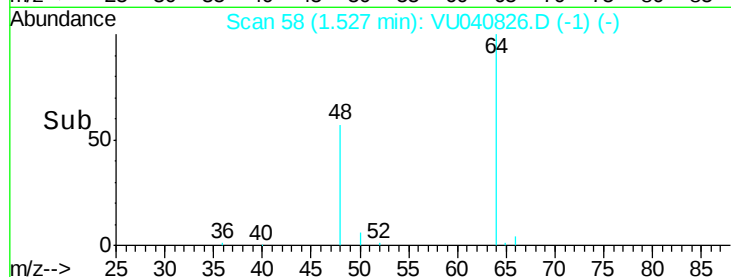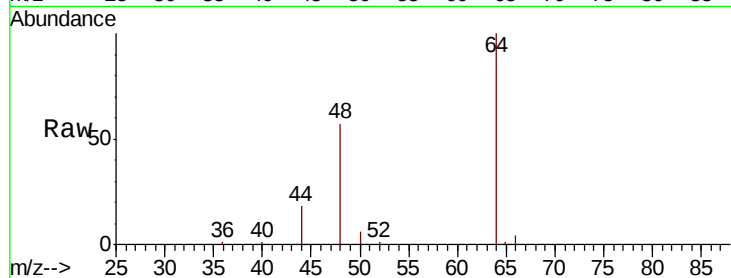

#5

Vinyl chloride

Concen: 0.284 ug/L

RT: 1.61 min Scan# 84

Delta R.T. -0.00 min

Lab File: VU040826.D




Acq: 20 Oct 2020 00:14


Tgt Ion: 62 Resp: 2912

Ion Ratio Lower Upper

62 100

64 318.8 23.7 44.1#

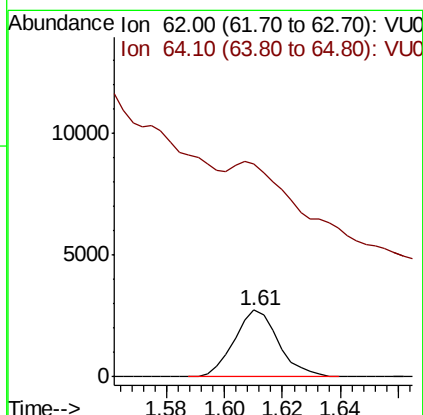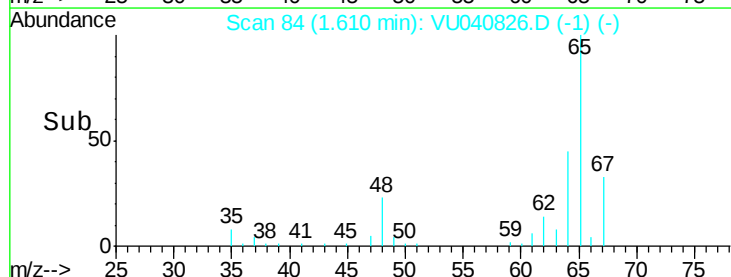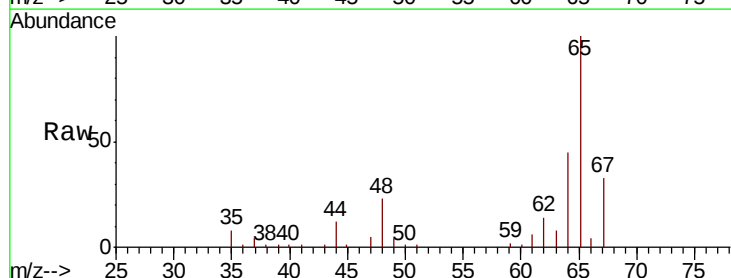

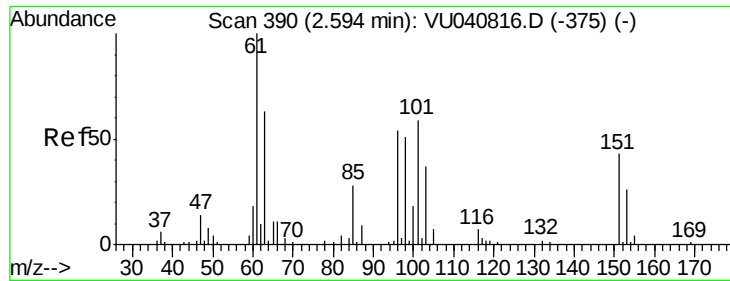

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.054 ug/L

RT: 2.59 min Scan# 388

Delta R.T. -0.01 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Instrument :

MSVOA\_U

ClientSampleId :

C0AK4


Tot Ion:101 Resp: 519

Ion Ratio Lower Upper

101 100

85 0.0 36.7 55.1#

151 0.0 58.0 87.0#

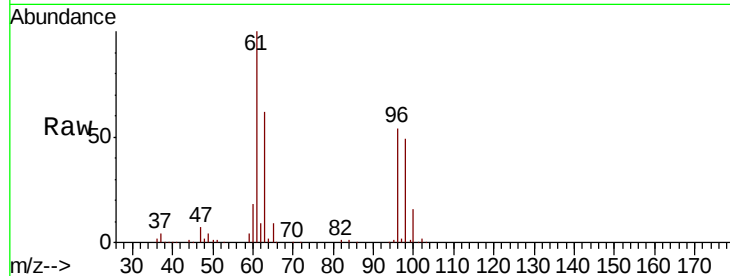

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VU0

Ion 151.00 (150.70 to 151.70): V

2.59



300

200

100

0

Time--> 2.54 2.56 2.58 2.60 2.62



#12

1,1-Dichloroethene

Concen: 9.329 ug/L

RT: 2.59 min Scan# 390

Delta R.T. -0.00 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14


Tgt Ion: 96 Resp: 76556

Ion Ratio Lower Upper

96 100

61 179.7 128.8 239.2

63 83.5 84.6 157.2#



Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 63.00 (62.70 to 63.70): VU0

2.59

100000

80000


60000


40000

20000

0

Time--> 2.55 2.60 2.65



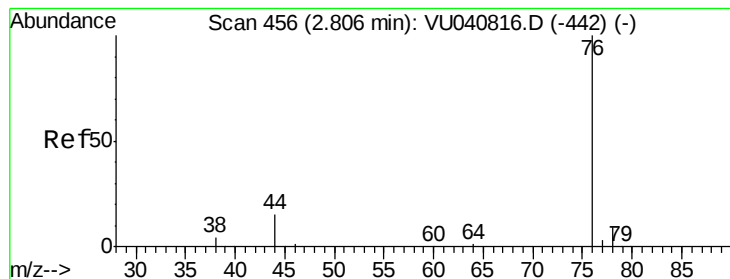

#14

Carbon disulfide

Concen: 0.122 ug/L

RT: 2.81 min Scan# 456

Delta R.T. -0.00 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Instrument :

MSVOA\_U

ClientSampleId :


C0AK4

Tot Ion: 76 Resp: 2810

Ion Ratio Lower Upper




76 100

78 6.2 6.8 10.2#



Abundance Ion 76.05 (75.75 to 76.75): VU0

Ion 78.00 (77.70 to 78.70): VU0

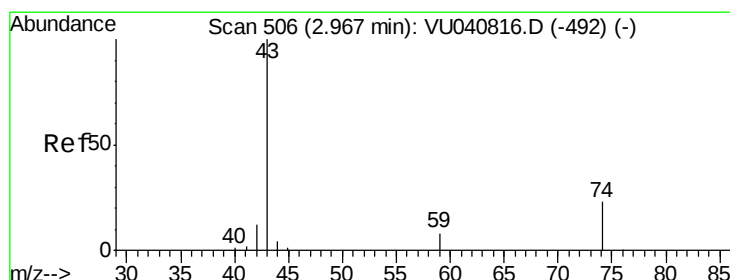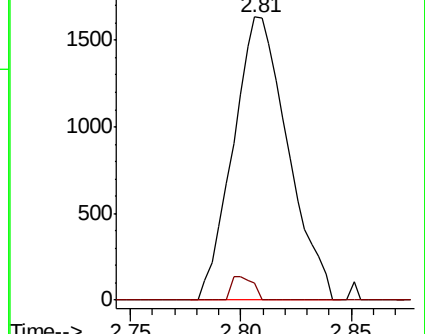

#15

Methyl Acetate

Concen: 0.132 ug/L

RT: 2.96 min Scan# 503

Delta R.T. -0.01 min

Lab File: VU040826.D


Acq: 20 Oct 2020 00:14

Tgt Ion: 43 Resp: 710

Ion Ratio Lower Upper



43 100


74 0.0 16.5 24.7#



Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 74.05 (73.75 to 74.75): VU0

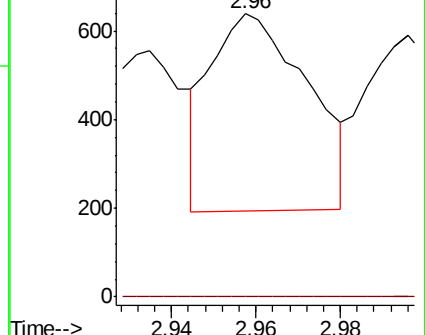

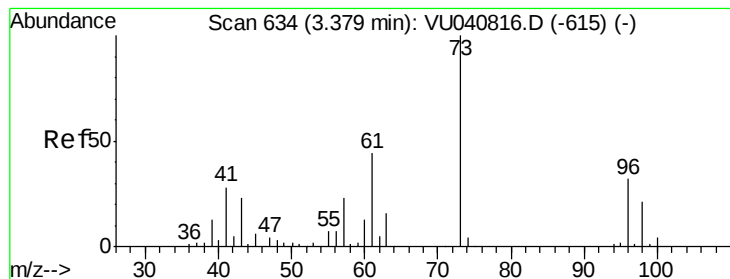


#17




Methvl tert-butvl Ether  
 Concen: 0.179 ug/L  
 RT: 3.39 min Scan# 637  
 Delta R.T. 0.01 min  
 Lab File: VU040826.D  
 Acq: 20 Oct 2020 00:14

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 C0AK4

Tot Ion: 73 Resp: 4163  
 Ion Ratio Lower Upper  
 73 100  
 43 24.6 18.2 27.4  
 57 24.1 18.6 28.0

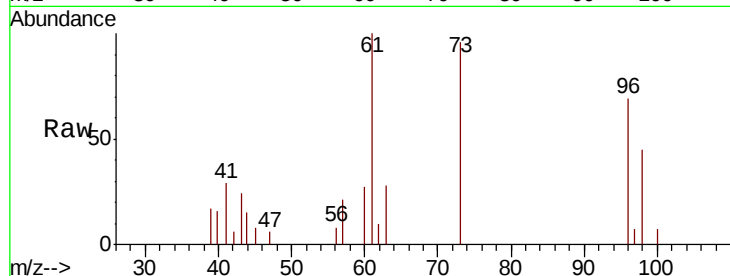


Abundance Ion 73.10 (72.80 to 73.80): VU0  
 Ion 43.05 (42.75 to 43.75): VU0  
 Ion 57.10 (56.80 to 57.80): VU0

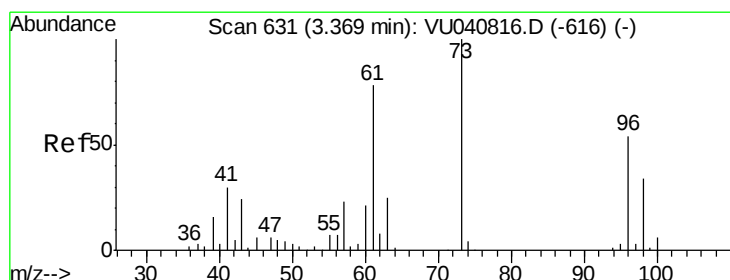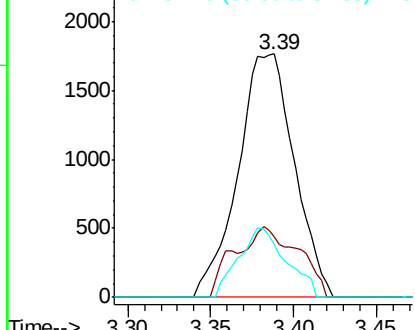



#18


trans-1,2-Dichloroethene  
 Concen: 0.625 ug/L  
 RT: 3.37 min Scan# 631  
 Delta R.T. -0.00 min  
 Lab File: VU040826.D  
 Acq: 20 Oct 2020 00:14

Tgt Ion: 96 Resp: 5371  
 Ion Ratio Lower Upper  
 96 100  
 61 149.6 105.9 196.7  
 98 62.4 43.8 81.3



Abundance Ion 96.00 (95.70 to 96.70): VU0  
 Ion 61.05 (60.75 to 61.75): VU0  
 Ion 97.95 (97.65 to 98.65): VU0

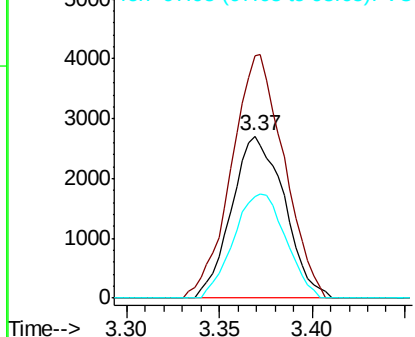

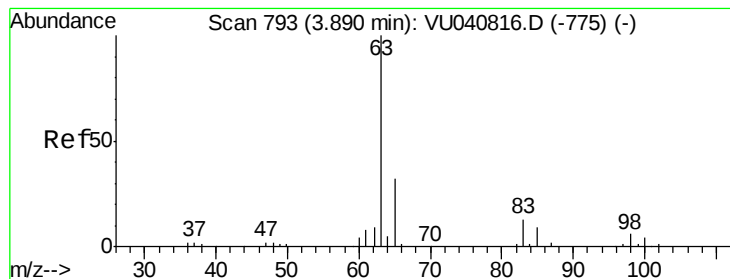

#19

1,1-Dichloroethane

Concen: 1.000 ug/L

RT: 3.89 min Scan# 793

Delta R.T. -0.00 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Instrument :

MSVOA\_U

ClientSampleId :

C0AK4


Tot Ion: 63 Resp: 17762

Ion Ratio Lower Upper

63 100

65 32.8 21.9 40.7




83 15.5 9.6 17.8



Abundance Ion 63.10 (62.80 to 63.80): VU040826.D (-775) (-)

Ion 65.10 (64.80 to 65.80): VU040826.D (-775) (-)

Ion 83.05 (82.75 to 83.75): VU040826.D (-775) (-)

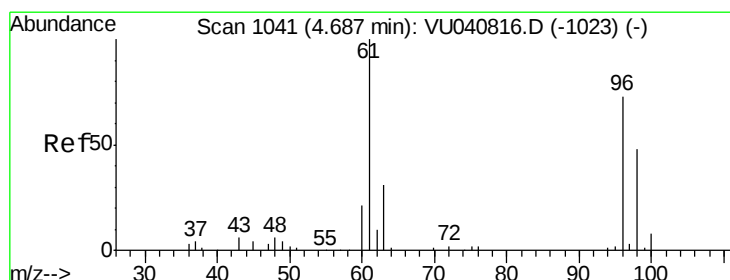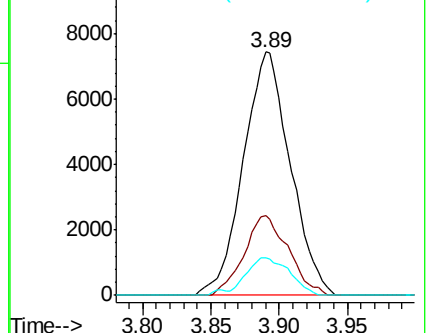

#22

cis-1,2-Dichloroethene

Concen: 13.956 ug/L

RT: 4.69 min Scan# 1041

Delta R.T. -0.00 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14


Tgt Ion: 96 Resp: 129282

Ion Ratio Lower Upper

96 100

61 136.4 99.8 185.4



68 0.0 0.0 0.0




Abundance Ion 96.00 (95.70 to 96.70): VU040826.D (-948) (-)

Ion 61.05 (60.75 to 61.75): VU040826.D (-948) (-)

Ion 68.15 (67.85 to 68.85): VU040826.D (-948) (-)



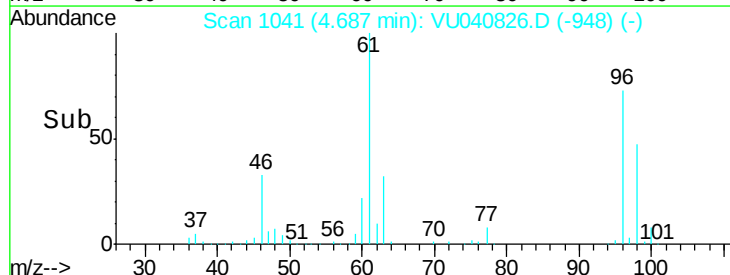
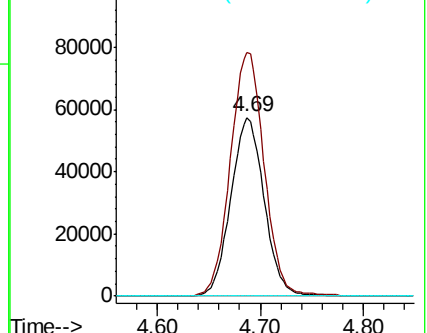


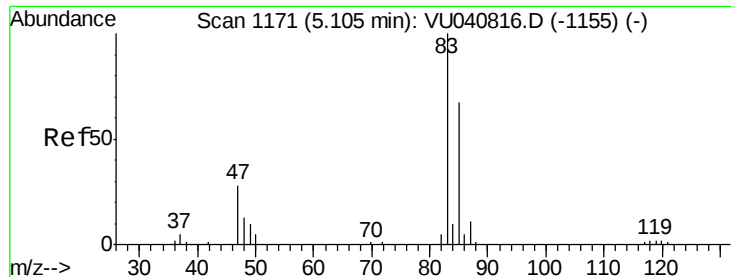

#25  
Chloroform  
Concen: 0.142 ug/L  
RT: 5.10 min Scan# 1170  
Delta R.T. -0.00 min  
Lab File: VU040826.D  
Acq: 20 Oct 2020 00:14




Instrument :  
MSVOA\_U  
ClientSampled :  
C0AK4


Tot Ion: 83 Resp: 2572  
Ion Ratio Lower Upper  
83 100  
85 55.9 46.5 86.5

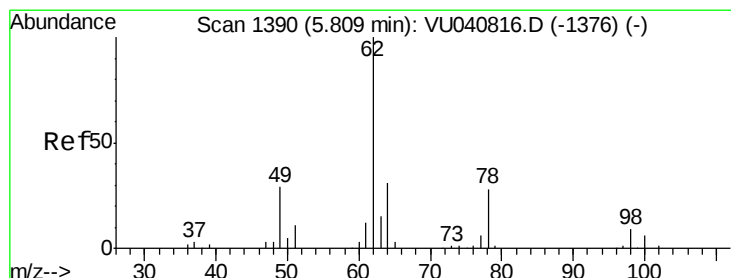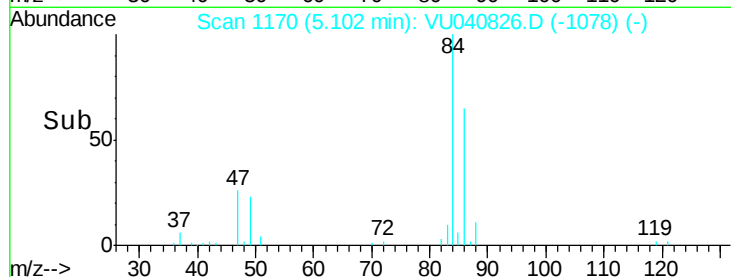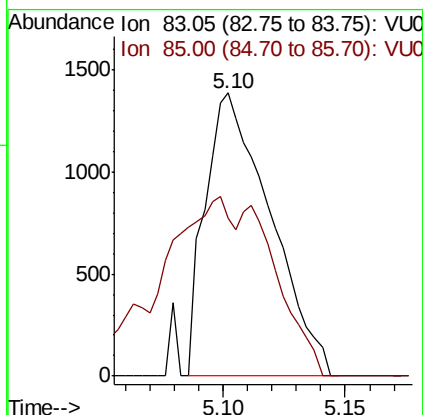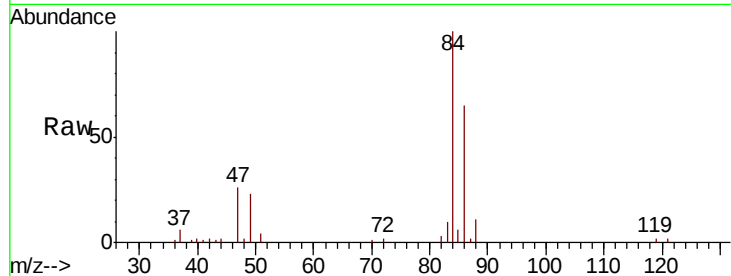

#27  
1,2-Dichloroethane  
Concen: 0.068 ug/L  
RT: 5.82 min Scan# 1392  
Delta R.T. 0.01 min  
Lab File: VU040826.D  
Acq: 20 Oct 2020 00:14

Tgt Ion: 62 Resp: 877  
Ion Ratio Lower Upper  
62 100  
98 0.0 6.6 10.0#


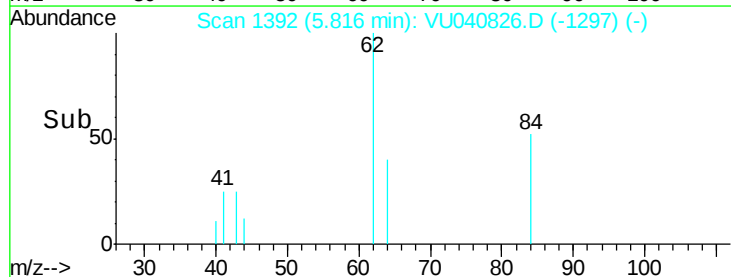
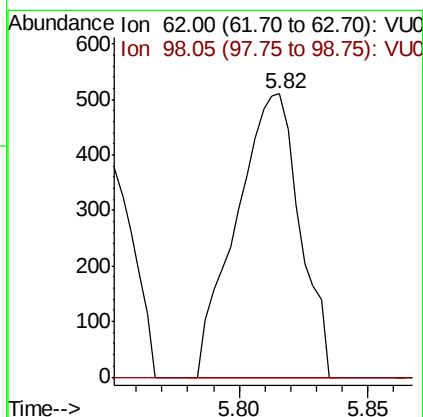
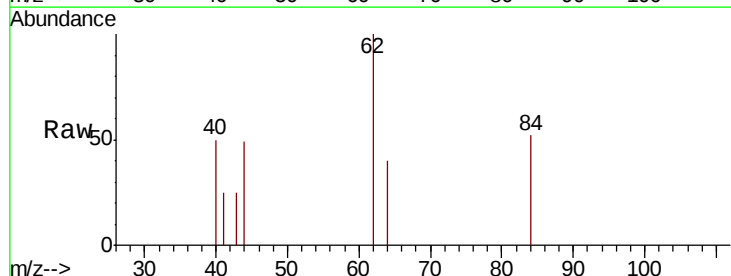


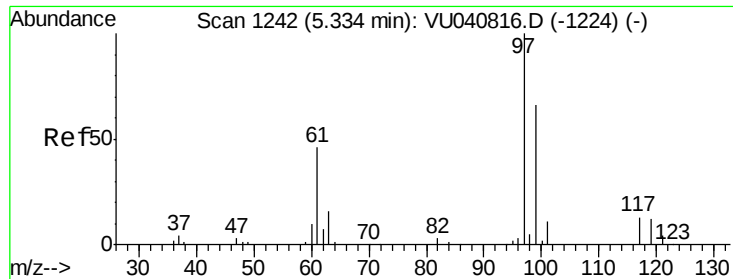

#29  
1,1,1-Trichloroethane  
Concen: 0.320 ug/L  
RT: 5.33 min Scan# 1242  
Delta R.T. -0.00 min  
Lab File: VU040826.D  
Acq: 20 Oct 2020 00:14




Instrument :  
MSVOA\_U  
ClientSampleId :  
C0AK4


Tot Ion: 97 Resp: 5211  
Ion Ratio Lower Upper  
97 100  
99 66.6 51.3 76.9  
61 49.3 39.4 59.2

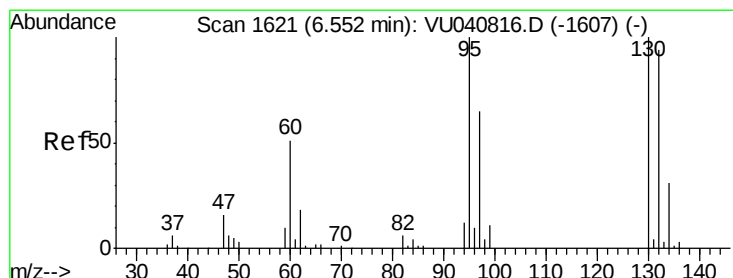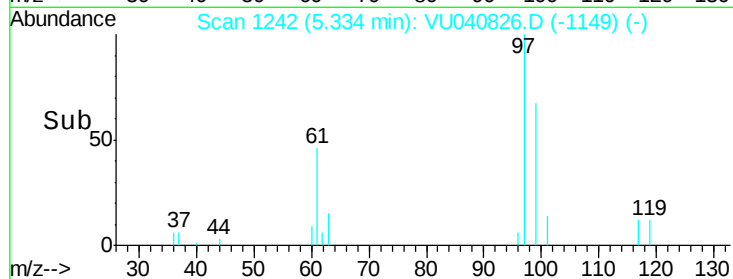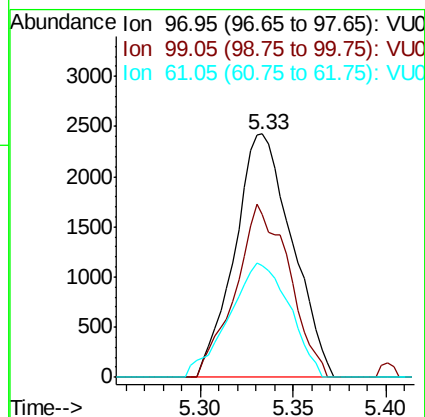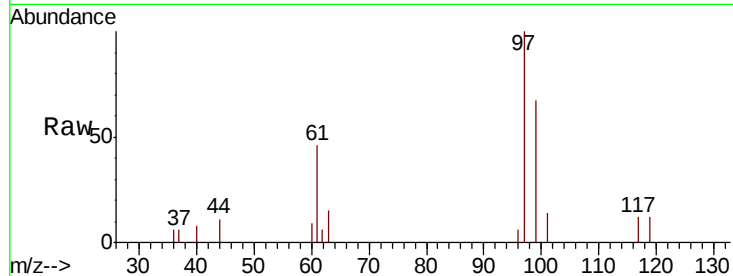

#34  
Trichloroethene  
Concen: 15.243 ug/L  
RT: 6.56 min Scan# 1622  
Delta R.T. 0.00 min  
Lab File: VU040826.D  
Acq: 20 Oct 2020 00:14

Tgt Ion: 95 Resp: 153699  
Ion Ratio Lower Upper  
95 100  
97 66.0 45.5 84.5  
132 93.0 67.5 125.4  
130 99.4 69.9 129.9

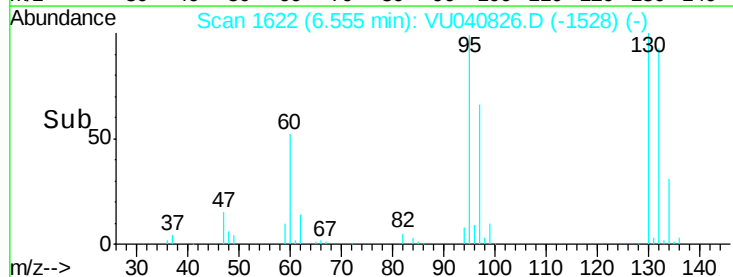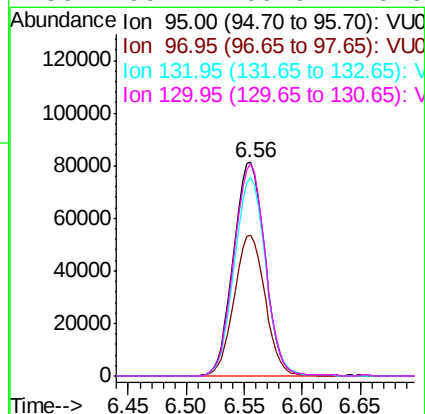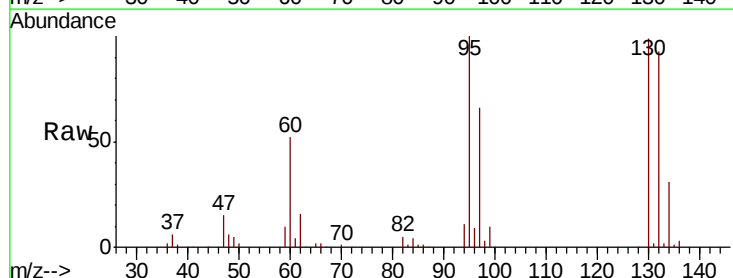

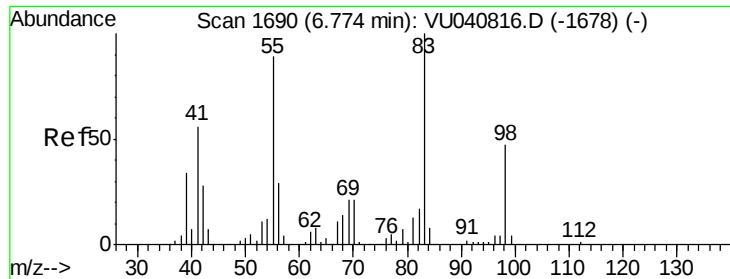

#35

Methylcyclohexane

Concen: 0.829 ug/L

RT: 6.70 min Scan# 1668

Delta R.T. -0.07 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Instrument :

MSVOA\_U

ClientSampleId :

C0AK4


Tot Ion: 83 Resp: 11853

Ion Ratio Lower Upper

83 100

55 0.0 70.7 106.1#




98 0.0 38.4 57.6#

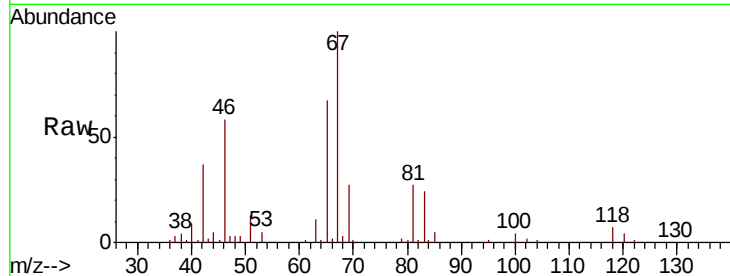

Abundance Ion 83.15 (82.85 to 83.85): VU0

Ion 55.10 (54.80 to 55.80): VU0

Ion 98.15 (97.85 to 98.85): VU0

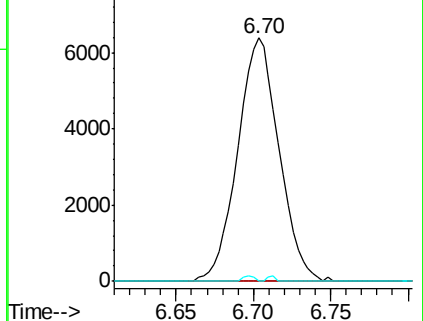

#37

1,2-Dichloropropane

Concen: 0.529 ug/L

RT: 6.70 min Scan# 1668

Delta R.T. -0.10 min

Lab File: VU040826.D


Acq: 20 Oct 2020 00:14

Tgt Ion: 63 Resp: 5737

Ion Ratio Lower Upper



63 100


112 0.0 3.5 5.3#



Abundance Ion 63.10 (62.80 to 63.80): VU0

Ion 112.10 (111.80 to 112.80): V

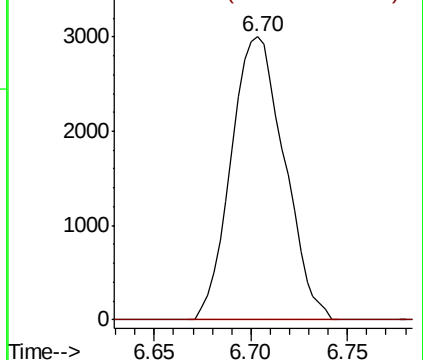

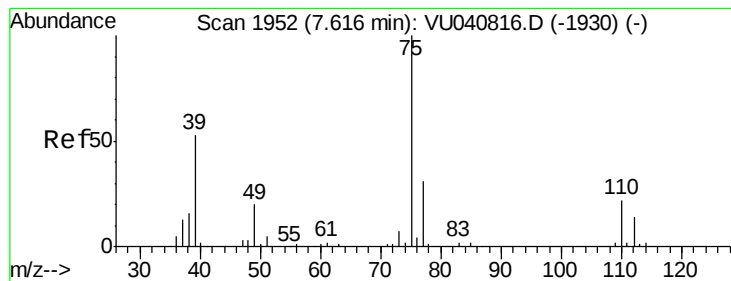

#39

cis-1,3-Dichloropropene

Concen: 0.085 ug/L

RT: 7.57 min Scan# 1939

Delta R.T. -0.04 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Instrument :

MSVOA\_U

ClientSampleId :


C0AK4

Tot Ion: 75 Resp: 1260

Ion Ratio Lower Upper

75 100

77 63.4 20.5 38.1#

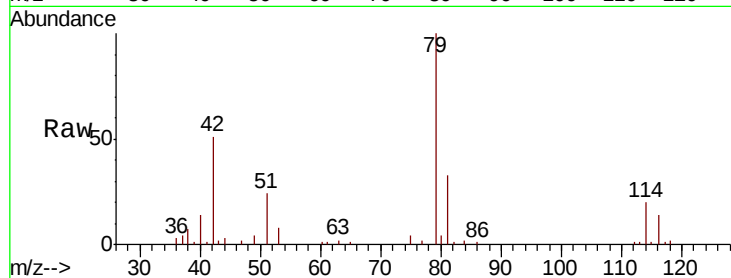

Abundance Ion 75.05 (74.75 to 75.75): VU0

Ion 77.05 (76.75 to 77.75): VU0

7.57

600



400

200

0

7.55 7.60

Time-->

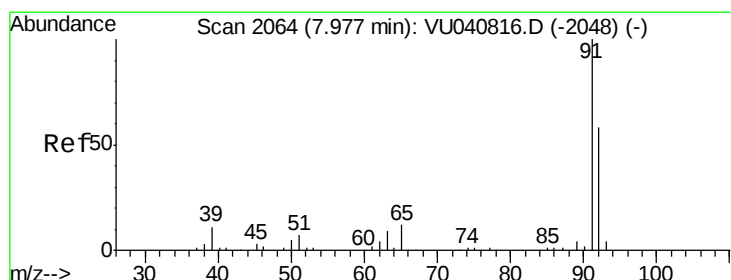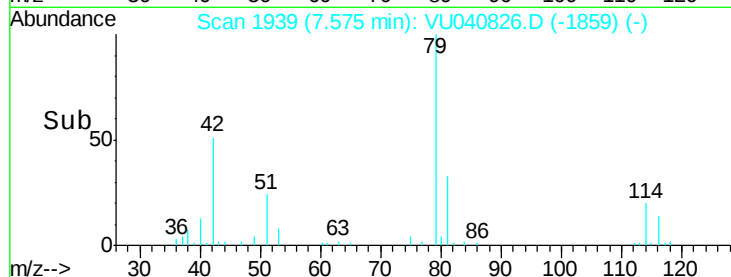

#42

Toluene

Concen: 0.047 ug/L

RT: 7.97 min Scan# 2063

Delta R.T. -0.00 min

Lab File: VU040826.D


Acq: 20 Oct 2020 00:14

Tgt Ion: 91 Resp: 1872

Ion Ratio Lower Upper

91 100

92 54.0 40.2 74.6

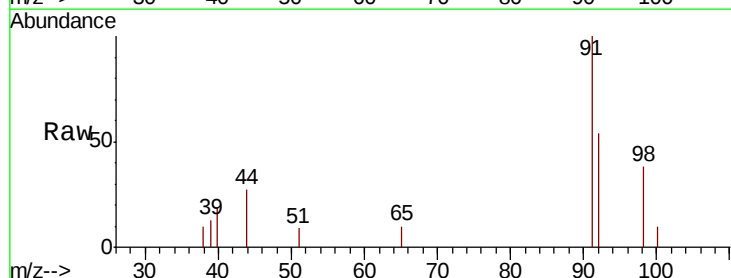

Abundance Ion 91.15 (90.85 to 91.85): VU0

Ion 92.15 (91.85 to 92.85): VU0

7.97

1200

1000

800

600


400


200

0

7.95 8.00

Time-->

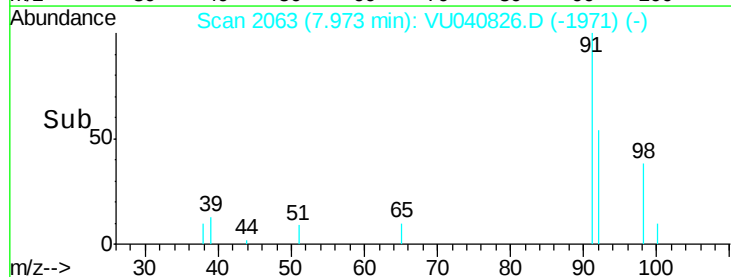

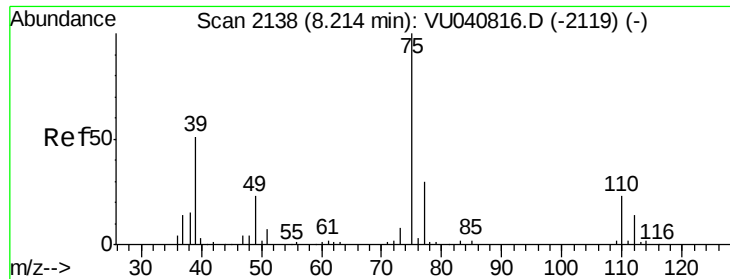

#44

trans-1,3-Dichloropropene

Concen: 0.062 ug/L

RT: 8.19 min Scan# 2129

Delta R.T. -0.03 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Instrument :

MSVOA\_U

ClientSampleId :


C0AK4

Tot Ion: 75 Resp: 846




Ion Ratio Lower Upper

75 100

77 80.5 20.4 38.0#

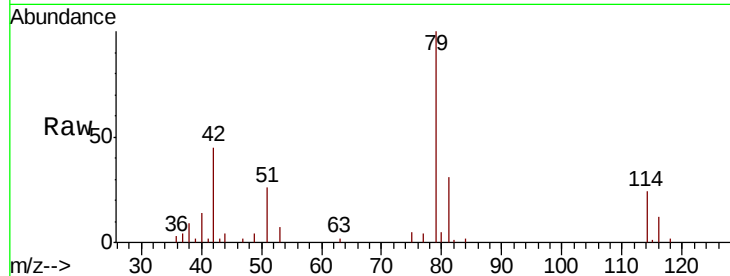

Abundance Ion 75.05 (74.75 to 75.75): VU040826.D (-2045) (-)

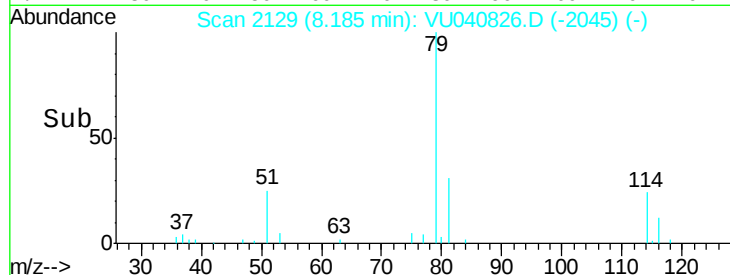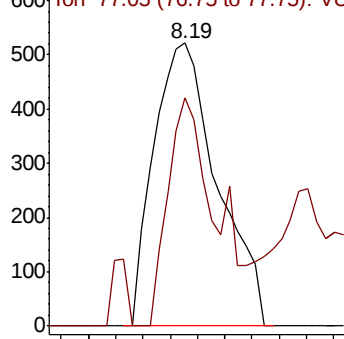

#45

1,1,2-Trichloroethane

Concen: 0.050 ug/L

RT: 8.40 min Scan# 2196

Delta R.T. -0.00 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Tgt Ion: 97 Resp: 405


Ion Ratio Lower Upper

97 100



99 50.0 44.0 81.6


83 86.1 62.9 116.9

85 39.5 40.3 74.8#



Abundance Ion 96.95 (96.65 to 97.65): VU040826.D (-2104) (-)

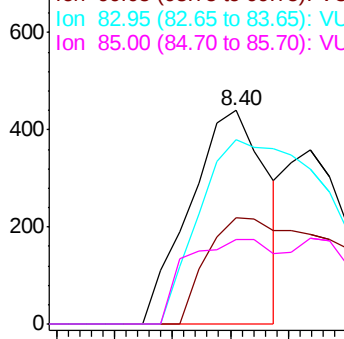

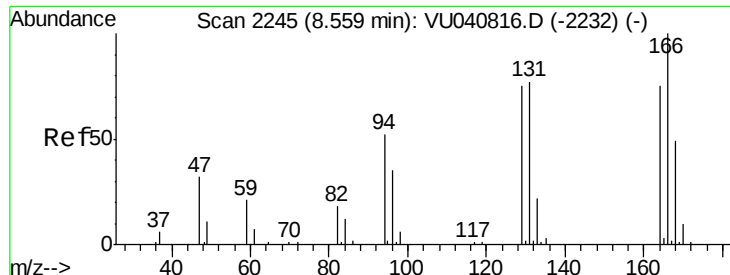

#47

Tetrachloroethene

Concen: 23.117 ug/L

RT: 8.56 min Scan# 2245

Delta R.T. -0.00 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Instrument :

MSVOA\_U

ClientSampled :

C0AK4

Tot Ion:164 Resp: 166299


Ion Ratio Lower Upper

164 100

129 97.6 68.8 127.8

131 95.3 66.7 123.9

166 128.8 83.9 155.7



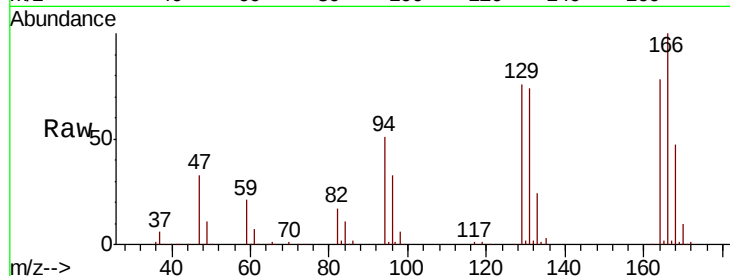


Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

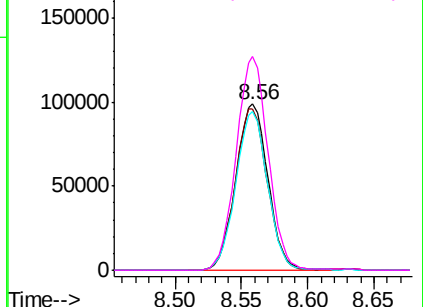

#48

2-Hexanone

Concen: 3.021 ug/L

RT: 8.64 min Scan# 2271

Delta R.T. -0.05 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Tgt Ion: 43 Resp: 19433


Ion Ratio Lower Upper

43 100

58 28.0 41.0 61.6#

57 26.8 14.4 21.6#

100 0.8 8.6 13.0#






Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

Ion 57.20 (56.90 to 57.90): VU0

Ion 100.15 (99.85 to 100.85): VU0

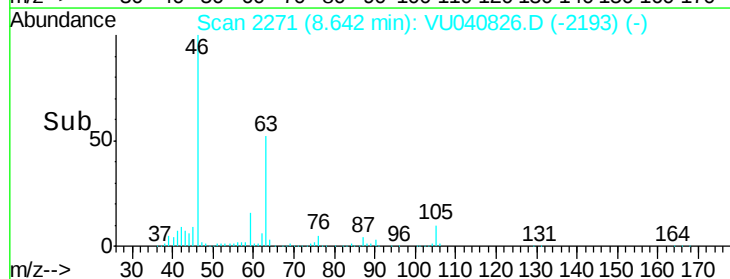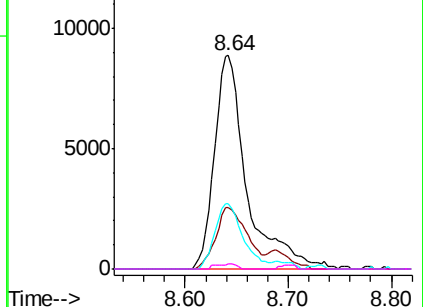

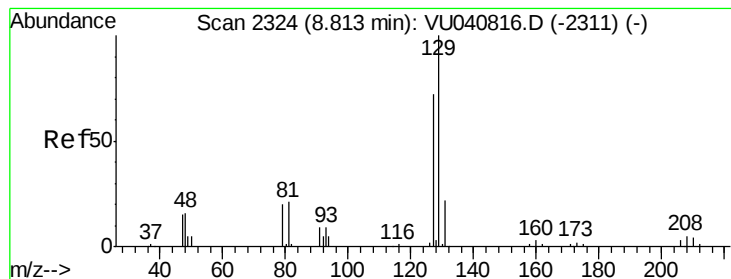

#49

Dibromochloromethane

Concen: 17.092 ug/L

RT: 8.56 min Scan# 2245

Delta R.T. -0.25 min

Lab File: VU040826.D

Acq: 20 Oct 2020 00:14

Instrument :

MSVOA\_U

ClientSampleId :


C0AK4

Tot Ion:129 Resp: 159638

Ion Ratio Lower Upper




129 100

127 0.1 55.8 103.6#

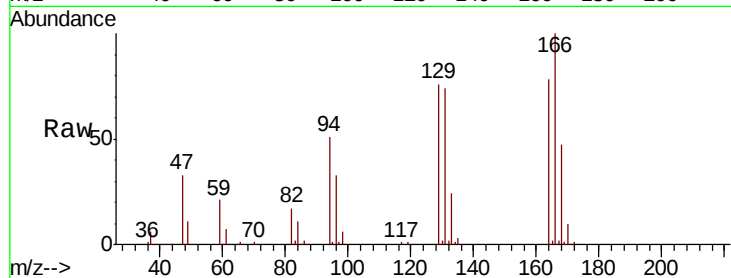

Abundance Ion 128.95 (128.65 to 129.65): V

Ion 126.90 (126.60 to 127.60): V

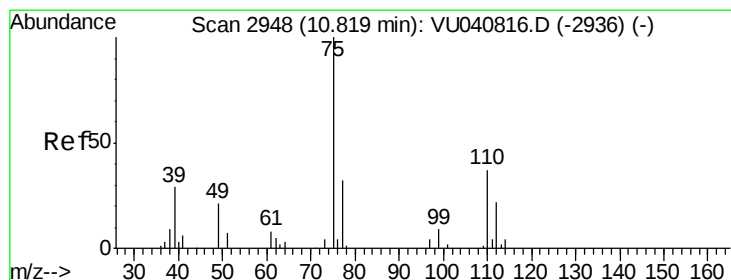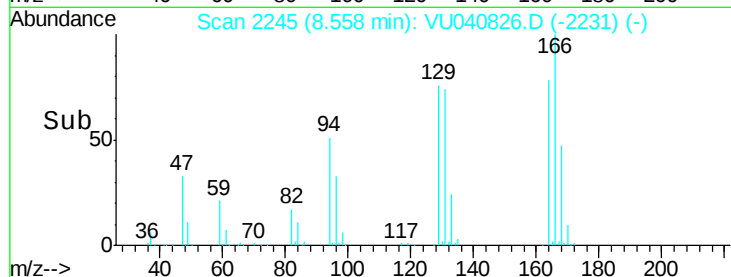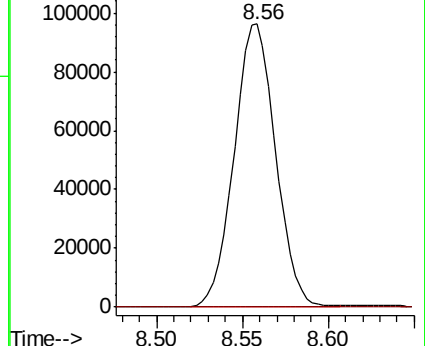

#59

1,2,3-Trichloropropane

Concen: 0.816 ug/L

RT: 11.81 min Scan# 3255

Delta R.T. 0.99 min

Lab File: VU040826.D


Acq: 20 Oct 2020 00:14

Tgt Ion: 75 Resp: 6495

Ion Ratio Lower Upper

75 100

77 38.4 26.4 39.6

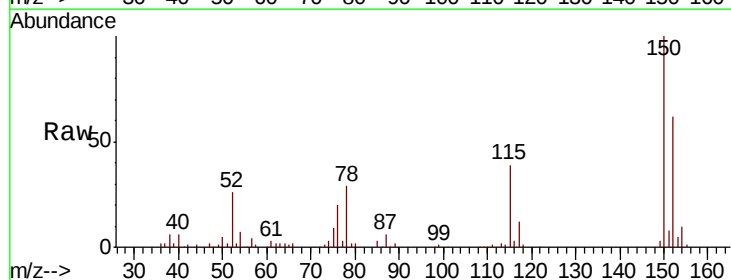

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 77.00 (76.70 to 77.70): VU0

