

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U101920\  
 Data File : VU040837.D  
 Acq On : 20 Oct 2020 04:28  
 Operator : SY/MD  
 Sample : L4428-08  
 Misc : 25.0mL/MSVOA U/WATER  
 ALS Vial : 50 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 ETZ34

Quant Time: Oct 20 06:58:13 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
 Quant Title : TRACE VOA SOM01.0  
 QLast Update : Tue Oct 20 05:12:18 2020  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Difluorobenzene     | 6.26  | 114  | 114346   | 5.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 9.42  | 117  | 116267   | 5.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 11.81 | 152  | 47407    | 5.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                                |        |       |          |          |      |         |
|--------------------------------|--------|-------|----------|----------|------|---------|
| 4) Vinyl Chloride-d3           | 1.60   | 65    | 28678    | 3.03     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 40 - 130 | Recovery | =    | 60.60%  |
| 7) Chloroethane-d5             | 1.92   | 69    | 27960    | 3.83     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 130 | Recovery | =    | 76.60%  |
| 11) 1,1-Dichloroethene-d2      | 2.58   | 63    | 43660    | 2.36     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 125 | Recovery | =    | 47.20%# |
| 20) 2-Butanone-d5              | 4.66   | 46    | 182518   | 60.20    | ug/L | 0.01    |
| Spiked Amount                  | 50.000 | Range | 40 - 130 | Recovery | =    | 120.40% |
| 24) Chloroform-d               | 5.08   | 84    | 77863    | 4.68     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 93.60%  |
| 26) 1,2-Dichloroethane-d4      | 5.72   | 65    | 48524    | 4.79     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 95.80%  |
| 32) Benzene-d6                 | 5.74   | 84    | 127663   | 4.07     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 125 | Recovery | =    | 81.40%  |
| 36) 1,2-Dichloropropane-d6     | 6.70   | 67    | 47385    | 4.55     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 60 - 140 | Recovery | =    | 91.00%  |
| 41) Toluene-d8                 | 7.91   | 98    | 94393    | 3.36     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 70 - 130 | Recovery | =    | 67.20%# |
| 43) trans-1,3-Dichloropropene- | 8.18   | 79    | 16881    | 3.83     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 55 - 130 | Recovery | =    | 76.60%  |
| 46) 2-Hexanone-d5              | 8.64   | 63    | 115111   | 50.65    | ug/L | 0.00    |
| Spiked Amount                  | 50.000 | Range | 45 - 130 | Recovery | =    | 101.30% |
| 57) 1,1,2,2-Tetrachloroethane- | 10.75  | 84    | 48008    | 5.14     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 65 - 120 | Recovery | =    | 102.80% |
| 64) 1,2-Dichlorobenzene-d4     | 12.19  | 152   | 44918    | 5.11     | ug/L | 0.00    |
| Spiked Amount                  | 5.000  | Range | 80 - 120 | Recovery | =    | 102.20% |

## Target Compounds


| Target Compounds             | R.T. | QIon | Response | Conc   | Units  | Ovalue |
|------------------------------|------|------|----------|--------|--------|--------|
| 5) Vinyl chloride            | 1.61 | 62   | 434871   | 42.621 | ug/L   | 88     |
| 12) 1,1-Dichloroethene       | 2.59 | 96   | 2582     | 0.316  | ug/L # | 1      |
| 17) Methyl tert-butyl Ether  | 3.38 | 73   | 10814    | 0.469  | ug/L # | 72     |
| 18) trans-1,2-Dichloroethene | 3.37 | 96   | 11039    | 1.293  | ug/L   | 98     |
| 22) cis-1,2-Dichloroethene   | 4.69 | 96   | 881027   | 95.660 | ug/L   | 99     |
| 30) Cyclohexane              | 5.40 | 56   | 2743     | 0.191  | ug/L   | 97     |
| 34) Trichloroethene          | 6.56 | 95   | 9715     | 1.003  | ug/L   | 94     |
| 35) Methylcyclohexane        | 6.77 | 83   | 1480     | 0.108  | ug/L # | 65     |
| 53) m,p-Xylene               | 9.69 | 106  | 2032     | 0.135  | ug/L   | 88     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU101920\  
Data File : VU040837.D  
Acq On : 20 Oct 2020 04:28  
Operator : SY/MD  
Sample : L4428-08  
Misc : 25.0mL/MSVOA U/WATER  
ALS Vial : 50 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
ETZ34

Quant Time: Oct 20 06:58:13 2020  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\SOMUTR100820WMA.M  
Quant Title : TRACE VOA SOM01.0  
QLast Update : Tue Oct 20 05:12:18 2020  
Response via : Initial Calibration

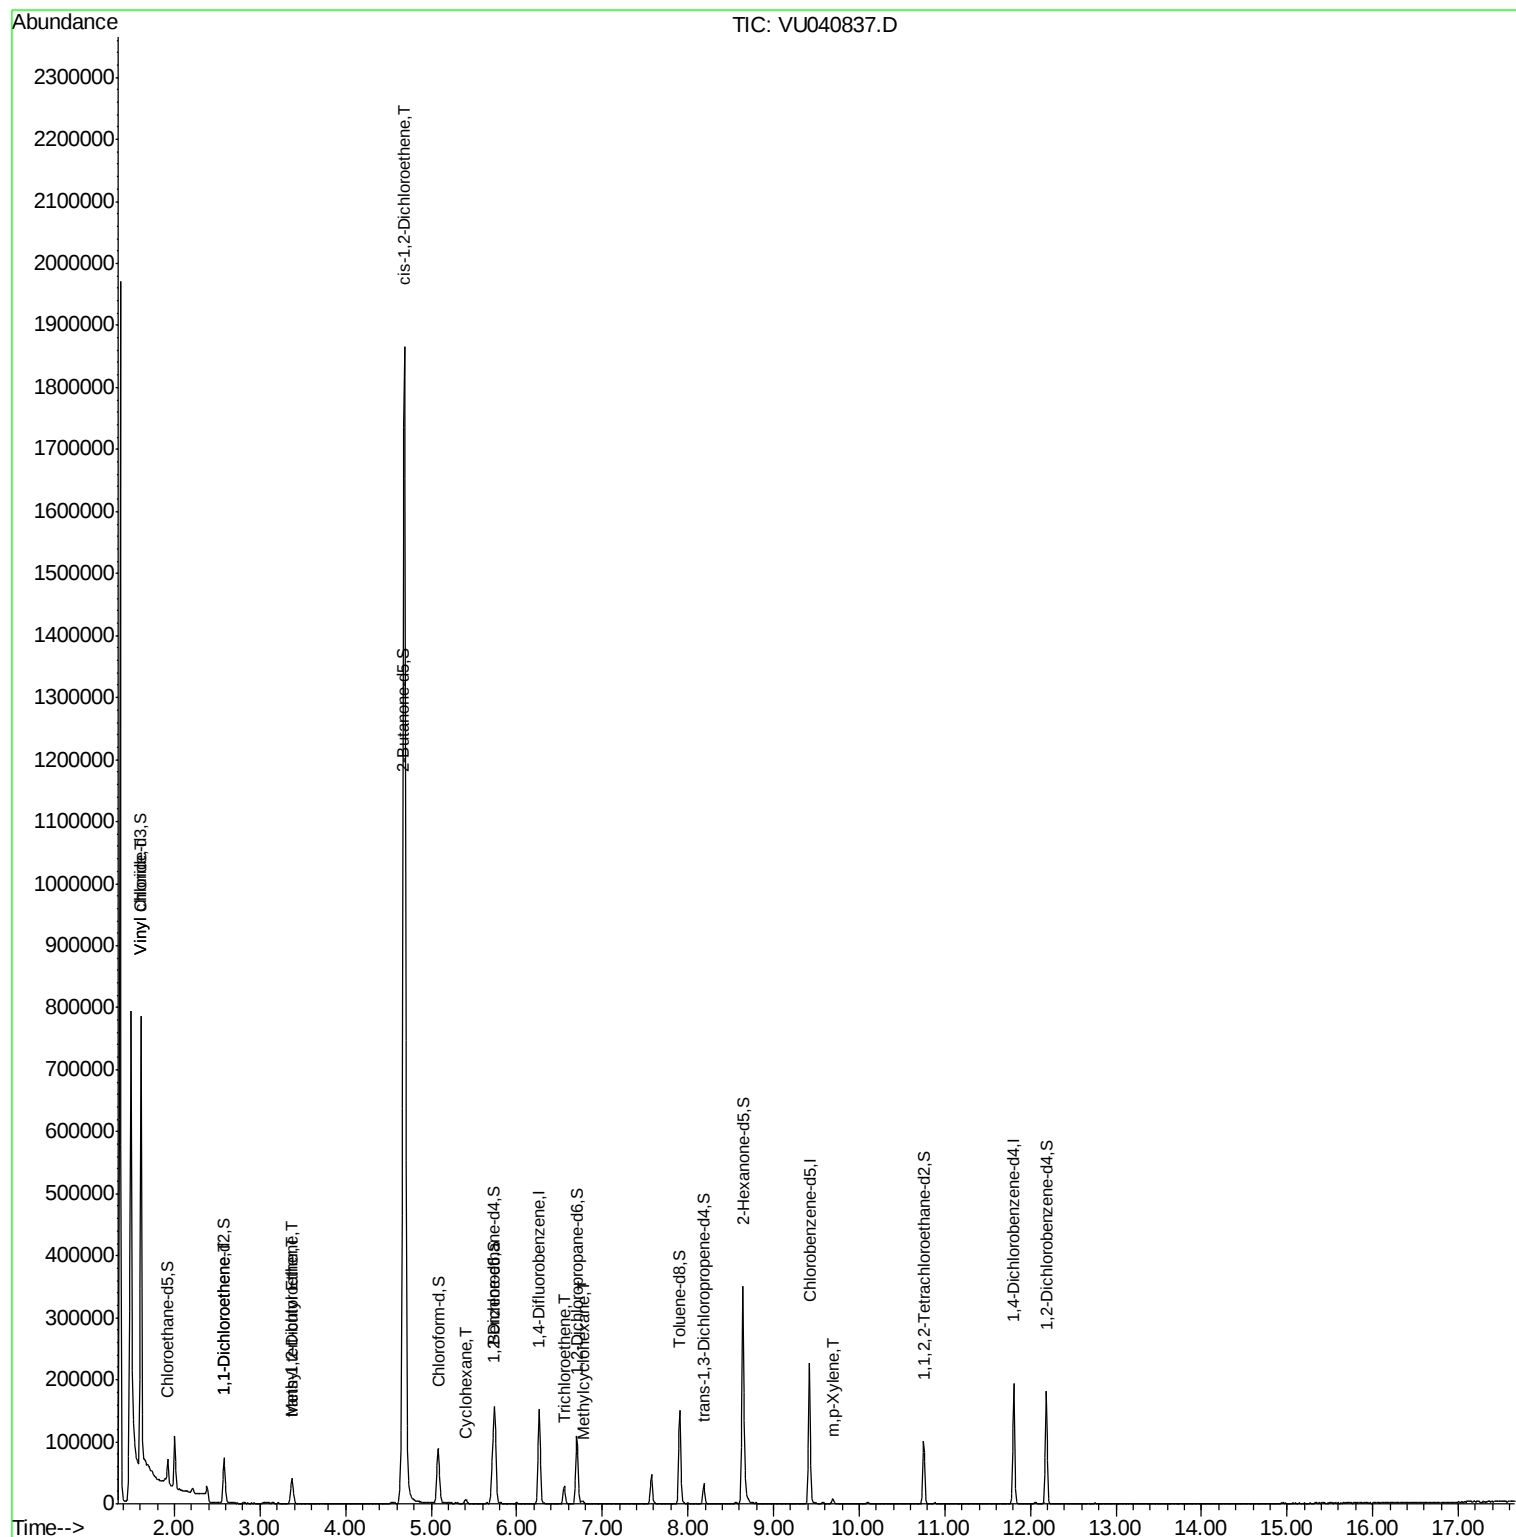

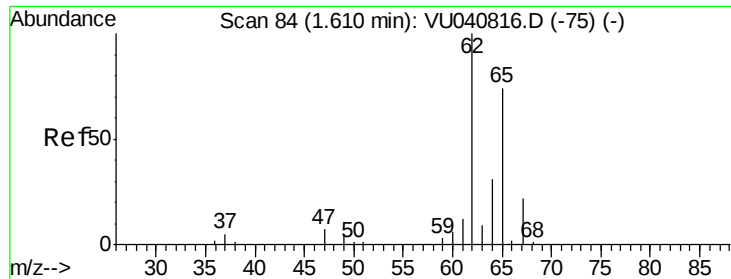

#5

Vinyl chloride

Concen: 42.621 ug/L

RT: 1.61 min Scan# 84

Delta R.T. 0.00 min

Lab File: VU040837.D

Acq: 20 Oct 2020 04:28

Instrument :

MSVOA\_U

ClientSampleId :


ETZ34

Tot Ion: 62 Resp: 434871

Ion Ratio Lower Upper




62 100

64 40.9 23.7 44.1

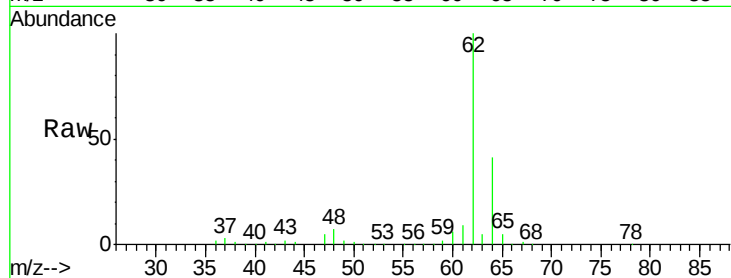

Abundance Ion 62.00 (61.70 to 62.70): VU0

Ion 64.10 (63.80 to 64.80): VU0

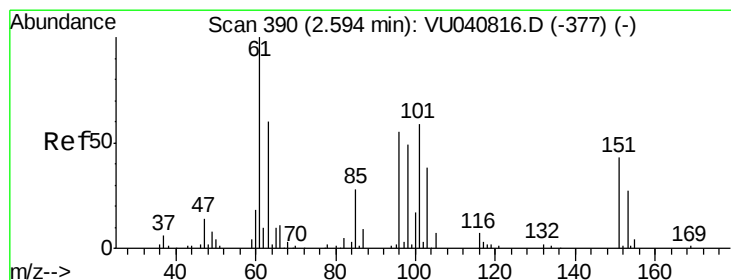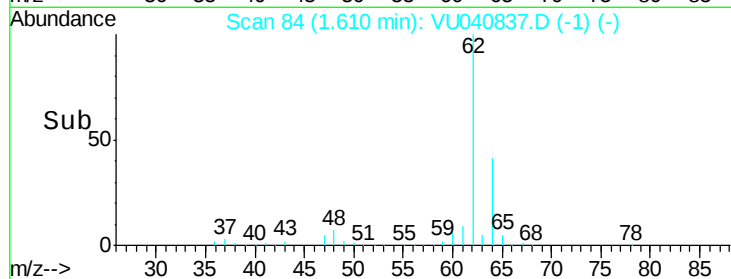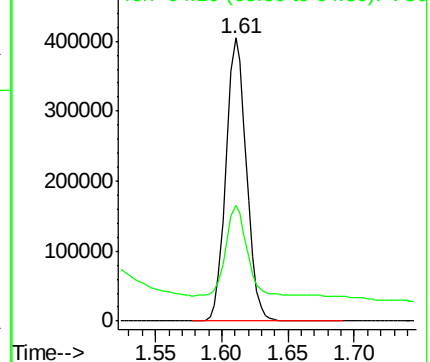

#12

1,1-Dichloroethene

Concen: 0.316 ug/L

RT: 2.59 min Scan# 389

Delta R.T. -0.00 min

Lab File: VU040837.D

Acq: 20 Oct 2020 04:28


Tgt Ion: 96 Resp: 2582

Ion Ratio Lower Upper

96 100

61 257.7 128.8 239.2#



63 954.2 84.6 157.2#

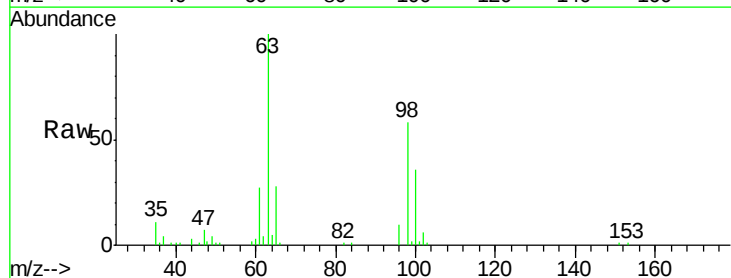


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 63.00 (62.70 to 63.70): VU0

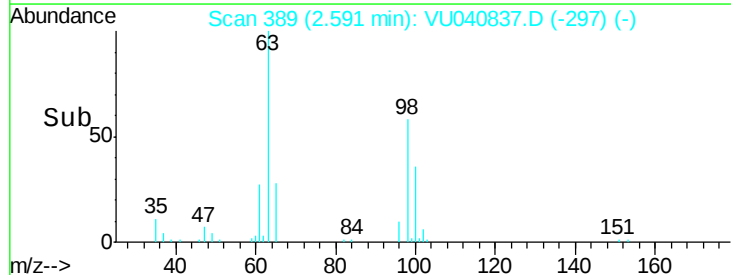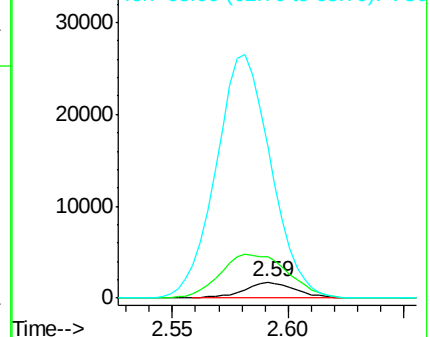


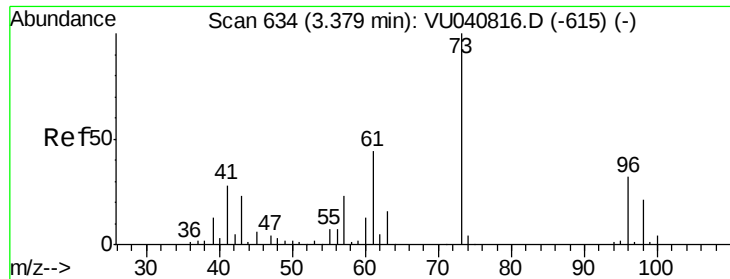




#17  
Methvl tert-butvl Ether  
Concen: 0.469 ug/L  
RT: 3.38 min Scan# 635  
Delta R.T. 0.00 min  
Lab File: VU040837.D  
Acq: 20 Oct 2020 04:28

Instrument :  
MSVOA\_U  
ClientSampleId :  
ETZ34

Tot Ion: 73 Resp: 10814  
Ion Ratio Lower Upper  
73 100  
43 29.7 18.2 27.4#  
57 43.1 18.6 28.0#

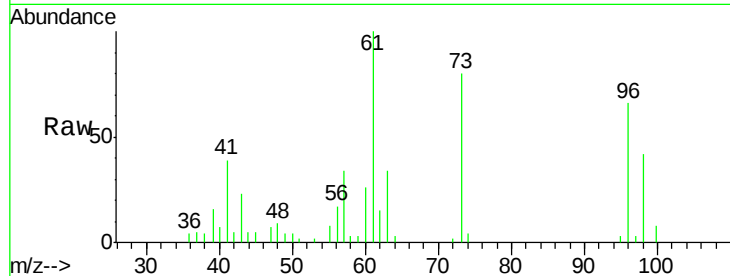


Abundance Ion 73.10 (72.80 to 73.80): VU0  
Ion 43.05 (42.75 to 43.75): VU0  
Ion 57.10 (56.80 to 57.80): VU0

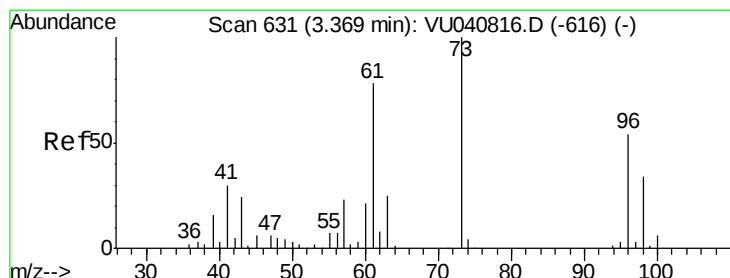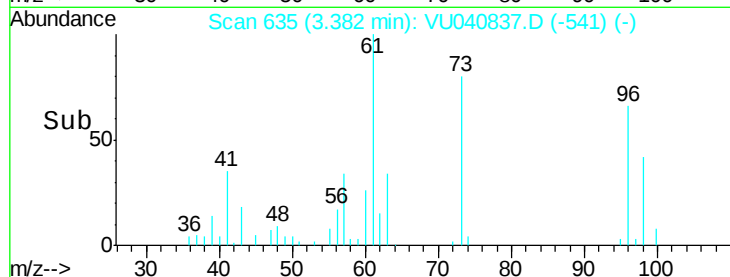
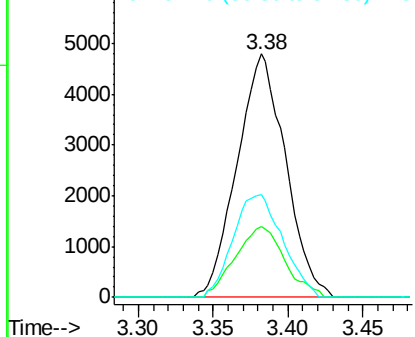



#18  
trans-1,2-Dichloroethene  
Concen: 1.293 ug/L  
RT: 3.37 min Scan# 631  
Delta R.T. 0.00 min  
Lab File: VU040837.D  
Acq: 20 Oct 2020 04:28

Tgt Ion: 96 Resp: 11039  
Ion Ratio Lower Upper  
96 100  
61 150.5 105.9 196.7  
98 65.9 43.8 81.3

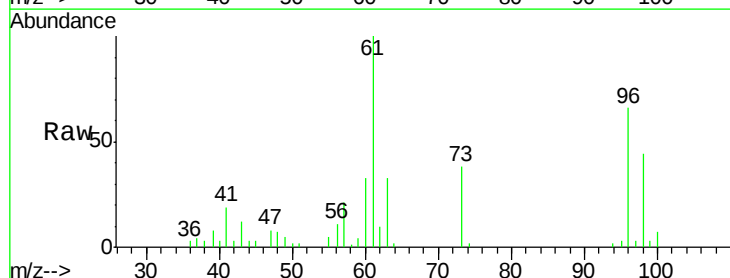

Abundance Ion 96.00 (95.70 to 96.70): VU0  
Ion 61.05 (60.75 to 61.75): VU0  
Ion 97.95 (97.65 to 98.65): VU0

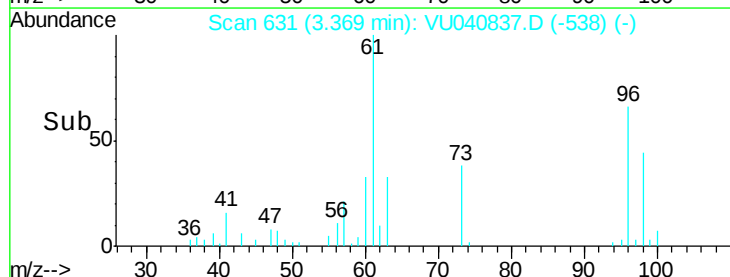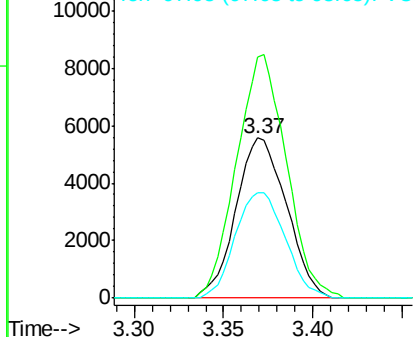

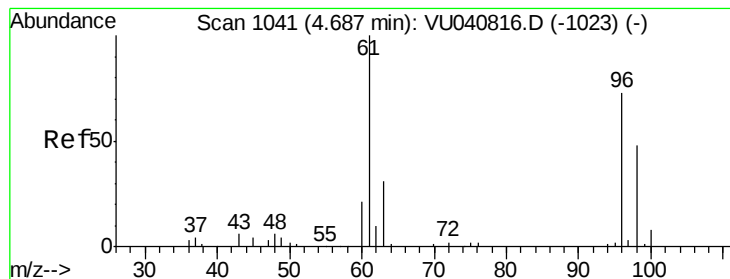

#22

cis-1,2-Dichloroethene

Concen: 95.660 ug/L

RT: 4.69 min Scan# 1041

Delta R.T. 0.00 min

Lab File: VU040837.D

Acq: 20 Oct 2020 04:28

Instrument :

MSVOA\_U

ClientSampleId :

ETZ34


Tot Ion: 96 Resp: 881027

Ion Ratio Lower Upper

96 100

61 141.0 99.8 185.4




68 0.0 0.0 0.0

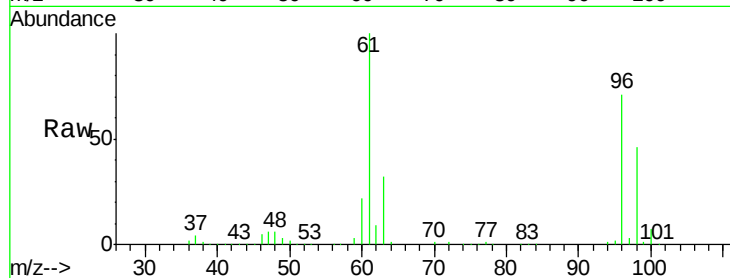

Abundance Ion 96.00 (95.70 to 96.70): VU040837.D (-948) (-)

Ion 61.05 (60.75 to 61.75): VU040837.D (-948) (-)

Ion 68.15 (67.85 to 68.85): VU040837.D (-948) (-)

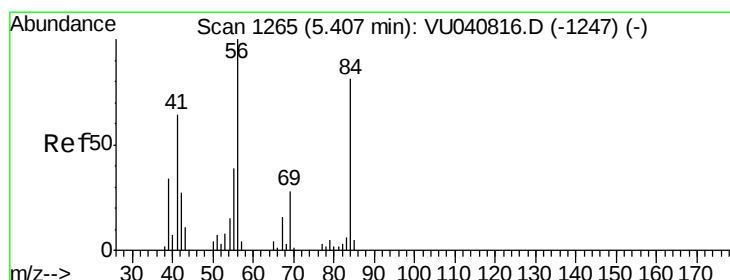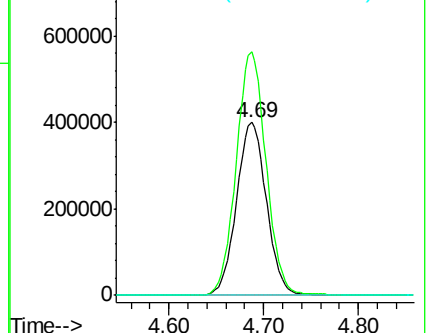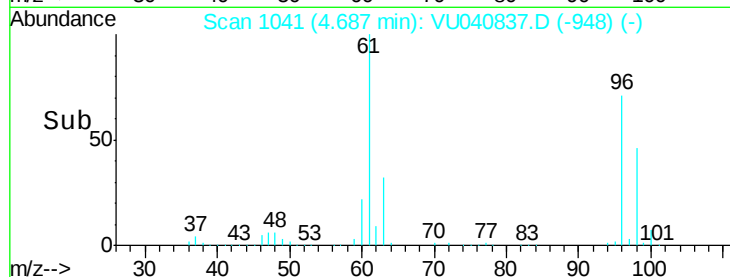

#30

Cyclohexane

Concen: 0.191 ug/L

RT: 5.40 min Scan# 1262

Delta R.T. -0.01 min

Lab File: VU040837.D

Acq: 20 Oct 2020 04:28


Tgt Ion: 56 Resp: 2743

Ion Ratio Lower Upper

56 100

69 32.5 23.8 35.8



84 78.1 64.0 96.0

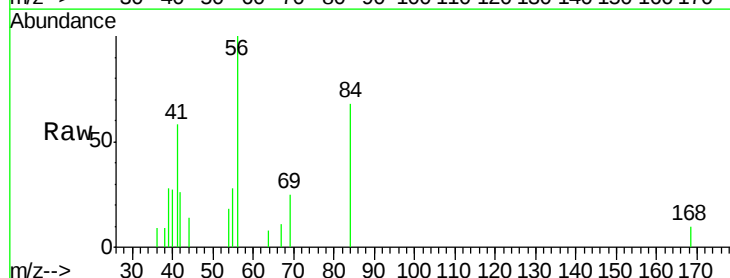


Abundance Ion 56.10 (55.80 to 56.80): VU040837.D (-1172) (-)

Ion 69.15 (68.85 to 69.85): VU040837.D (-1172) (-)

Ion 84.15 (83.85 to 84.85): VU040837.D (-1172) (-)

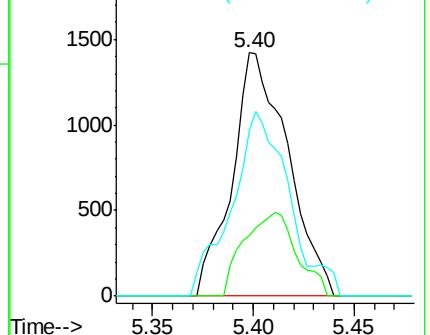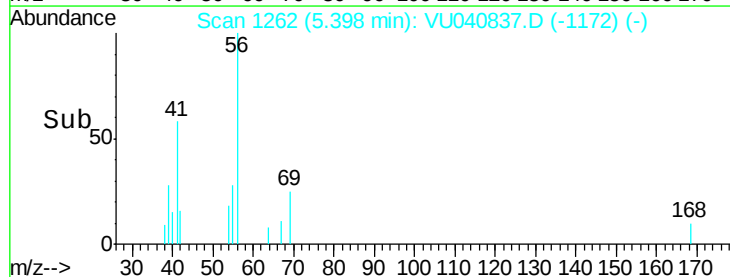


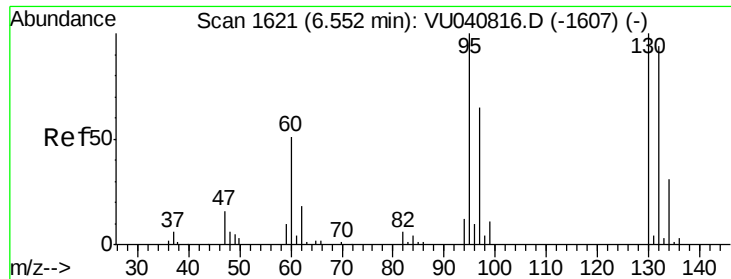




#34  
 Trichloroethene  
 Concen: 1.003 ug/L  
 RT: 6.56 min Scan# 1622  
 Delta R.T. 0.00 min  
 Lab File: VU040837.D  
 Acq: 20 Oct 2020 04:28

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 ETZ34

Tot Ion: 95 Resp: 9715  
 Ion Ratio Lower Upper  
 95 100  
 97 70.4 45.5 84.5  
 132 91.3 67.5 125.4  
 130 92.8 69.9 129.9

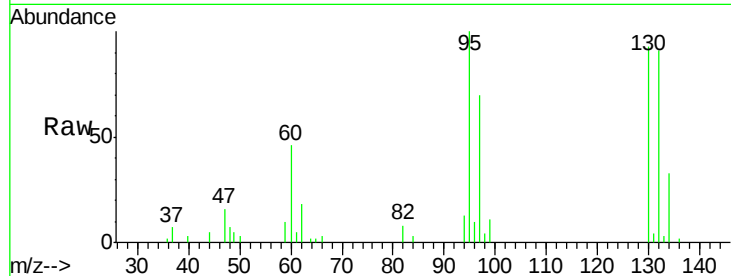


Abundance Ion 95.00 (94.70 to 95.70): VU0  
 Ion 96.95 (96.65 to 97.65): VU0  
 Ion 131.95 (131.65 to 132.65): V  
 Ion 129.95 (129.65 to 130.65): V

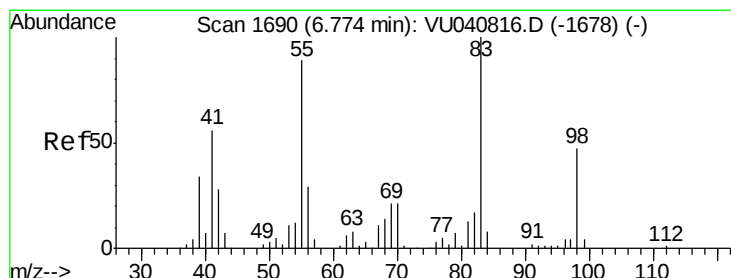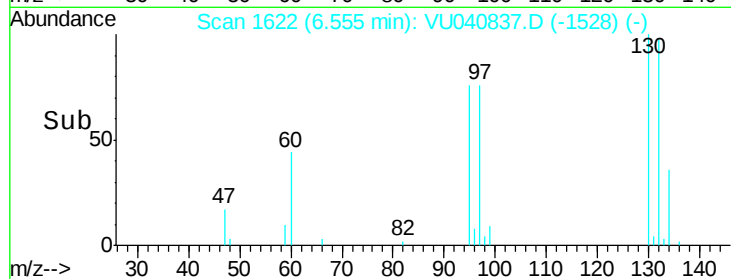
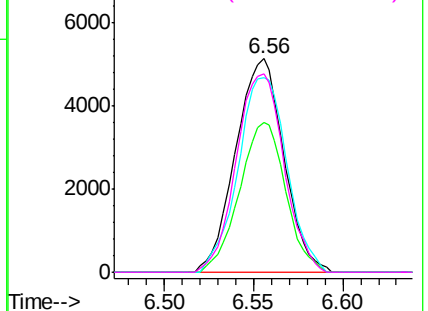



#35  
 Methylcyclohexane  
 Concen: 0.108 ug/L  
 RT: 6.77 min Scan# 1688  
 Delta R.T. -0.01 min  
 Lab File: VU040837.D  
 Acq: 20 Oct 2020 04:28

Tgt Ion: 83 Resp: 1480  
 Ion Ratio Lower Upper  
 83 100  
 55 52.1 70.7 106.1#  
 98 28.5 38.4 57.6#

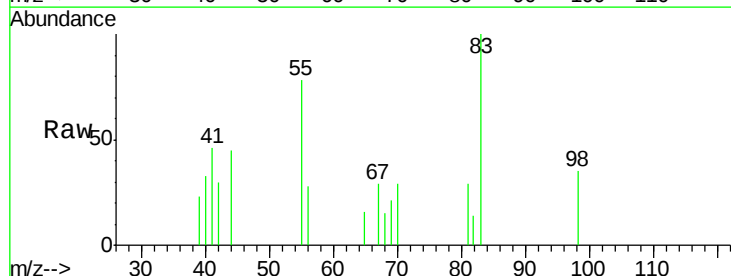

Abundance Ion 83.15 (82.85 to 83.85): VU0  
 Ion 55.10 (54.80 to 55.80): VU0  
 Ion 98.15 (97.85 to 98.85): VU0

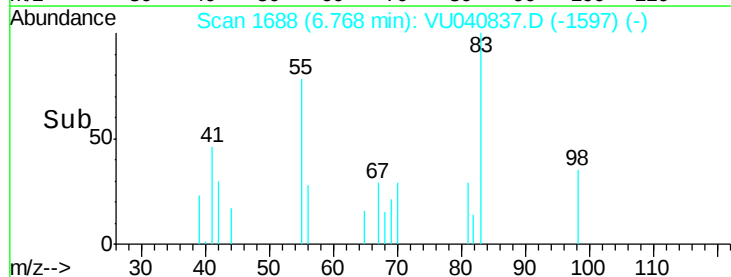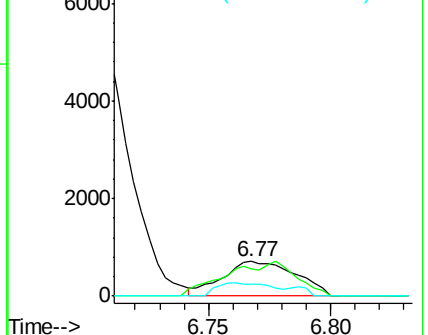

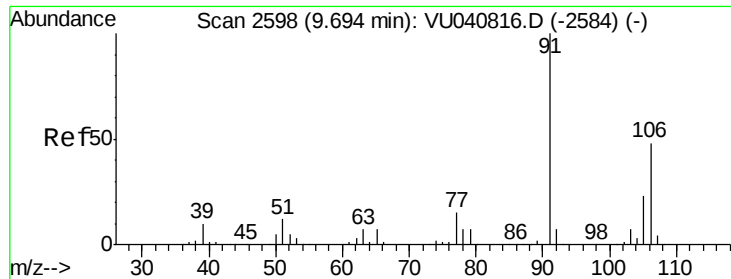

#53

m,p-Xylene

Concen: 0.135 ug/L

RT: 9.69 min Scan# 2598

Delta R.T. 0.00 min

Lab File: VU040837.D

Acq: 20 Oct 2020 04:28



Instrument :  
MSVOA\_U  
ClientSampleId :  
ETZ34

Tot Ion:106 Resp: 2032

Ion Ratio Lower Upper

106 100

91 193.9 148.5 275.7

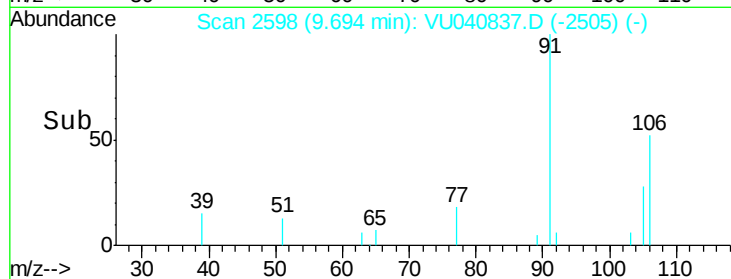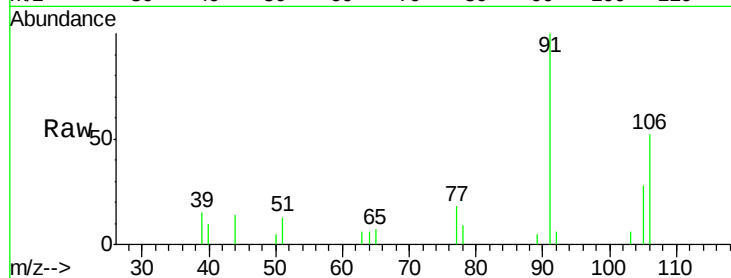

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VU0

