


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU101920\
 Data File : VU040791.D
 Acq On : 19 Oct 2020 09:24
 Operator : SY/MD
 Sample : BFB24
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB24

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Oct 20 05:12:18 2020

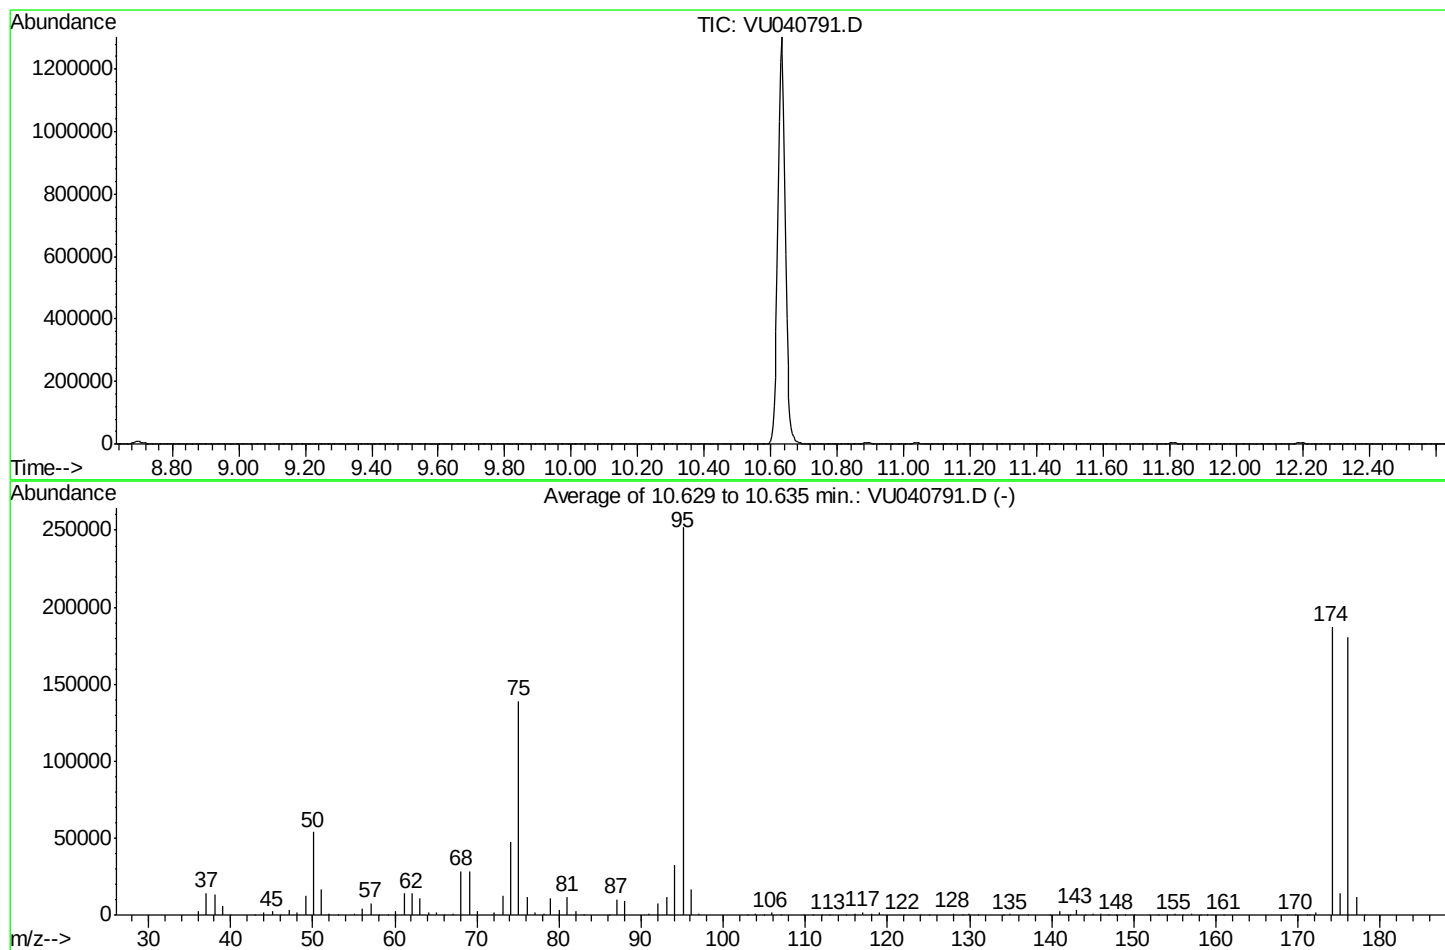

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	53757	PASS
75	95	30	80	55.3	139349	PASS
95	95	100	100	100.0	251946	PASS
96	95	5	9	6.7	16806	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.4	187498	PASS
175	174	5	9	7.7	14355	PASS
176	174	95	101	96.2	180330	PASS
177	176	5	9	6.6	11833	PASS

m/z	Abundance
36.10	2620.0
37.10	14716.0
38.00	12950.0
39.00	5765.0
40.00	303.0
42.90	143.0
44.00	2132.0
45.10	2253.0
46.10	322.0
47.10	3514.0
48.00	1803.0
49.10	11979.0
50.10	52736.0
51.10	17032.0
52.00	696.0
53.00	287.0
55.10	723.0
56.00	4431.0
57.10	7556.0
58.00	312.0
60.10	2663.0
61.10	13790.0
62.10	13728.0
63.10	11160.0
64.10	1752.0
65.10	1803.0
66.00	191.0
67.10	737.0
68.10	28312.0
69.10	27064.0
70.00	2044.0
72.10	1509.0
73.10	12082.0
74.10	46768.0
75.10	135424.0
76.10	11949.0
77.00	1761.0
78.00	731.0
79.00	10592.0
80.00	3351.0
81.00	11468.0
82.00	2544.0
83.00	346.0
86.10	422.0
87.00	10175.0
88.00	8377.0
91.00	1298.0
92.10	7862.0
93.10	11676.0
94.10	30672.0
95.10	245120.0
96.10	16984.0
97.00	451.0
102.90	139.0
103.90	1258.0
104.90	415.0
105.90	1402.0
106.90	299.0
109.80	137.0
111.00	128.0
112.00	241.0
112.90	323.0
115.00	327.0
116.00	1200.0
117.00	2056.0
118.00	1094.0
119.00	1729.0
124.00	110.0
125.10	111.0
128.00	783.0
129.10	338.0
129.90	797.0
131.00	421.0
134.90	496.0
137.00	436.0
139.80	182.0
141.00	2863.0
142.00	295.0
142.20	297.0
143.00	3594.0
144.00	225.0
145.10	914.0
146.00	525.0
146.90	203.0
147.90	453.0
148.90	138.0
150.00	289.0
151.80	163.0
153.10	128.0
155.00	471.0
157.00	385.0
159.00	311.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

161.10	250.0
171.00	437.0
172.10	1788.0
174.10	178816.0
175.10	13729.0
176.10	170752.0
177.10	11283.0
178.00	348.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.10	2727.0
37.10	14686.0
38.10	13668.0
39.00	5845.0
40.00	342.0
42.90	170.0
44.00	2231.0
45.10	2552.0
46.10	322.0
47.10	3605.0
48.00	1908.0
49.10	12747.0
50.10	55744.0
51.10	17536.0
52.00	822.0
53.10	249.0
55.00	793.0
56.00	4340.0
57.10	7983.0
58.00	353.0
59.10	125.0
60.10	2693.0
61.10	14351.0
62.10	14704.0
63.10	11495.0
64.10	1577.0
65.10	1693.0
66.00	159.0
67.10	797.0
68.10	29640.0
69.10	29160.0
70.00	2182.0
72.10	1566.0
73.10	13081.0
74.10	49392.0
75.10	144384.0
76.10	12544.0
77.00	1807.0
78.10	832.0
79.00	11407.0
80.00	3273.0
81.00	12141.0
82.00	2642.0
83.00	305.0
86.10	364.0
87.00	10849.0
88.00	9083.0
91.00	1259.0
92.10	8256.0
93.10	12107.0
94.10	33408.0
95.10	260800.0
96.10	17560.0
97.00	462.0
102.90	136.0
104.00	1301.0
104.90	420.0
105.90	1453.0
106.90	301.0
109.80	151.0
110.80	153.0
112.00	290.0
112.90	276.0
115.00	320.0
116.00	1308.0
117.00	2108.0
118.00	1231.0
119.00	1831.0
122.00	137.0
124.00	171.0
125.10	103.0
128.00	956.0
129.00	390.0
130.00	888.0
131.00	430.0
134.10	107.0
135.00	591.0
137.00	435.0
139.70	170.0
141.00	2975.0
141.90	255.0
143.00	3747.0
144.00	232.0
145.10	876.0
146.00	550.0
146.90	221.0
147.90	432.0
149.00	164.0
150.00	252.0
151.80	135.0
153.00	159.0
154.00	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

155.00	538.0
155.90	116.0
157.00	474.0
158.10	105.0
158.90	338.0
161.00	270.0
169.70	120.0
171.30	404.0
172.10	2059.0
174.10	194240.0
175.10	14813.0
176.10	186496.0
177.10	12199.0
178.10	382.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.10	2627.0
37.00	13345.0
38.10	12769.0
39.00	5199.0
40.10	369.0
43.00	156.0
44.00	2004.0
45.10	2476.0
46.10	300.0
47.10	3396.0
48.00	1829.0
49.10	12027.0
50.10	52792.0
51.10	16392.0
52.00	807.0
53.10	187.0
55.00	867.0
56.10	4053.0
57.10	7615.0
58.00	338.0
59.10	107.0
60.10	2532.0
61.10	13475.0
62.10	13571.0
63.10	10873.0
64.00	1279.0
65.10	1448.0
66.10	161.0
67.10	788.0
68.10	27728.0
69.10	28272.0
70.00	2122.0
72.00	1418.0
73.10	12686.0
74.10	46776.0
75.10	138240.0
76.10	11741.0
77.00	1558.0
78.20	891.0
79.00	11153.0
80.00	2874.0
81.00	11519.0
82.00	2511.0
83.00	242.0
86.20	280.0
87.00	10112.0
88.00	9042.0
91.00	1121.0
92.10	7458.0
93.10	11437.0
94.10	32384.0
95.10	249920.0
96.10	15875.0
97.10	471.0
102.90	138.0
104.00	1267.0
104.90	385.0
105.90	1367.0
107.00	250.0
109.90	172.0
110.90	188.0
111.90	251.0
112.90	198.0
115.00	288.0
116.00	1174.0
117.00	1967.0
118.00	1226.0
119.00	1634.0
121.90	127.0
124.00	241.0
128.00	1080.0
129.00	427.0
130.00	869.0
131.00	398.0
135.00	576.0
137.00	432.0
139.80	170.0
141.00	2706.0
142.00	232.0
143.00	3500.0
144.10	201.0
145.00	794.0
146.00	490.0
146.90	190.0
147.90	414.0
149.00	158.0
150.00	222.0
151.90	113.0
153.00	170.0
154.00	108.0
155.00	590.0
155.90	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

157.00	527.0
158.90	312.0
160.90	299.0
169.70	124.0
171.30	383.0
172.10	2070.0
174.10	189440.0
175.10	14524.0
176.10	183744.0
177.10	12017.0
178.10	357.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

Scan 2874 (10.581 min): VU040791.D
BFB24

m/z	Abundance
40.00	103.0
43.90	242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24