


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101921\
 Data File : VU045324.D
 Acq On : 19 Oct 2021 11:36
 Operator : SY/MD
 Sample : BFB013
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB013

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101921WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 21 01:57:14 2021

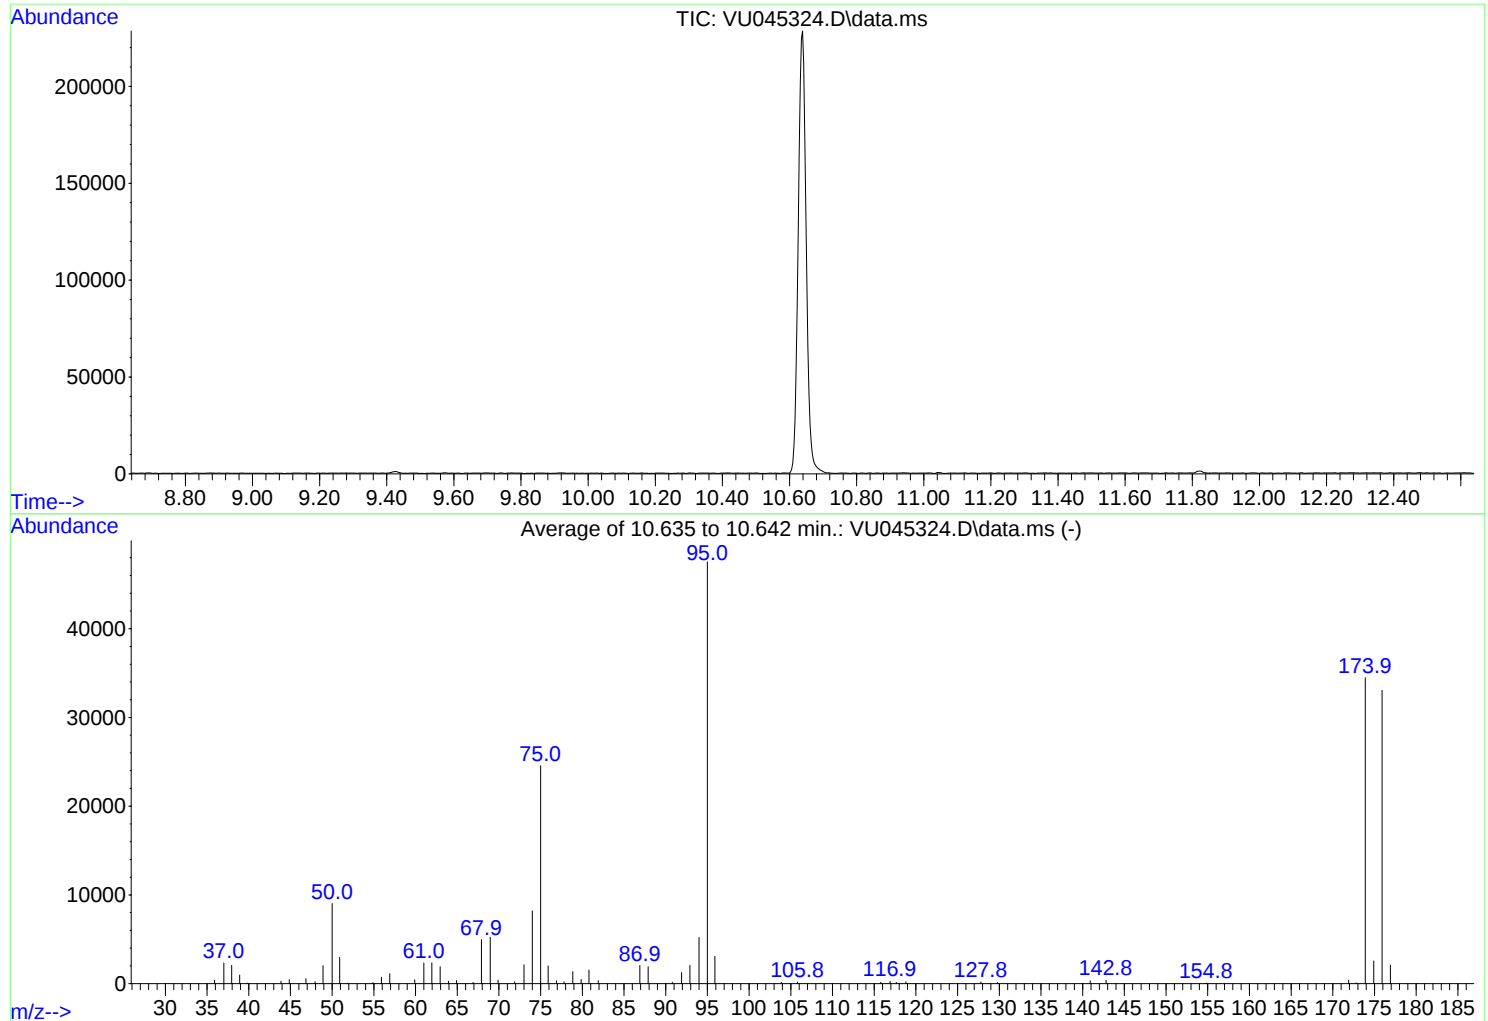

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	9043	PASS
75	95	30	80	51.7	24565	PASS
95	95	100	100	100.0	47544	PASS
96	95	5	9	6.5	3069	PASS
173	174	0.00	2	0.3	88	PASS
174	95	50	120	72.5	34477	PASS
175	174	5	9	7.4	2560	PASS
176	174	95	101	95.9	33064	PASS
177	176	5	9	6.3	2079	PASS

m/z	Abundance
35.90	330.0
37.00	2184.0
37.90	1943.0
38.90	927.0
39.80	200.0
43.90	550.0
44.80	367.0
46.80	516.0
47.90	209.0
48.90	1879.0
50.00	8572.0
50.90	2808.0
54.90	100.0
55.90	700.0
56.90	1141.0
59.90	401.0
61.00	2166.0
62.00	2225.0
62.90	1714.0
64.00	244.0
64.90	394.0
66.90	137.0
67.90	4797.0
69.00	5018.0
69.90	397.0
71.90	192.0
73.00	2021.0
74.00	7669.0
75.00	23512.0
75.90	1850.0
76.90	384.0
77.80	204.0
78.80	1329.0
79.80	441.0
80.80	1444.0
81.90	320.0
86.90	1915.0
87.90	1862.0
90.80	141.0
91.90	1163.0
92.90	1925.0
94.00	4891.0
95.00	44864.0
95.90	2957.0
103.90	140.0
105.80	189.0
115.80	153.0
116.90	281.0
117.70	146.0
118.80	196.0
127.80	182.0
129.80	126.0
140.90	315.0
142.80	372.0
171.90	374.0
172.80	263.0
173.90	33648.0
174.90	2456.0
175.90	32160.0
176.90	1995.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

Scan 2879 (10.597 min): VU045324.D\data.ms
BFB013

m/z	Abundance
39.90	135.0
43.90	278.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.90	457.0
37.00	2390.0
38.00	2117.0
38.90	977.0
39.80	202.0
43.80	539.0
44.90	529.0
46.90	560.0
47.90	206.0
48.90	2105.0
50.00	9291.0
50.90	3037.0
51.80	103.0
54.90	134.0
55.90	738.0
56.90	1067.0
59.90	445.0
61.00	2398.0
61.90	2415.0
63.00	2056.0
63.90	305.0
64.90	316.0
66.90	144.0
67.90	4972.0
68.90	5219.0
69.90	399.0
71.90	223.0
73.00	2168.0
74.00	8455.0
75.00	24832.0
75.90	2102.0
76.90	255.0
77.80	212.0
78.90	1367.0
79.80	499.0
80.80	1565.0
81.90	370.0
86.90	2116.0
87.90	1928.0
90.80	171.0
91.90	1324.0
92.90	2132.0
94.00	5407.0
95.00	48680.0
95.90	3082.0
97.00	108.0
103.80	172.0
105.80	173.0
115.80	174.0
116.90	245.0
117.70	132.0
118.80	238.0
127.80	194.0
129.80	110.0
140.90	358.0
142.80	390.0
154.80	120.0
171.90	417.0
173.90	34232.0
174.90	2574.0
175.90	32984.0
176.90	2090.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013

m/z	Abundance
35.90	398.0
37.00	2422.0
37.90	2133.0
38.90	1017.0
39.80	222.0
43.90	557.0
44.90	462.0
46.80	580.0
48.00	215.0
48.90	2067.0
50.00	9266.0
50.90	3031.0
51.90	100.0
54.90	130.0
55.90	742.0
56.90	1134.0
59.90	441.0
61.00	2400.0
61.90	2416.0
62.90	1942.0
63.90	283.0
64.90	349.0
66.90	149.0
67.90	5164.0
68.90	5477.0
69.90	422.0
71.90	210.0
73.00	2205.0
74.00	8483.0
75.00	25352.0
75.90	2063.0
76.90	315.0
77.80	234.0
78.80	1379.0
79.90	496.0
80.80	1575.0
81.90	349.0
86.90	2113.0
87.90	1960.0
90.80	159.0
91.90	1268.0
92.90	2106.0
94.00	5362.0
95.00	49088.0
95.90	3167.0
103.90	169.0
105.80	195.0
115.80	178.0
116.90	275.0
117.60	141.0
118.80	217.0
127.80	206.0
129.80	128.0
140.90	327.0
142.80	391.0
154.80	102.0
171.90	416.0
173.90	35552.0
174.90	2651.0
175.90	34048.0
176.90	2152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB013