

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101922\
 Data File : VU051449.D
 Acq On : 19 Oct 2022 10:44
 Operator : JC/MD
 Sample : VU1019WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1019WBL01

Quant Time: Oct 20 07:12:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Oct 18 04:53:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.115	96	48167	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.632	95	12386	0.733	ug/l	0.00
Spiked Amount 1.000			Recovery	=	73.000%	
68) 1,2-Dichlorobenzene-d4	12.192	152	14741	0.781	ug/l	0.00
Spiked Amount 1.000			Recovery	=	78.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101922\
Data File : VU051449.D
Acq On : 19 Oct 2022 10:44
Operator : JC/MD
Sample : VU1019WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1019WBL01

Quant Time: Oct 20 07:12:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Oct 18 04:53:19 2022
Response via : Initial Calibration




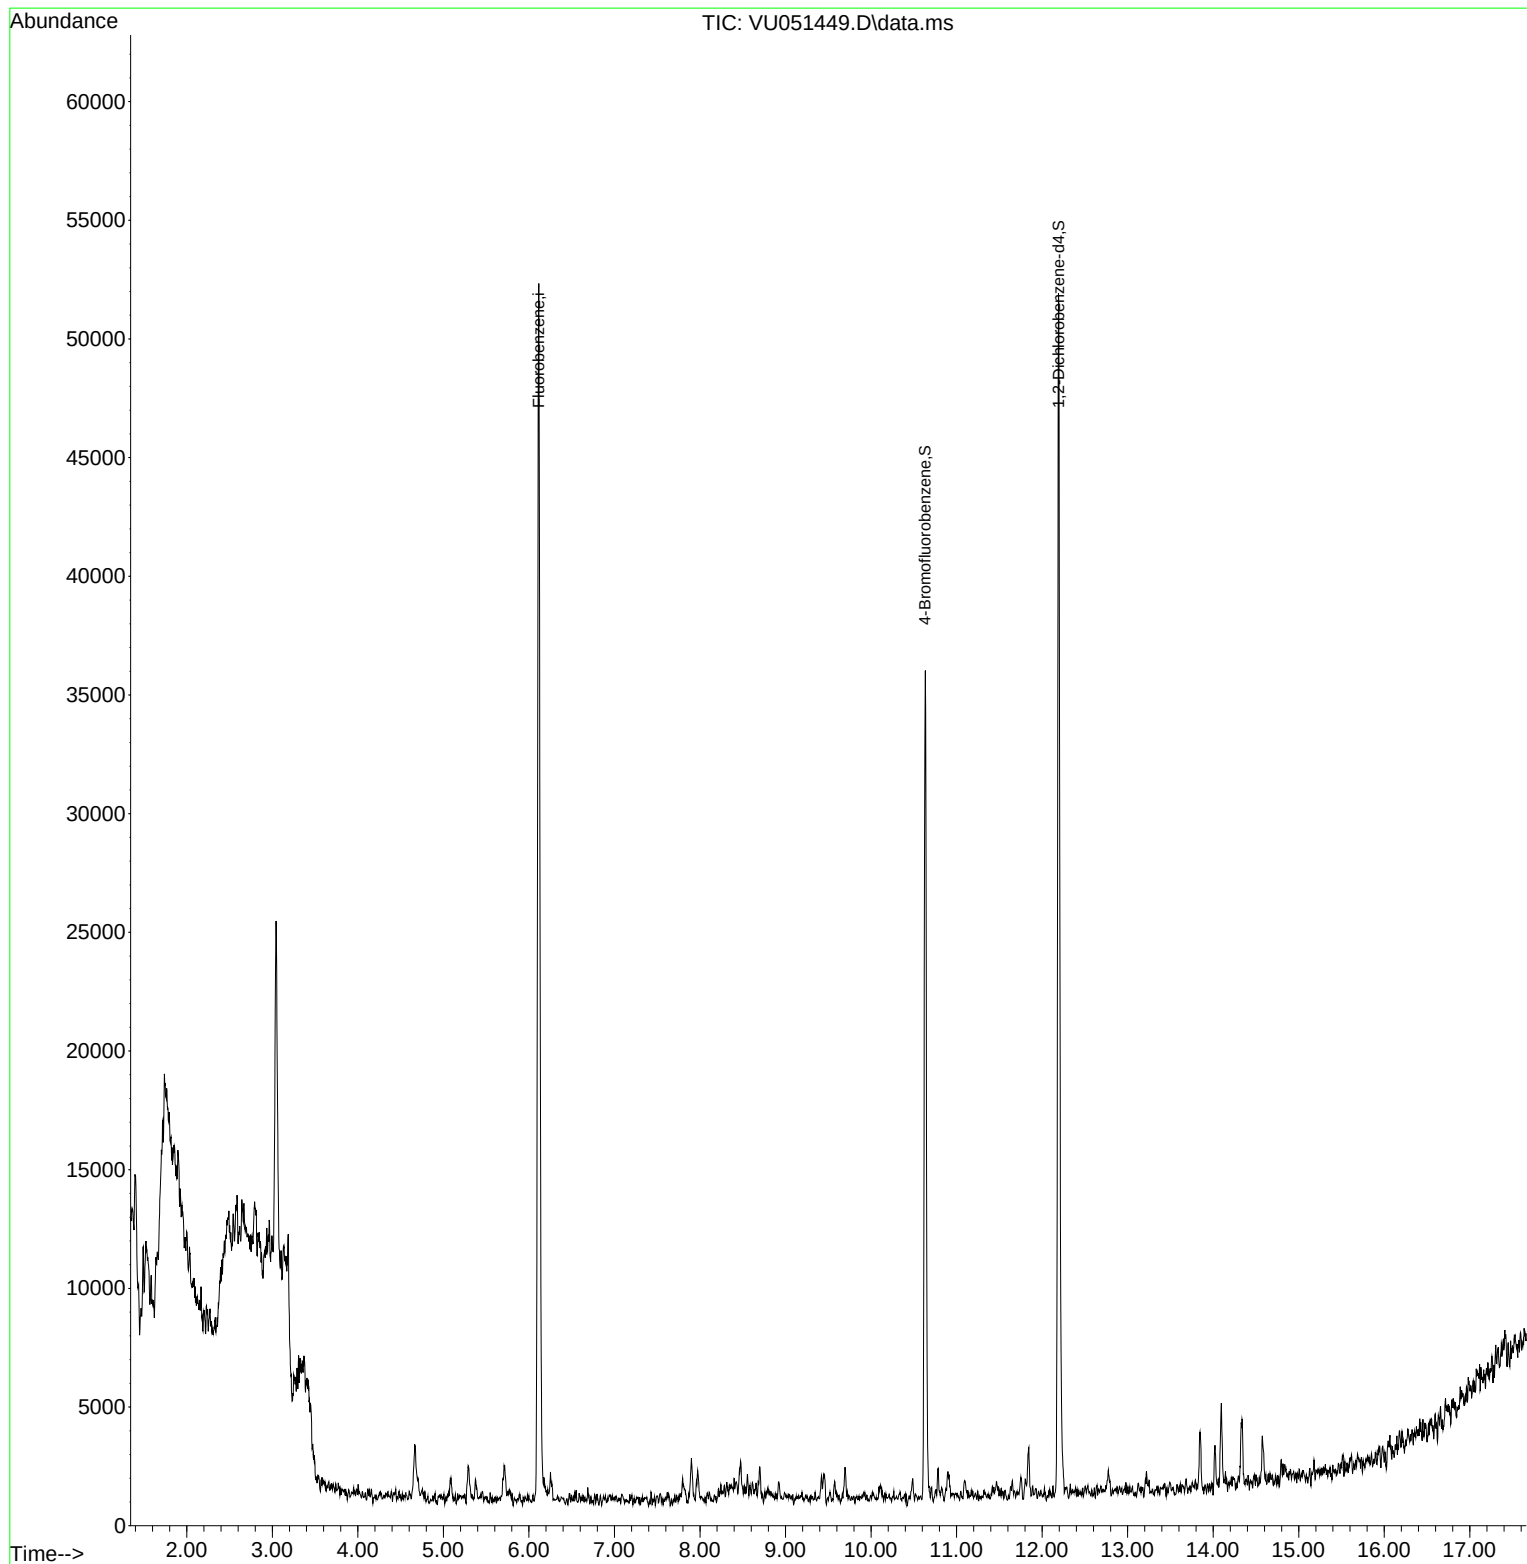


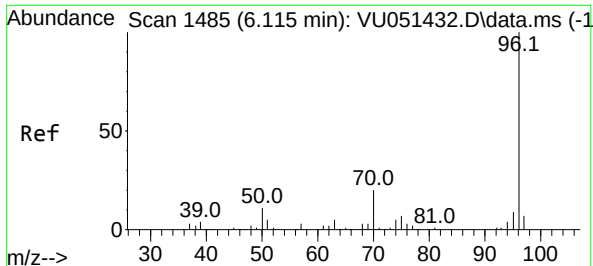

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.115 min Scan# 1485
Delta R.T. -0.000 min
Lab File: VU051449.D
Acq: 19 Oct 2022 10:44




Instrument :
MSVOA_U
ClientSampleId :
VU1019WBL01


Tgt Ion:	96	Resp:	48167
Ion	Ratio	Lower	Upper
96	100		
70	19.4	16.7	25.1
95	9.2	7.5	11.3
97	5.7	0.0	0.0

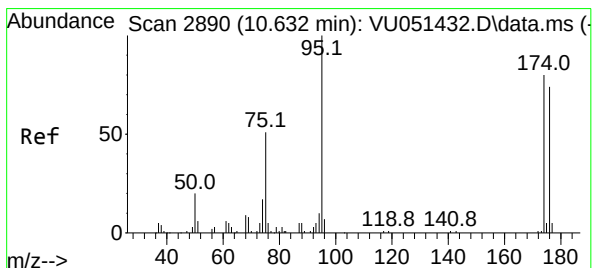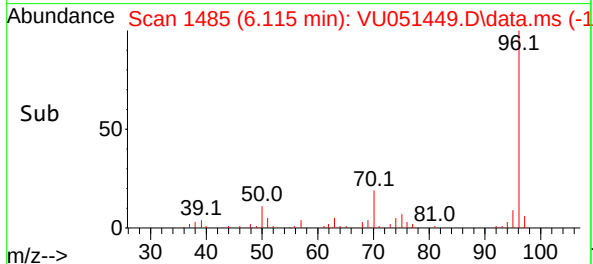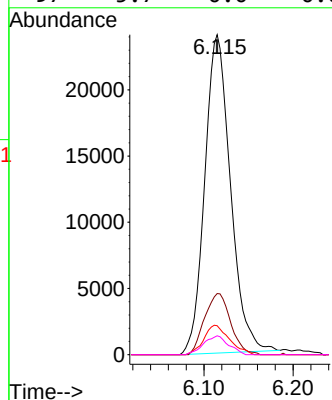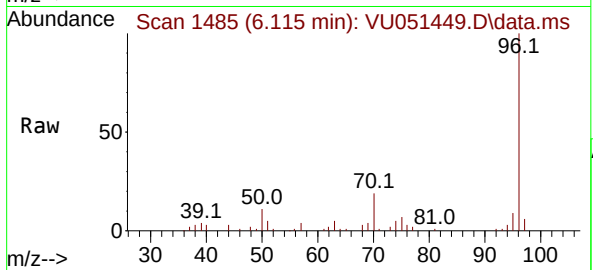

#57
4-Bromofluorobenzene
Concen: 0.733 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.000 min
Lab File: VU051449.D
Acq: 19 Oct 2022 10:44


Tgt Ion:	95	Resp:	12386
Ion	Ratio	Lower	Upper
95	100		
174	87.6	63.0	94.6
176	79.3	59.8	89.6

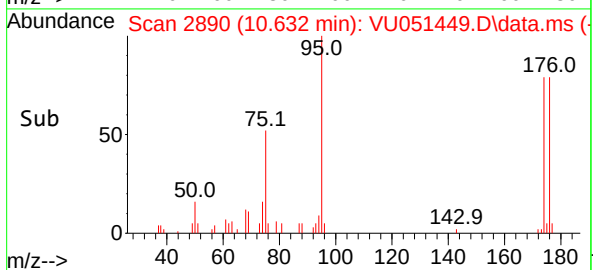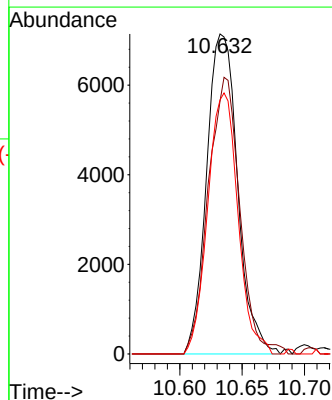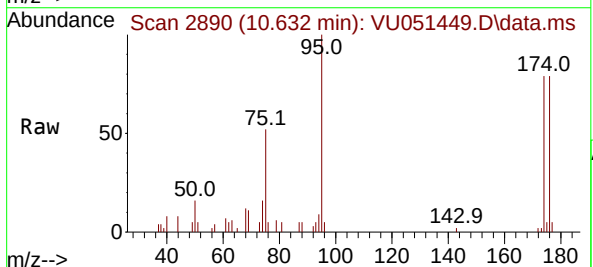

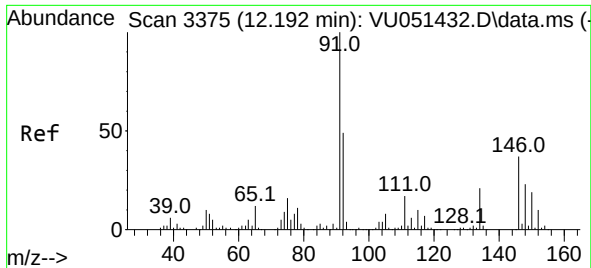

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.781 ug/l
 RT: 12.192 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VU051449.D
 Acq: 19 Oct 2022 10:44

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1019WBL01

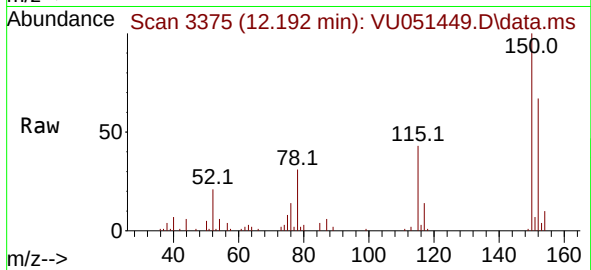

Tgt Ion:152	Resp:	14741
Ion	Ratio	Lower Upper
152	100	
115	65.4	0.0 333.0
150	159.0	0.0 662.0

