

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101922\
 Data File : VU051449.D
 Acq On : 19 Oct 2022 10:44
 Operator : JC/MD
 Sample : VU1019WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1019WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU051449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.044	522	530	545	rVB3	14614	28472	28.14%	8.662%
2	4.665	1021	1034	1044	rBV4	2303	5071	5.01%	1.543%
3	5.288	1221	1228	1229	rBV3	1562	1564	1.55%	0.476%
4	5.710	1356	1359	1369	rVB5	1270	1820	1.80%	0.554%
5	6.115	1468	1485	1502	rBV	51309	101169	100.00%	30.777%
6	7.899	2032	2040	2047	rBV2	1634	2332	2.31%	0.709%
7	7.973	2060	2063	2074	rVB3	1225	1547	1.53%	0.471%
8	8.475	2216	2219	2229	rVB4	1398	1659	1.64%	0.505%
9	8.697	2285	2288	2294	rVB3	1148	1186	1.17%	0.361%
10	9.420	2506	2513	2516	rBV2	978	1074	1.06%	0.327%
11	9.697	2591	2599	2605	rBV4	1314	1807	1.79%	0.550%
12	10.488	2835	2845	2851	rVB3	963	1619	1.60%	0.493%
13	10.635	2878	2891	2906	rBV3	34925	59693	59.00%	18.160%
14	10.783	2932	2937	2945	rVB3	1187	1301	1.29%	0.396%
15	11.095	3028	3034	3042	rBV4	770	1390	1.37%	0.423%
16	11.751	3231	3238	3245	rVB5	933	1447	1.43%	0.440%
17	11.803	3248	3254	3259	rBV6	842	1237	1.22%	0.376%
18	11.844	3260	3267	3272	rVB6	1704	2265	2.24%	0.689%
19	12.192	3359	3375	3396	rBV2	50715	90202	89.16%	27.441%
20	13.844	3881	3889	3899	rVB7	2407	3738	3.69%	1.137%
21	14.021	3937	3944	3952	rBV7	2111	3208	3.17%	0.976%
22	14.095	3958	3967	3977	rBV2	3559	5463	5.40%	1.662%
23	14.327	4032	4039	4041	rBV4	2501	2424	2.40%	0.737%
24	14.574	4112	4116	4127	rVB3	1856	2585	2.56%	0.786%
25	14.796	4178	4185	4189	rBV2	1155	1423	1.41%	0.433%
26	15.983	4547	4554	4560	rBV7	901	1385	1.37%	0.421%
27	16.047	4567	4574	4577	rBV5	1191	1631	1.61%	0.496%




Sum of corrected areas: 328712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101922\
Data File : VU051449.D
Acq On : 19 Oct 2022 10:44
Operator : JC/MD
Sample : VU1019WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1019WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

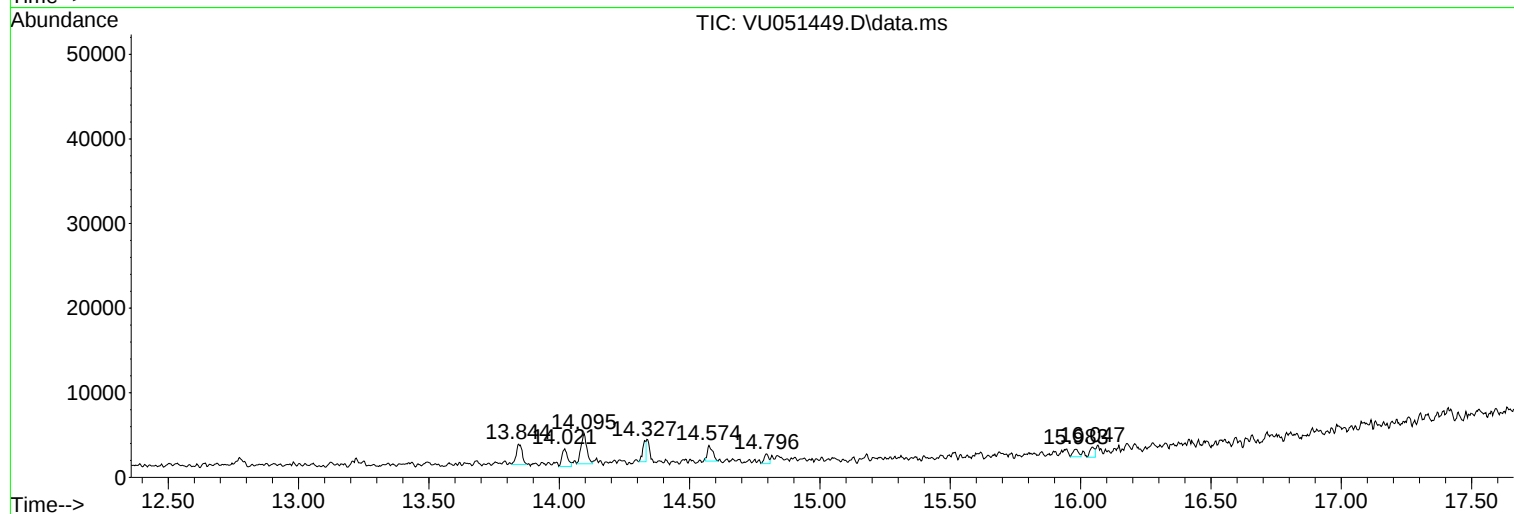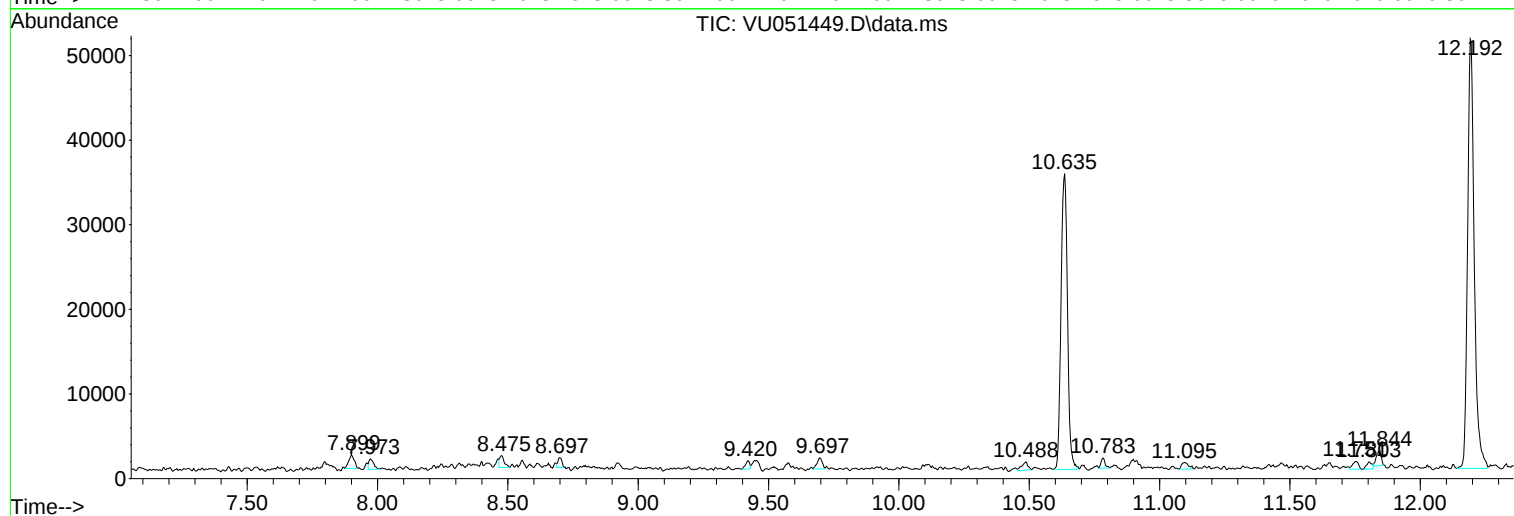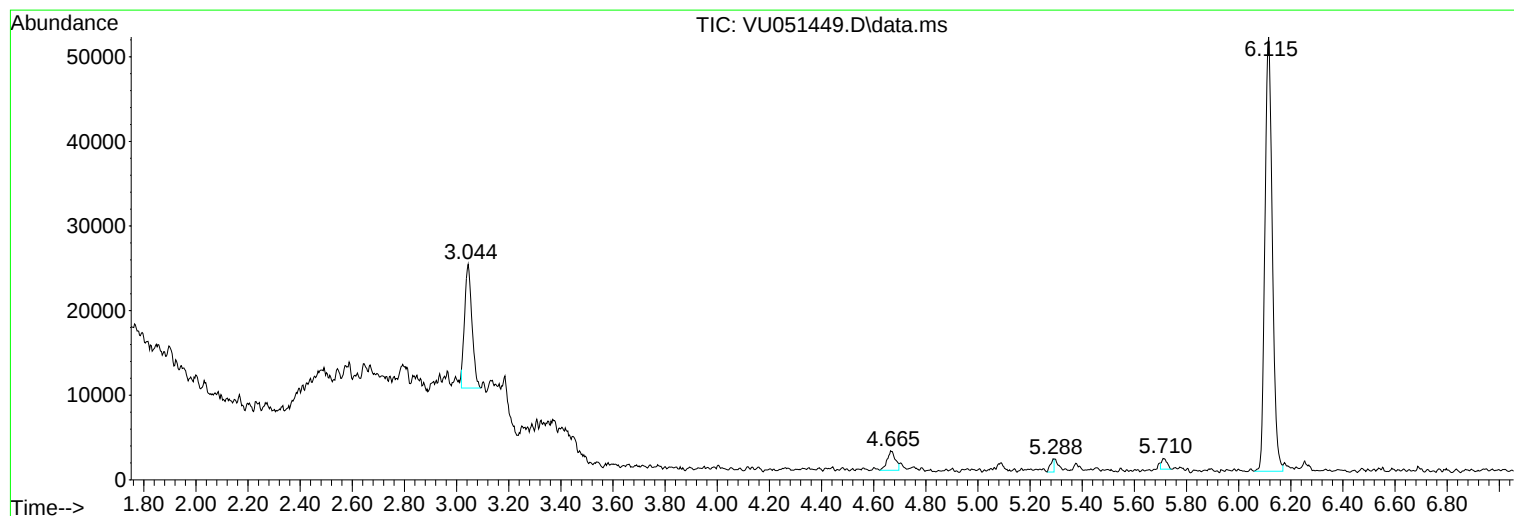

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101922\
Data File : VU051449.D
Acq On : 19 Oct 2022 10:44
Operator : JC/MD
Sample : VU1019WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1019WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101922\
Data File : VU051449.D
Acq On : 19 Oct 2022 10:44
Operator : JC/MD
Sample : VU1019WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1019WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------