
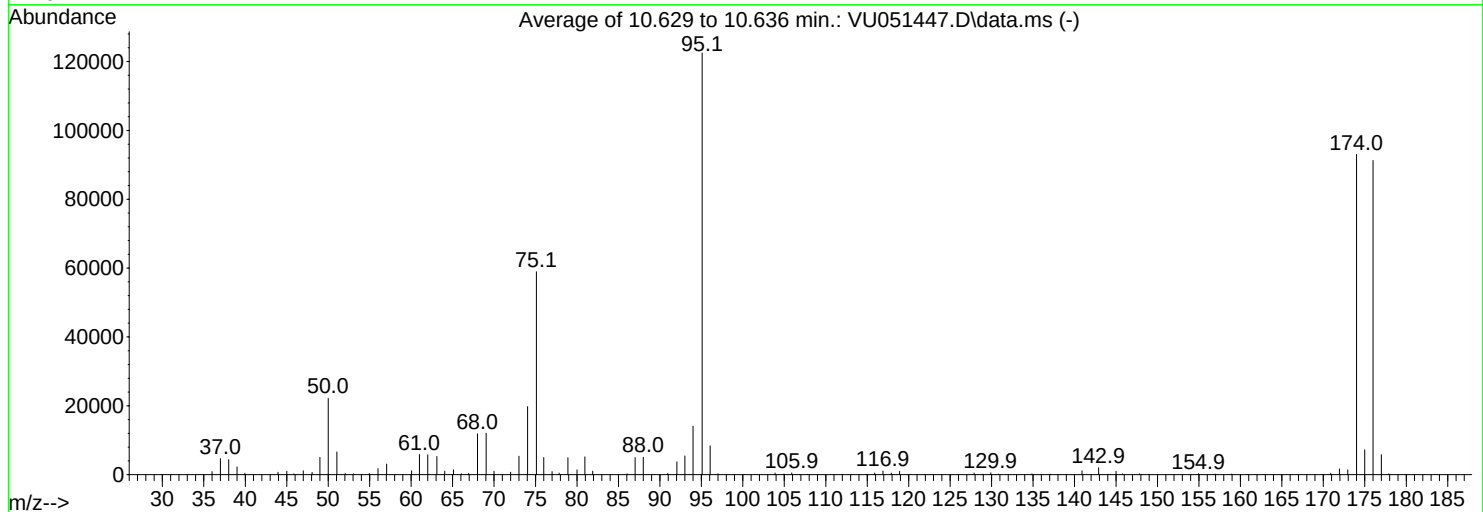


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101922\
Data File : VU051447.D
Acq On : 19 Oct 2022 09:14
Operator : JC/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101722DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Oct 18 04:53:19 2022

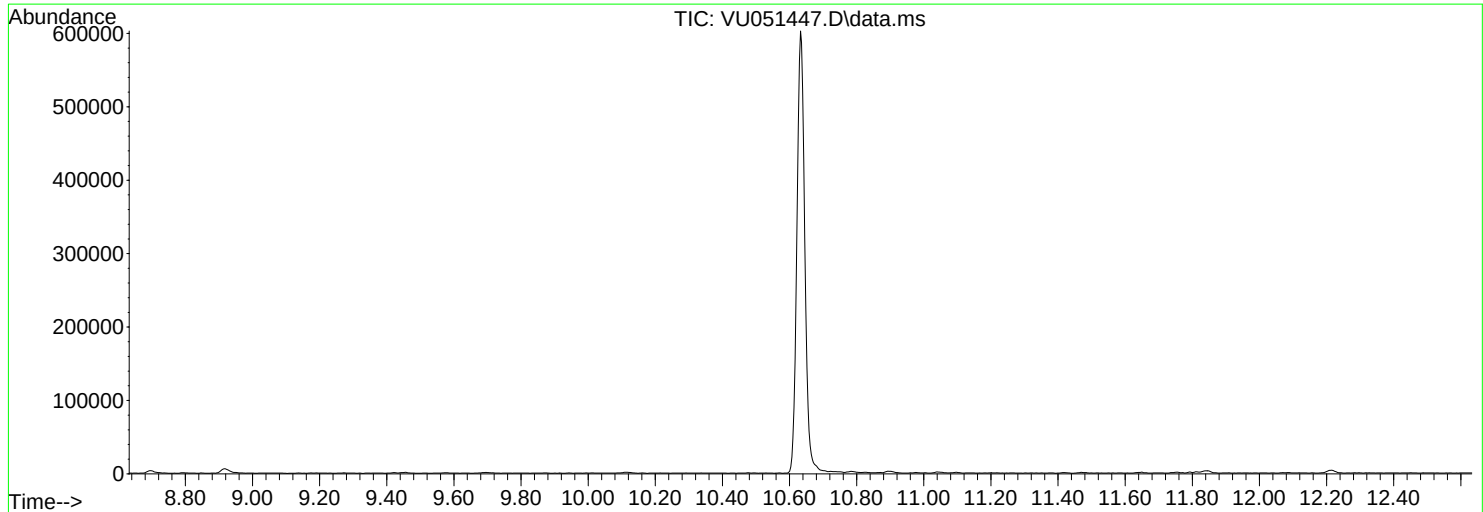

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	22179	PASS
75	95	30	60	48.1	58928	PASS
95	95	100	100	100.0	122533	PASS
96	95	5	9	6.8	8390	PASS
173	174	0.00	2	1.5	1397	PASS
174	95	50	100	75.9	93024	PASS
175	174	5	9	7.8	7216	PASS
176	174	95	101	98.2	91315	PASS
177	176	5	9	6.4	5809	PASS