

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101923\
 Data File : VU055809.D
 Acq On : 19 Oct 2023 10:51
 Operator : MD/SY
 Sample : VU1019WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK13

Quant Time: Oct 20 01:37:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101823DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Oct 19 03:10:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.113	96	73373	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	24401	0.843	ug/l	0.00
Spiked Amount	1.000		Recovery	=	84.000%	
68) 1,2-Dichlorobenzene-d4	12.193	152	21184	0.790	ug/l	0.00
Spiked Amount	1.000		Recovery	=	79.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101923\
Data File : VU055809.D
Acq On : 19 Oct 2023 10:51
Operator : MD/SY
Sample : VU1019WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK13

Quant Time: Oct 20 01:37:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101823DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Oct 19 03:10:04 2023
Response via : Initial Calibration




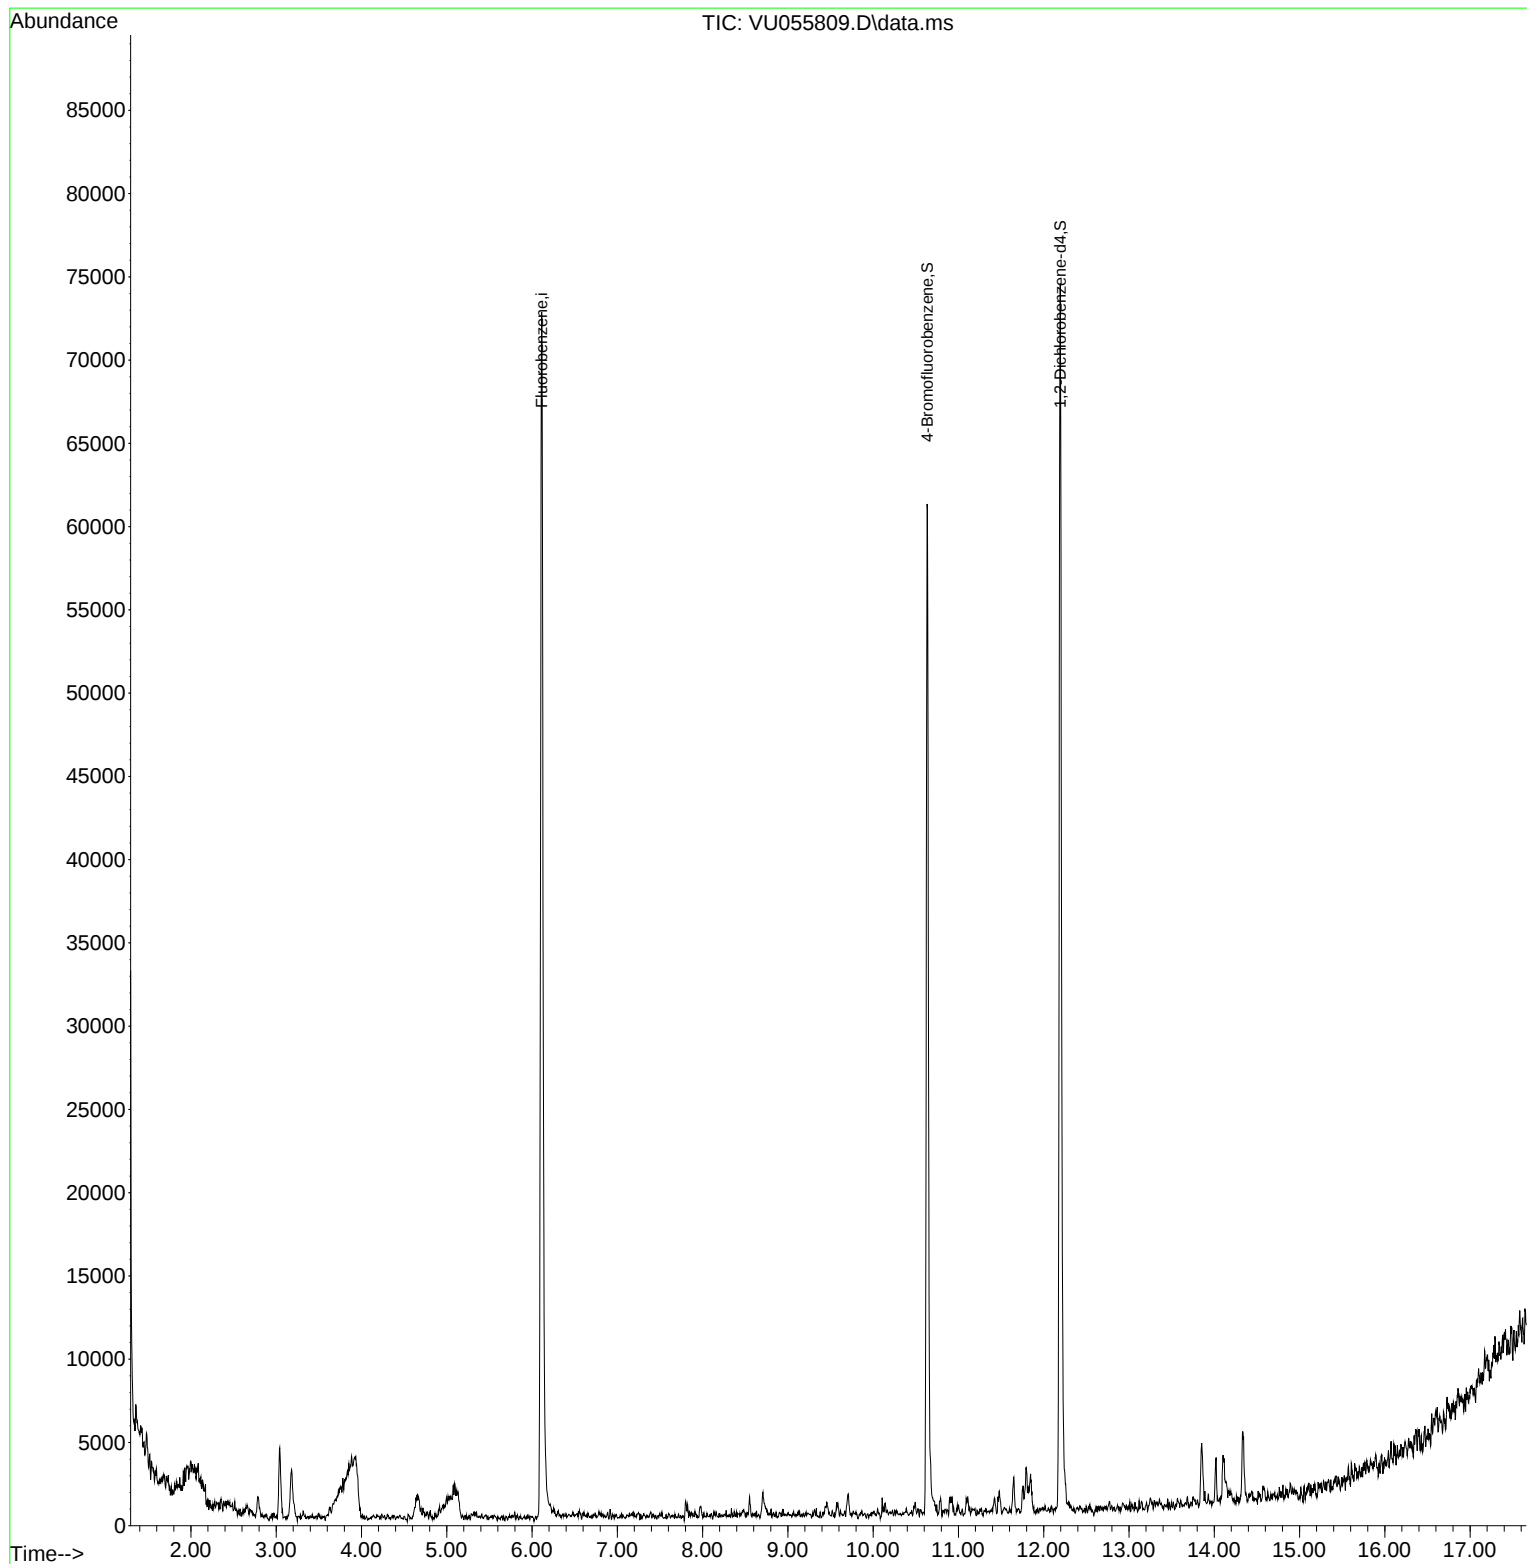


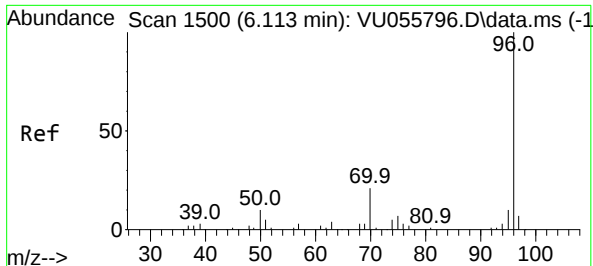

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.113 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU055809.D
Acq: 19 Oct 2023 10:51




Instrument :
MSVOA_U
ClientSampleId :
VBLK13


Tgt Ion: 96	Resp: 73373
Ion Ratio	Lower Upper
96 100	
70 20.5	16.5 24.7
95 8.9	7.4 11.0
97 5.9	0.0 0.0

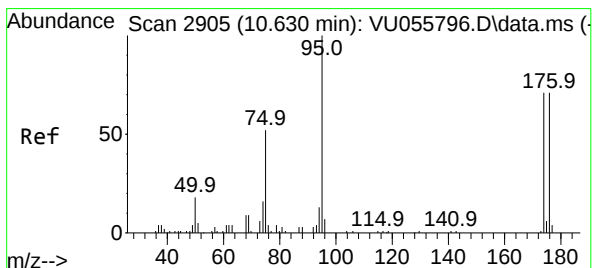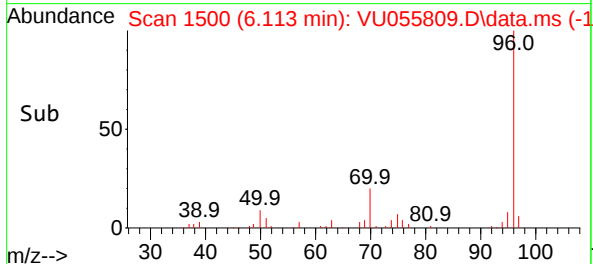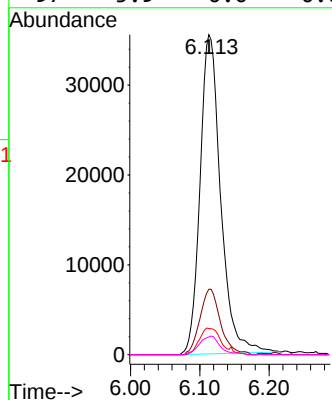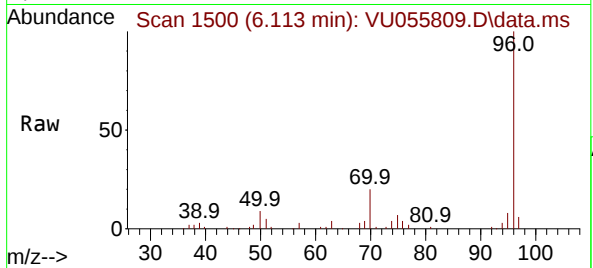

#57
4-Bromofluorobenzene
Concen: 0.843 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.004 min
Lab File: VU055809.D
Acq: 19 Oct 2023 10:51


Tgt Ion: 95	Resp: 24401
Ion Ratio	Lower Upper
95 100	
174 75.3	63.3 94.9
176 69.6	59.3 88.9

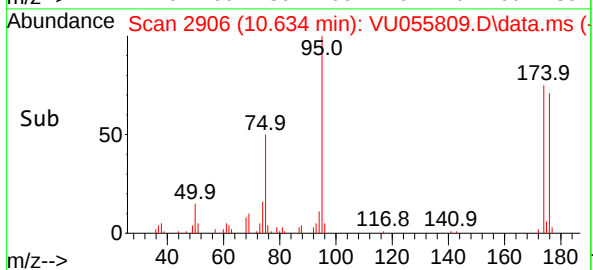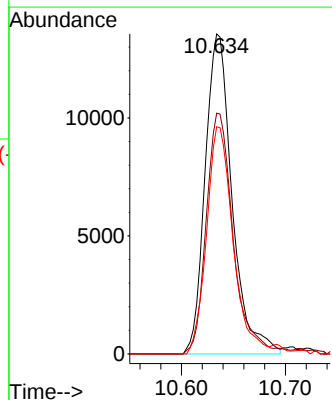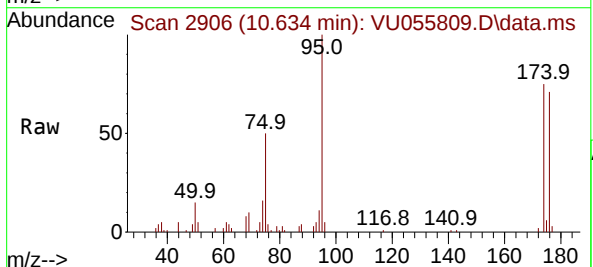

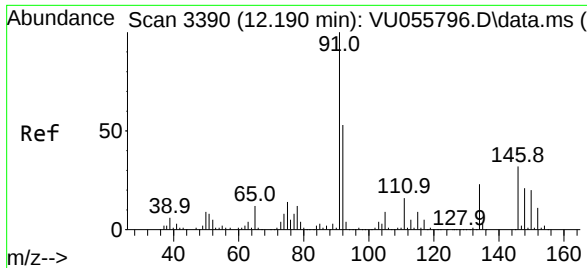

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.790 ug/l
 RT: 12.193 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU055809.D
 Acq: 19 Oct 2023 10:51

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK13

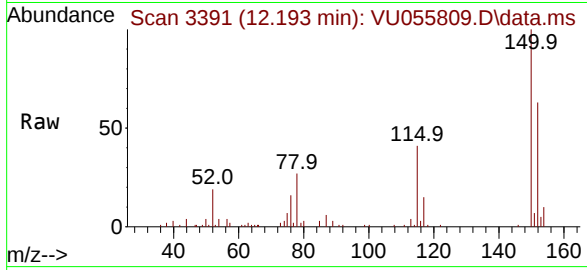

Tgt Ion:152	Resp:	21184
Ion	Ratio	Lower Upper
152	100	
115	69.2	0.0 308.8
150	160.5	0.0 635.0

