


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101923\
Data File : VU055807.D
Acq On : 19 Oct 2023 09:01
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101823DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Oct 19 03:10:04 2023

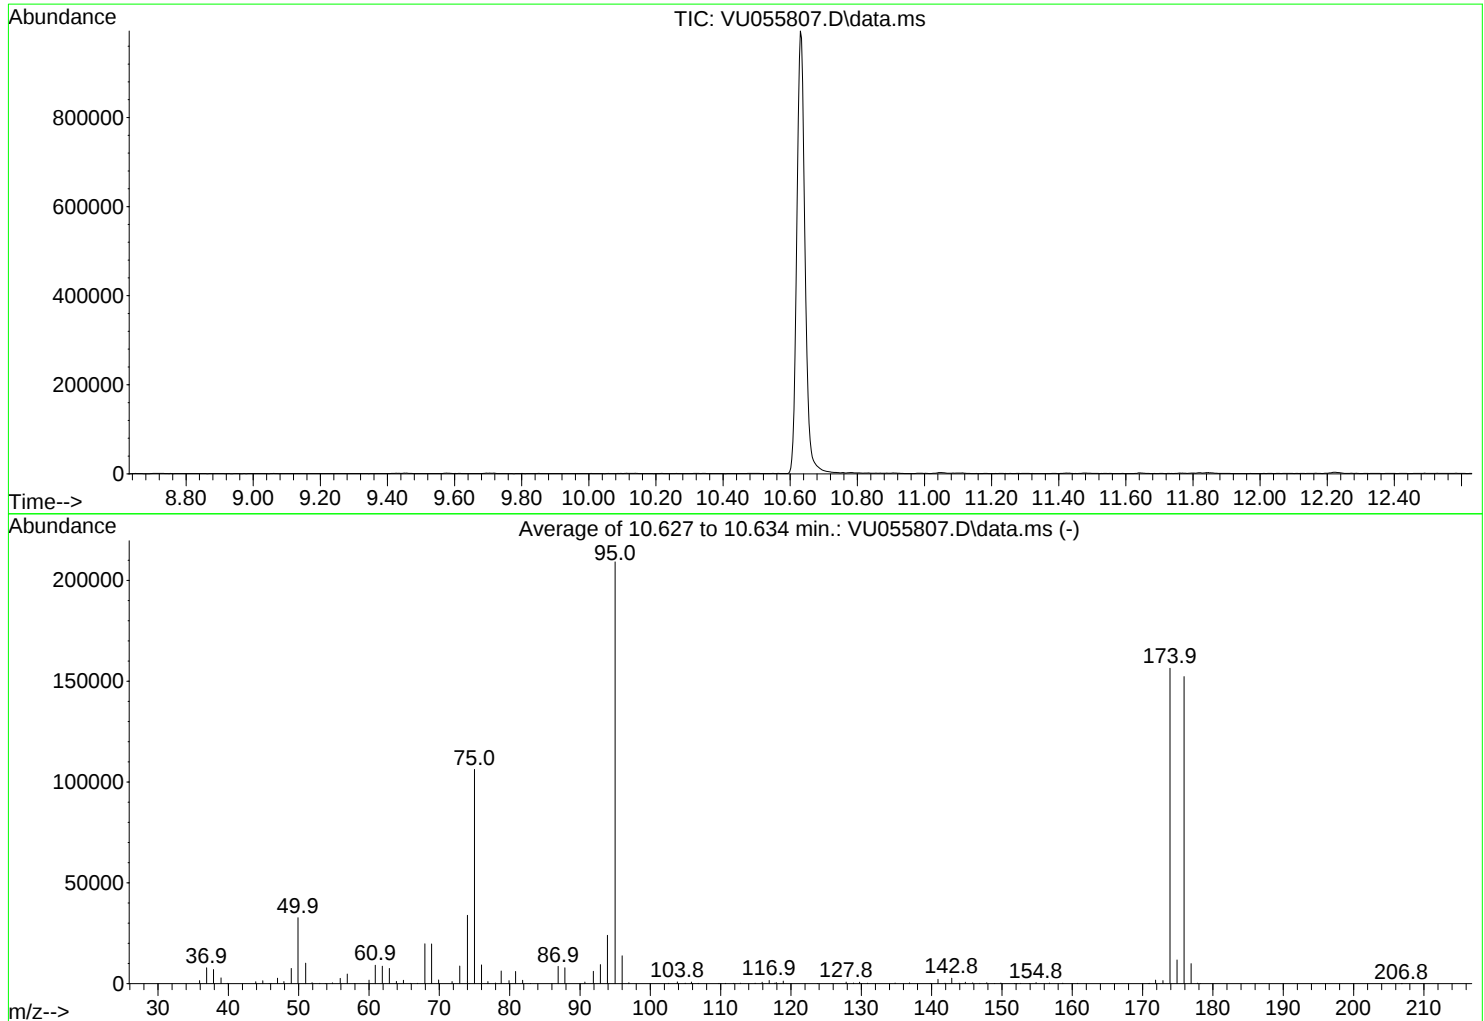

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	32669	PASS
75	95	30	60	50.8	106240	PASS
95	95	100	100	100.0	209195	PASS
96	95	5	9	6.6	13846	PASS
173	174	0.00	2	0.9	1483	PASS
174	95	50	100	74.8	156395	PASS
175	174	5	9	7.5	11791	PASS
176	174	95	101	97.4	152299	PASS
177	176	5	9	6.5	9928	PASS